
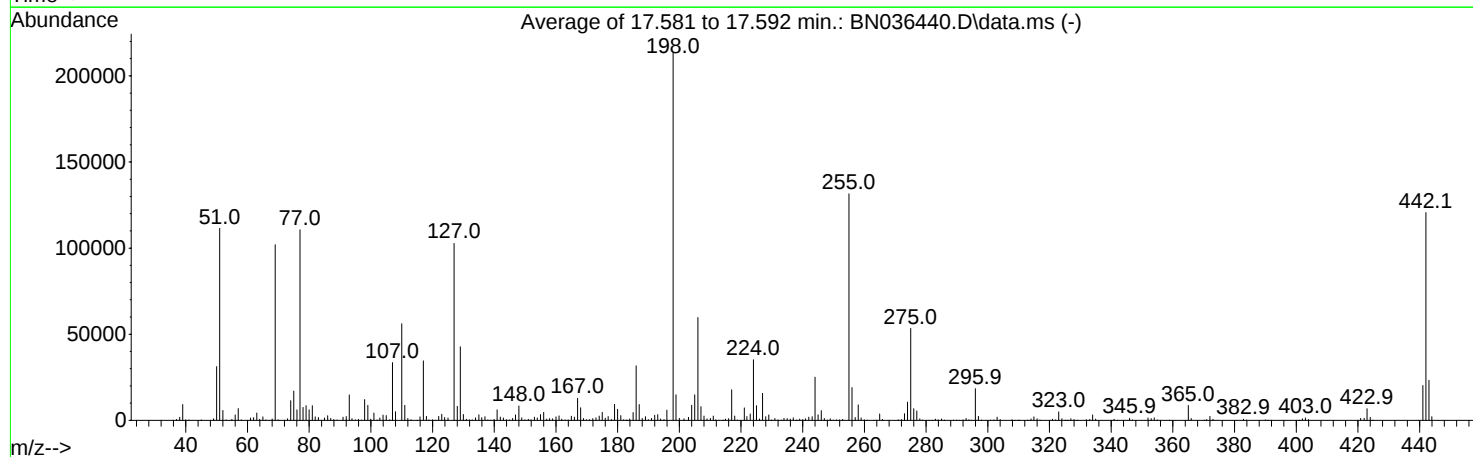


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036440.D
Acq On : 12 Feb 2025 15:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 11 01:17:14 2025

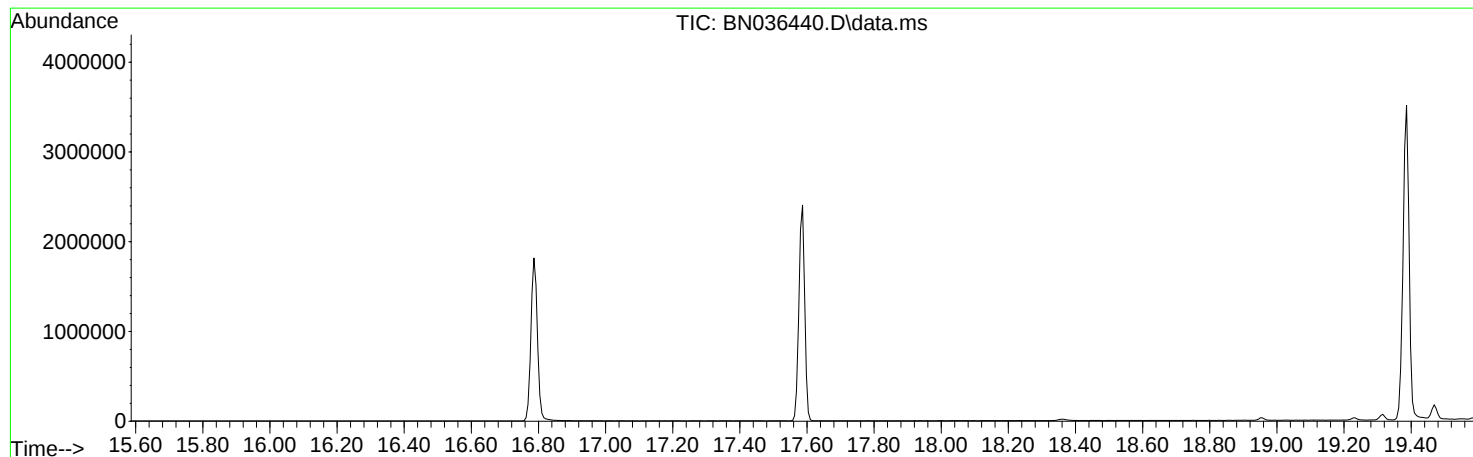

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.2	111435	PASS
68	69	0.00	2	0.9	873	PASS
69	198	0.00	100	47.7	101952	PASS
70	69	0.00	2	0.4	407	PASS
127	198	10	80	48.1	102789	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	213568	PASS
199	198	5	9	7.0	14856	PASS
275	198	10	60	25.0	53379	PASS
365	198	1	100	4.0	8641	PASS
441	198	0.01	100	9.5	20264	PASS
442	442	50	100	100.0	120632	PASS
443	442	15	24	19.2	23216	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/12/2025	BNA_N	<u>BN036440.D</u>
Compound Name	Response	Retention Time
DDT	836564	20.622
DDD	8606	20.233
DDE	0	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8606	845170	1.02

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036440.D
Acq On : 12 Feb 2025 15:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 12 17:06:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

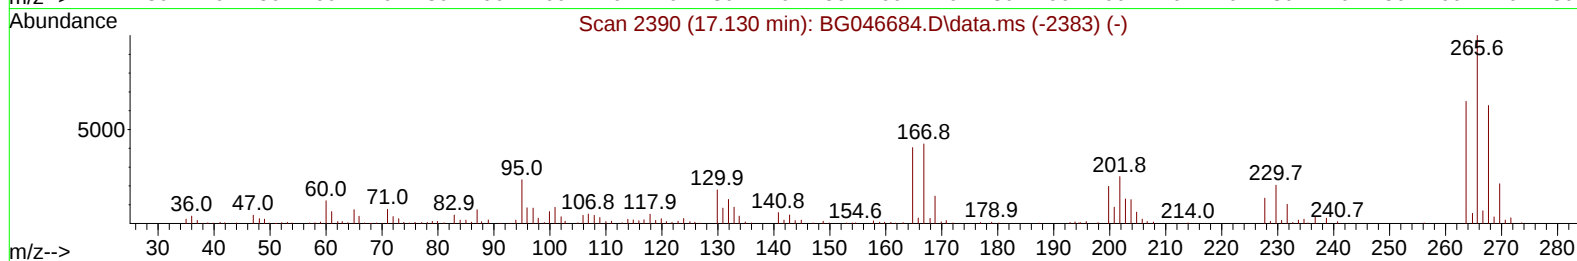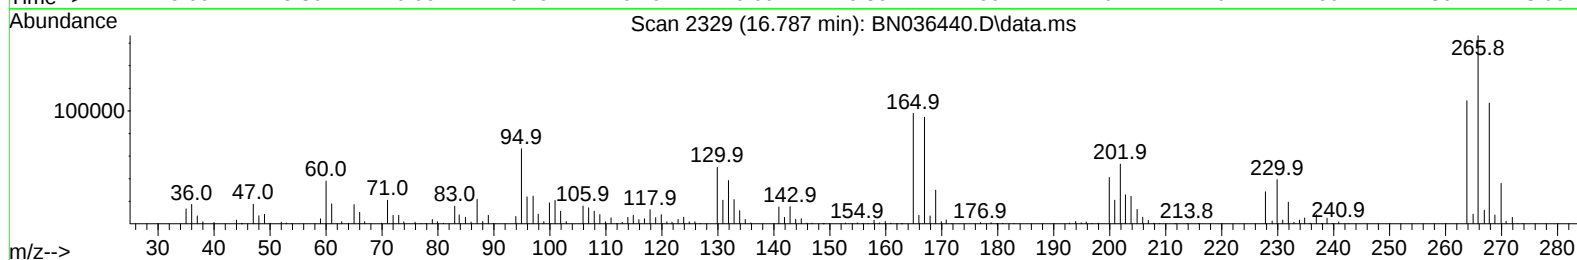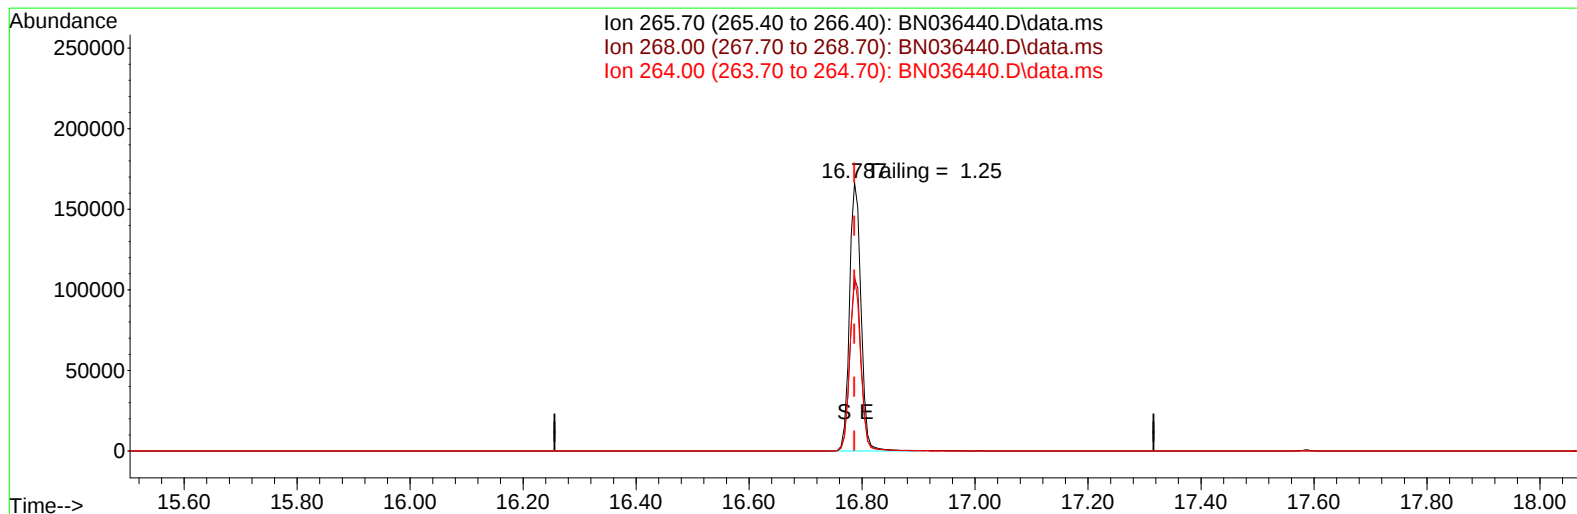

TIC: BN036440.D\data.ms

(70) Pentachlorophenol (C)

16.787min (+ 0.001) 20072.93 ng

response 236291

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.22
264.00	61.60	65.47
0.00	0.00	0.00

