


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021125\
Data File : BF141550.D
Acq On : 11 Feb 2025 10:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

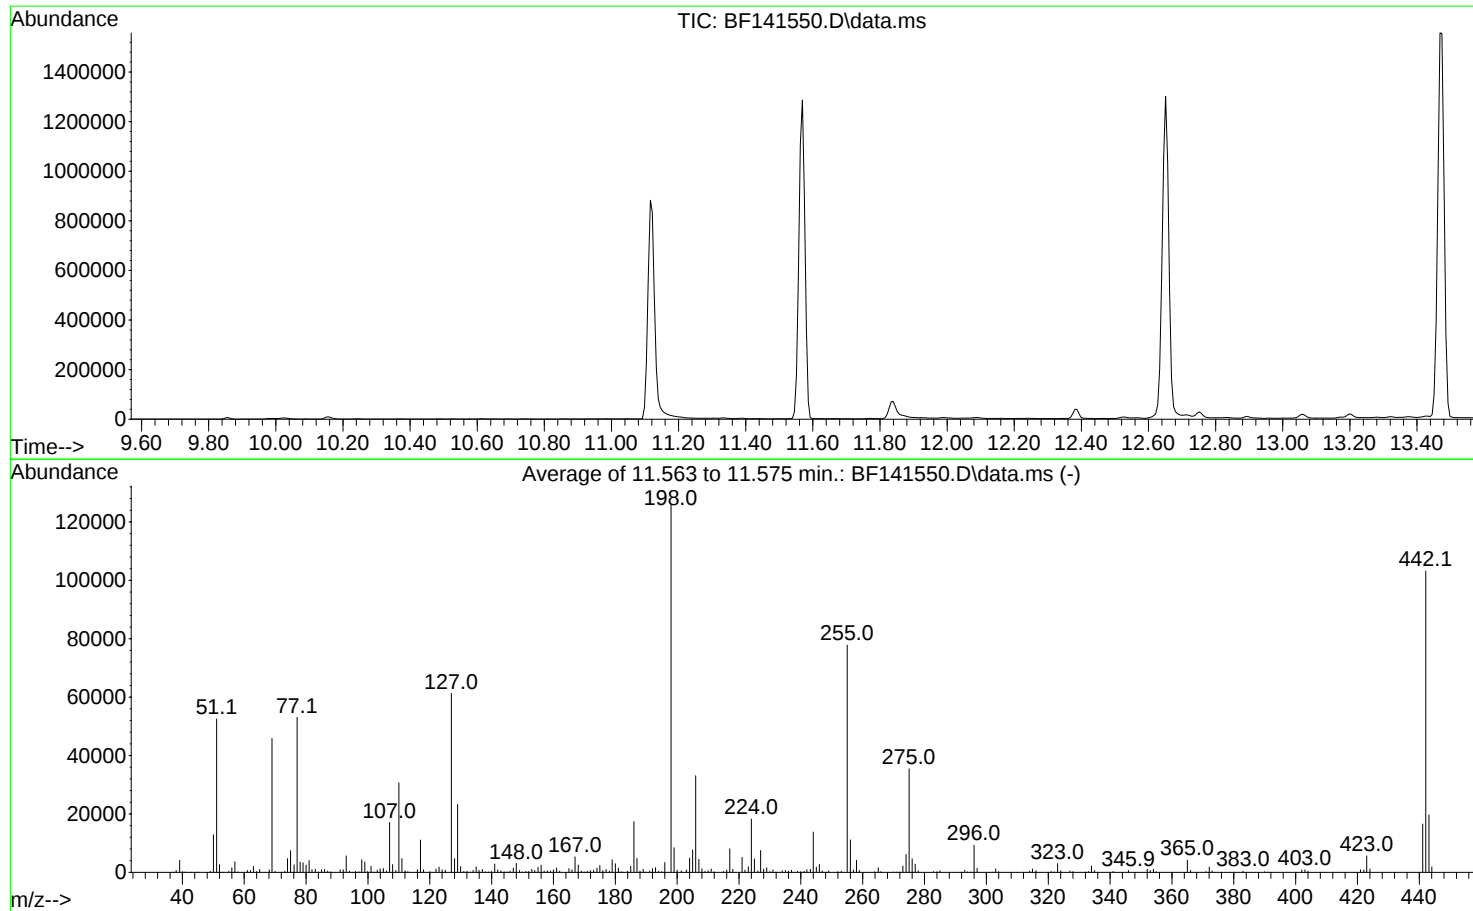

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	52576	PASS
68	69	0.00	2	1.9	880	PASS
69	198	0.00	100	36.4	45864	PASS
70	69	0.00	2	0.7	312	PASS
127	198	10	80	48.6	61283	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125976	PASS
199	198	5	9	6.7	8465	PASS
275	198	10	60	28.2	35464	PASS
365	198	1	100	3.3	4164	PASS
441	198	0.01	100	13.1	16543	PASS
442	442	50	100	100.0	103163	PASS
443	442	15	24	19.1	19671	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/11/2025	BNA_F	<u>BF141550.D</u>
Compound Name	Response	Retention Time
DDT	411059	13.474
DDD	6230	13.204
DDE	573	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6803	417862	1.63

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021125\
Data File : BF141550.D
Acq On : 11 Feb 2025 10:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 11 10:57:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

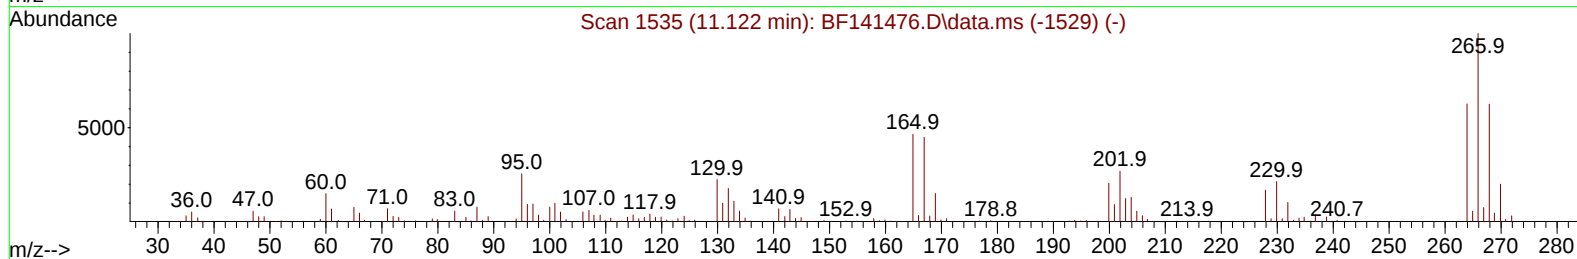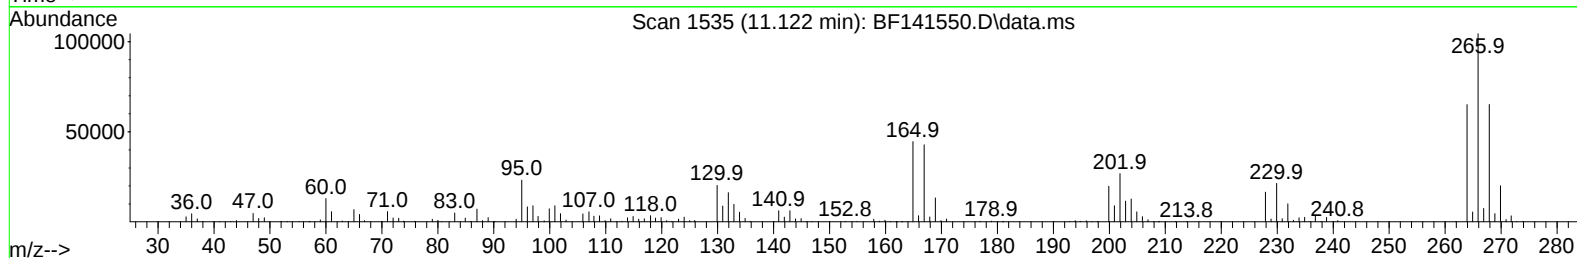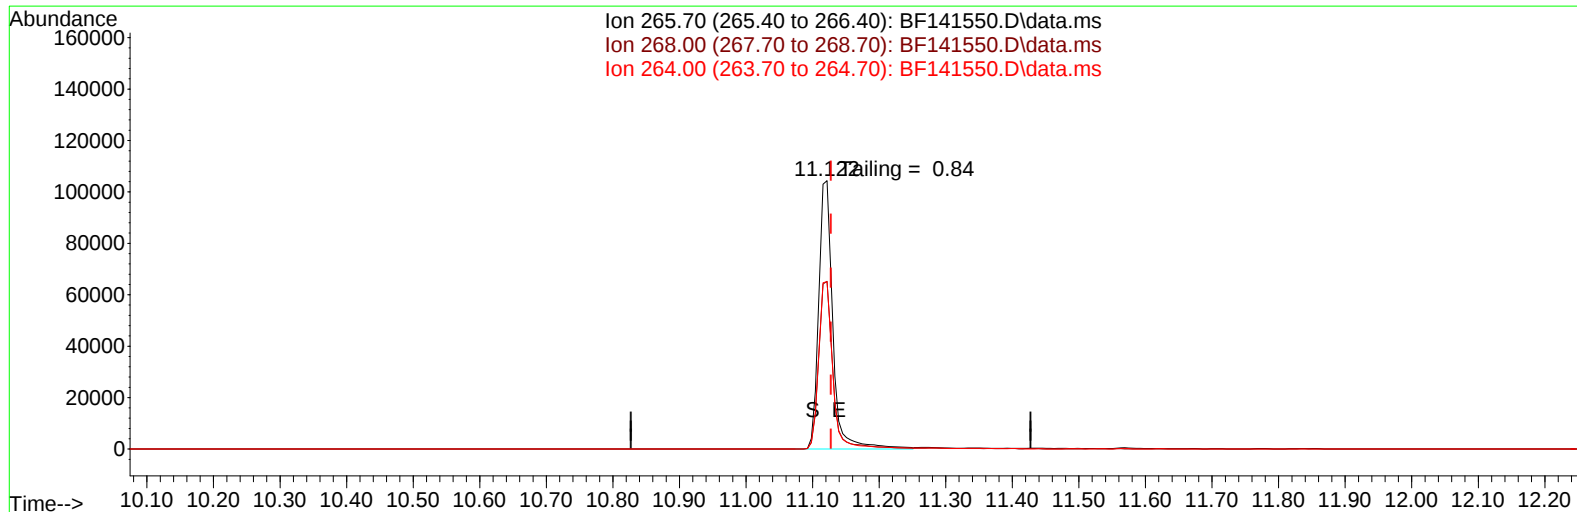

TIC: BF141550.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 16244.81 ng




response 154688

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.47
264.00	62.60	62.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021125\
Data File : BF141550.D
Acq On : 11 Feb 2025 10:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 11 10:57:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

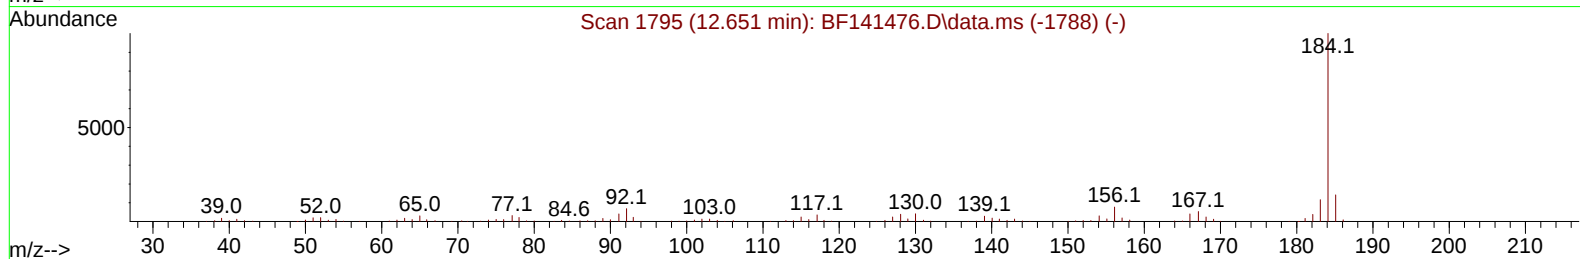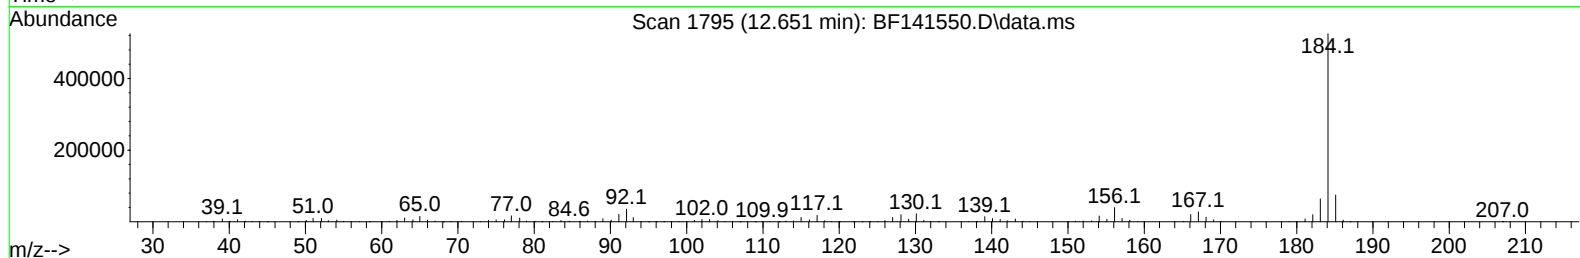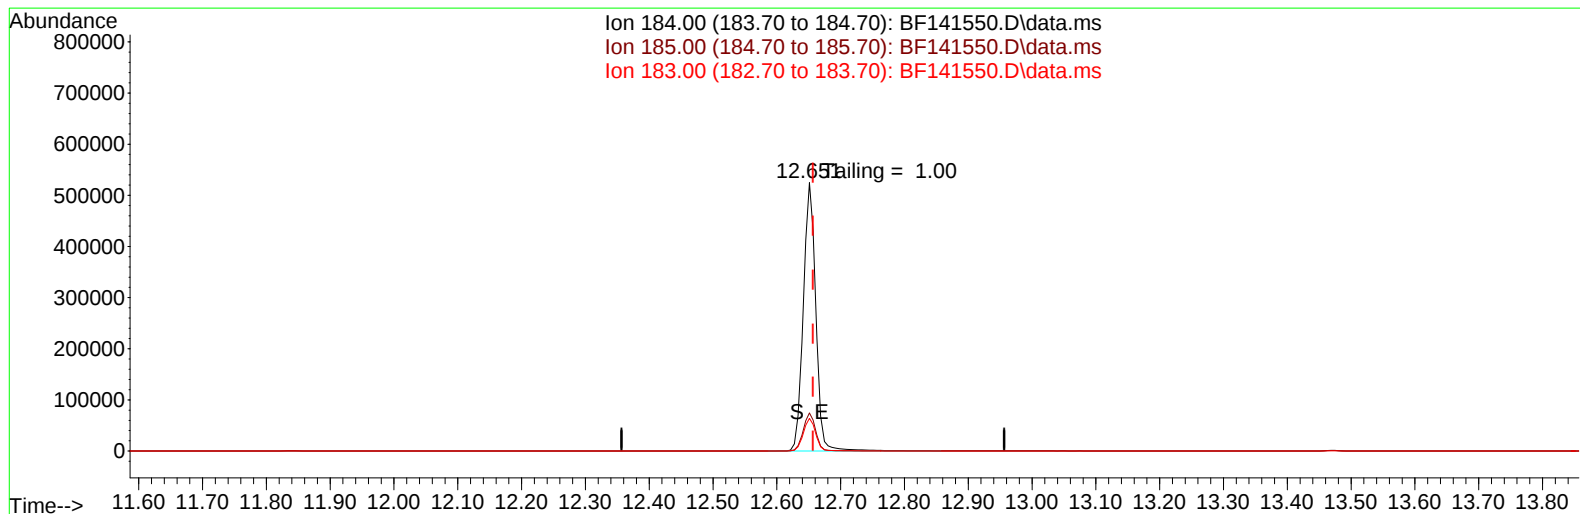

TIC: BF141550.D\data.ms

(77) Benzidine

12.651min (-0.006) 26925.30 ng

response 718522

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.23
183.00	11.60	12.19
0.00	0.00	0.00