
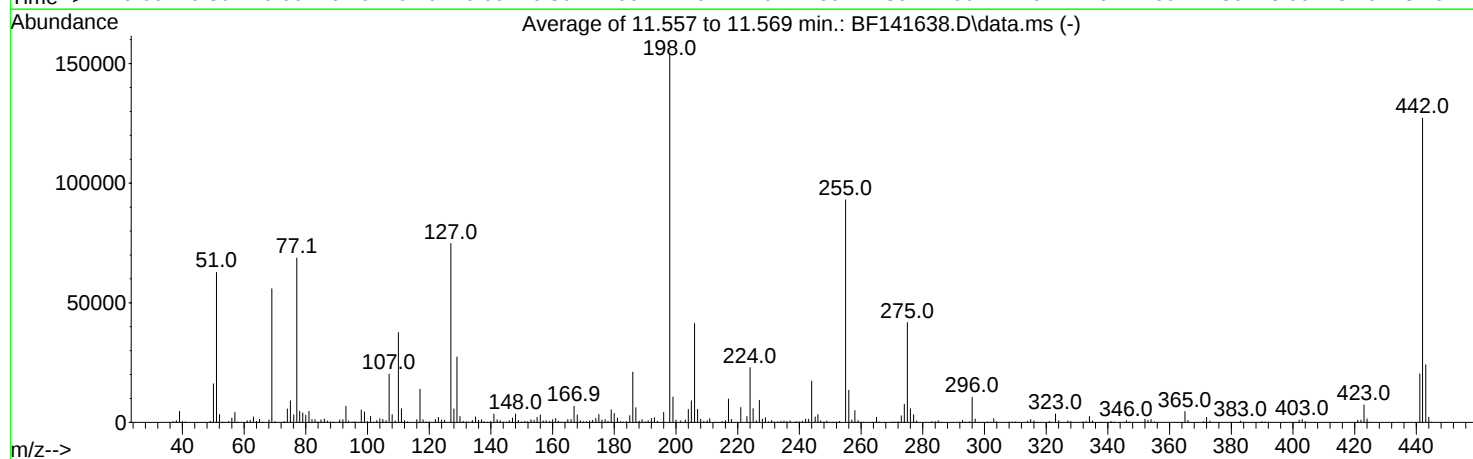


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141638.D
Acq On : 14 Feb 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

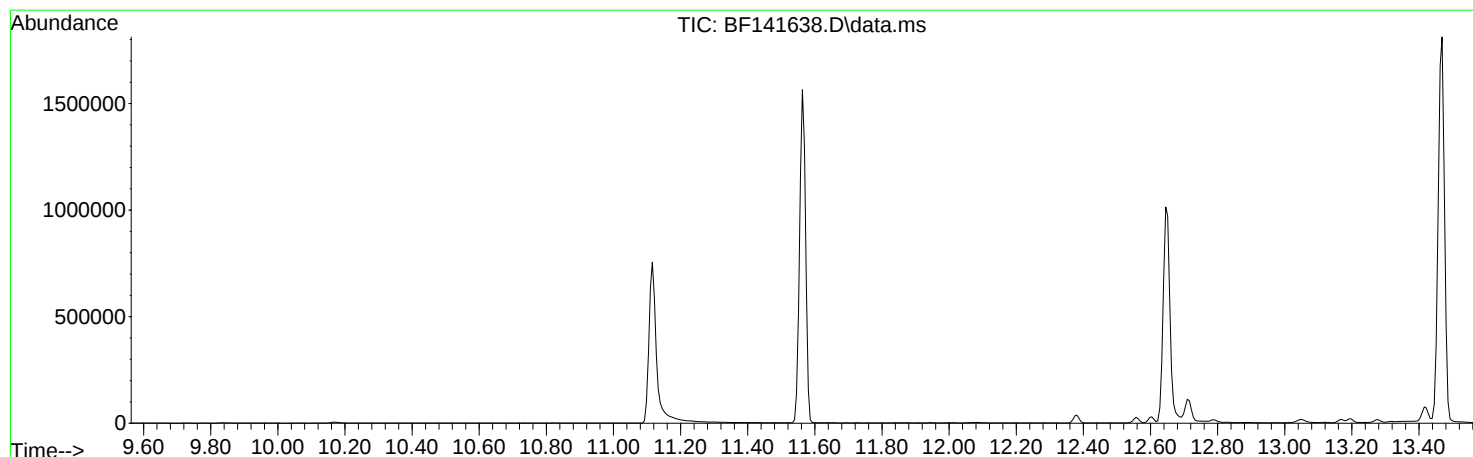

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	62680	PASS
68	69	0.00	2	1.8	1020	PASS
69	198	0.00	100	36.3	55875	PASS
70	69	0.00	2	0.5	301	PASS
127	198	10	80	48.6	74800	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153792	PASS
199	198	5	9	6.9	10562	PASS
275	198	10	60	27.2	41765	PASS
365	198	1	100	3.0	4538	PASS
441	198	0.01	100	13.2	20278	PASS
442	442	50	100	100.0	127181	PASS
443	442	15	24	18.9	24067	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/14/2025	BNA_F	<u>BF141638.D</u>
Compound Name	Response	Retention Time
DDT	469880	13.469
DDD	12079	13.169
DDE	518	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12597	482477	2.61

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141638.D
Acq On : 14 Feb 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 14 15:24:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

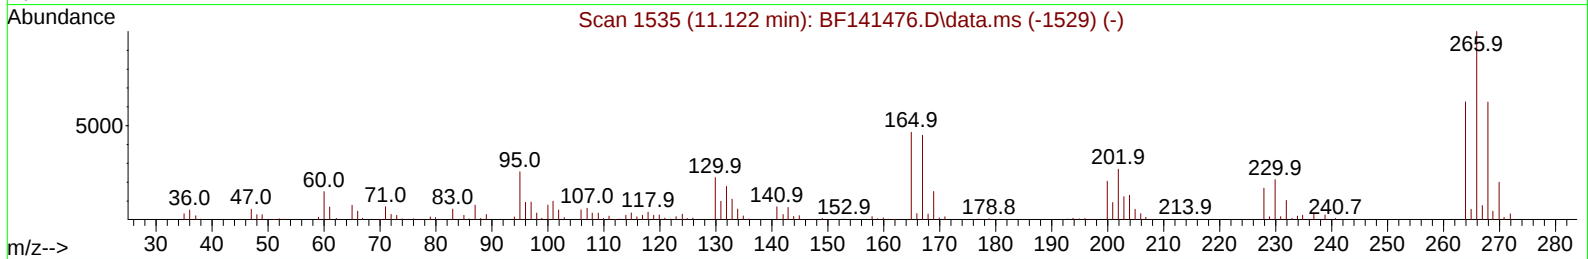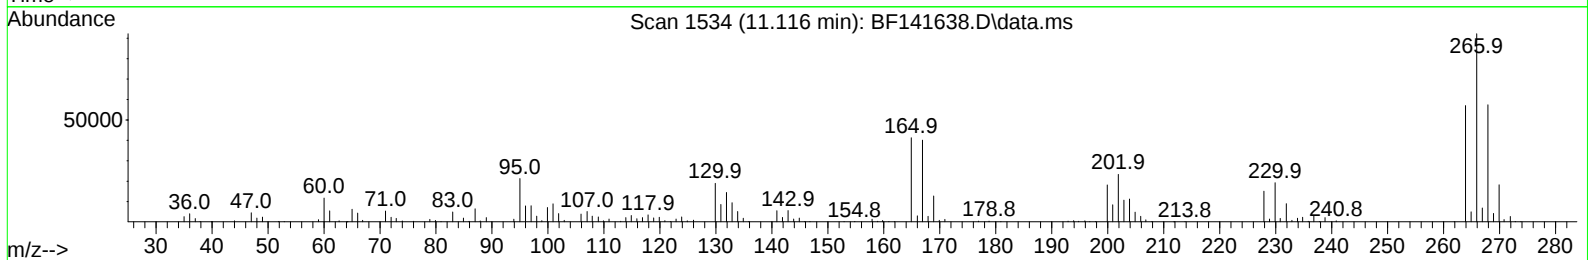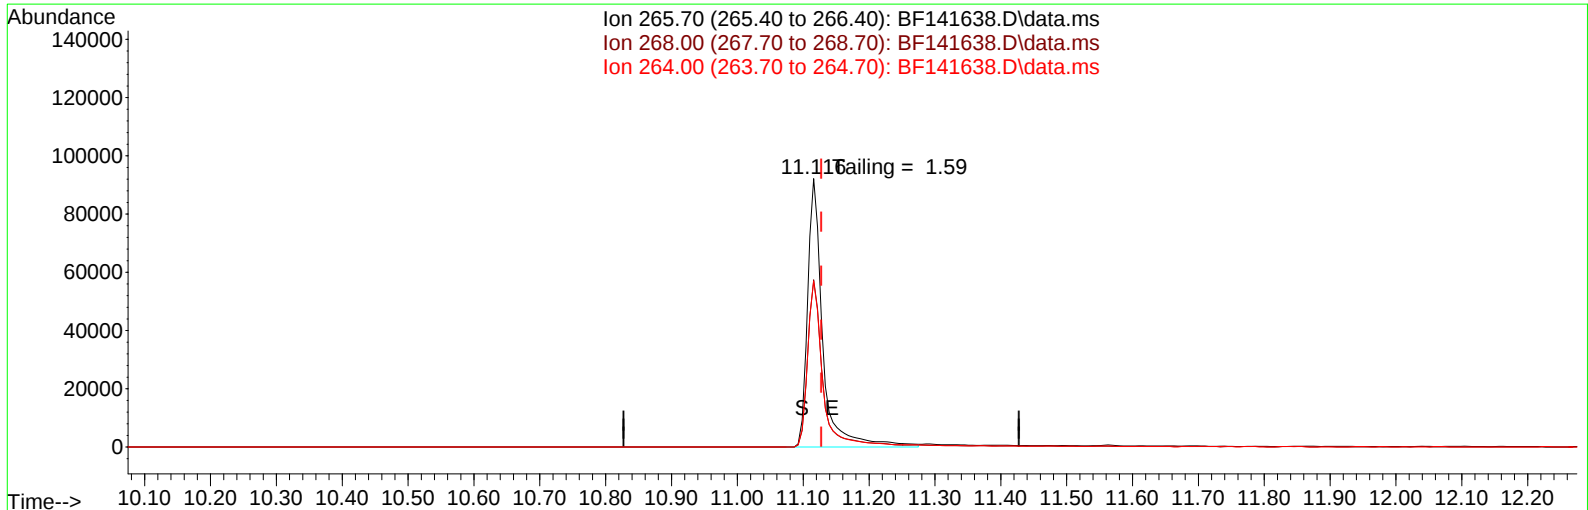

TIC: BF141638.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.011) 158475.01 ng




response 149272

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.28
264.00	62.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141638.D
Acq On : 14 Feb 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 14 15:24:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

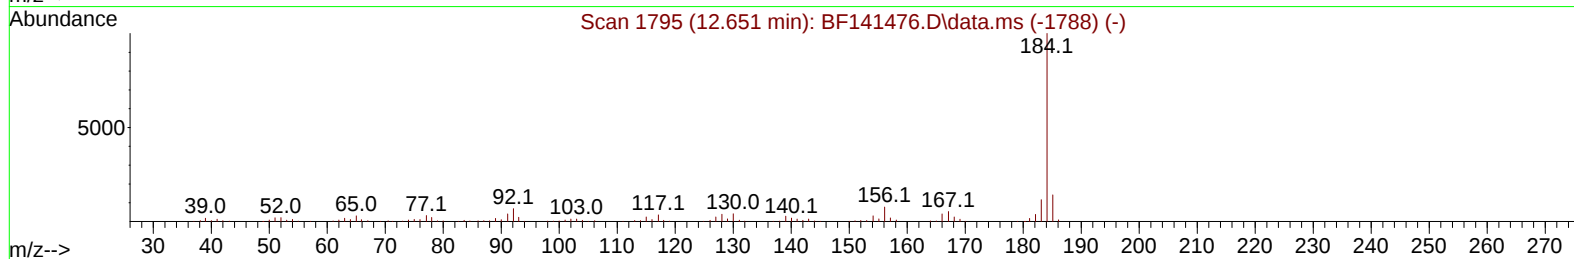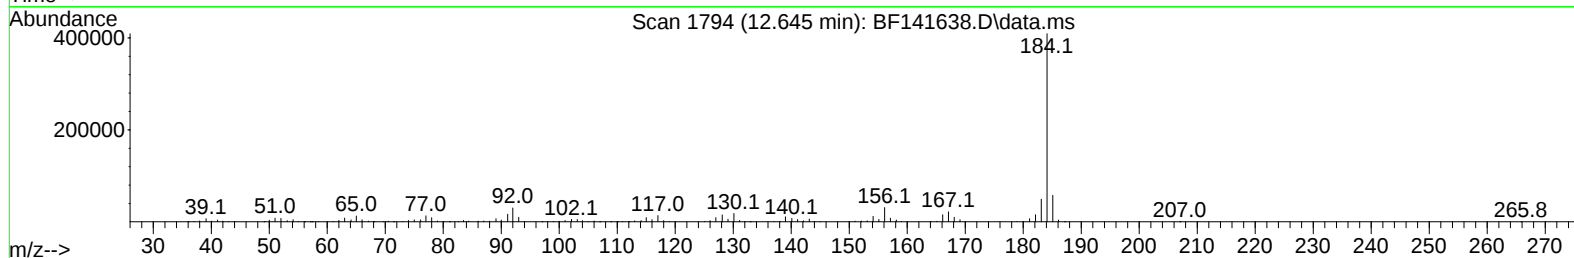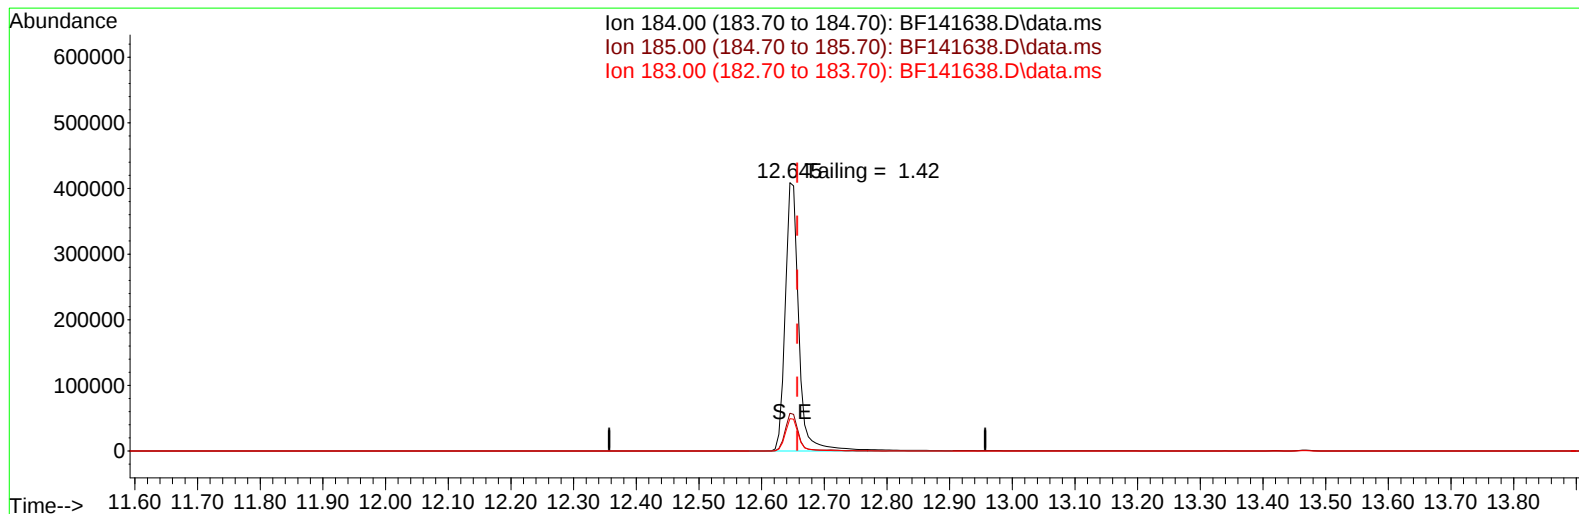

TIC: BF141638.D\data.ms

(77) Benzidine

12.645min (-0.011) 0.00 ng

response 621132

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.06
183.00	11.60	12.06
0.00	0.00	0.00