
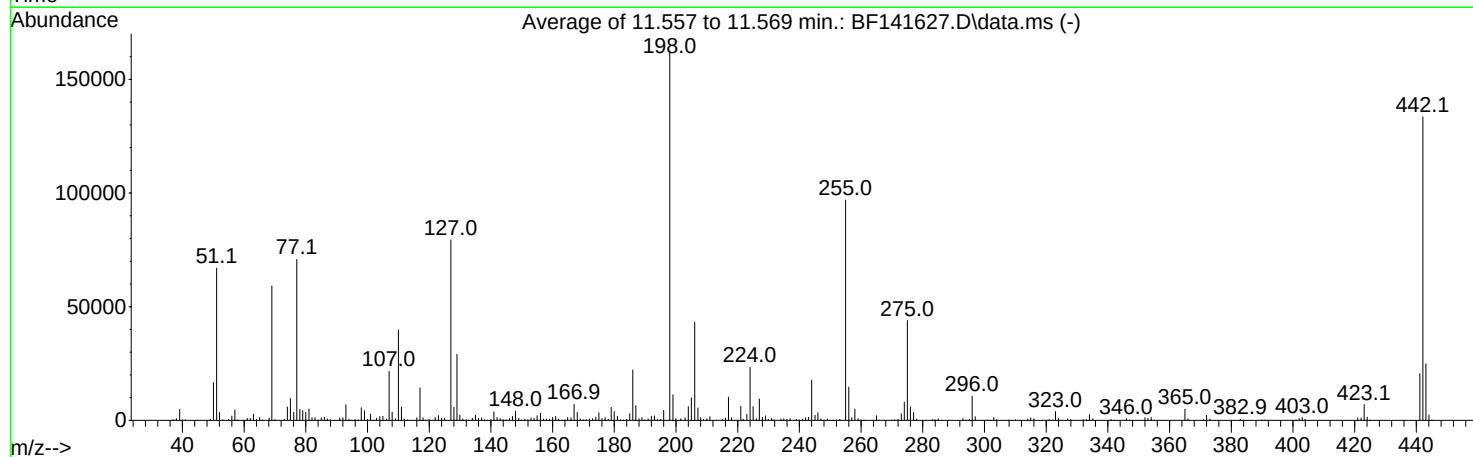


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141627.D
Acq On : 14 Feb 2025 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

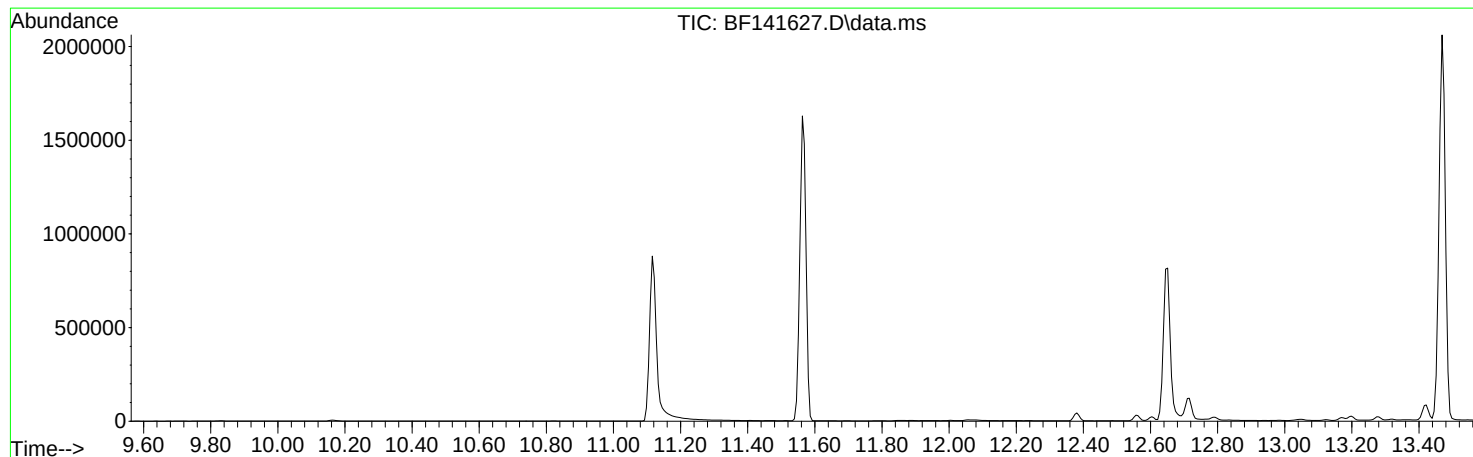

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	41.3	66885	PASS
68	69	0.00	2	1.8	1044	PASS
69	198	0.00	100	36.6	59152	PASS
70	69	0.00	2	0.5	324	PASS
127	198	10	80	49.1	79389	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	161827	PASS
199	198	5	9	6.9	11232	PASS
275	198	10	60	27.2	43941	PASS
365	198	1	100	3.0	4916	PASS
441	198	0.01	100	12.7	20590	PASS
442	442	50	100	100.0	133499	PASS
443	442	15	24	18.6	24881	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/14/2025	BNA_F	<u>BF141627.D</u>
Compound Name	Response	Retention Time
DDT	532922	13.469
DDD	11412	13.198
DDE	640	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12052	544974	2.21

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141627.D
Acq On : 14 Feb 2025 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 14 10:34:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

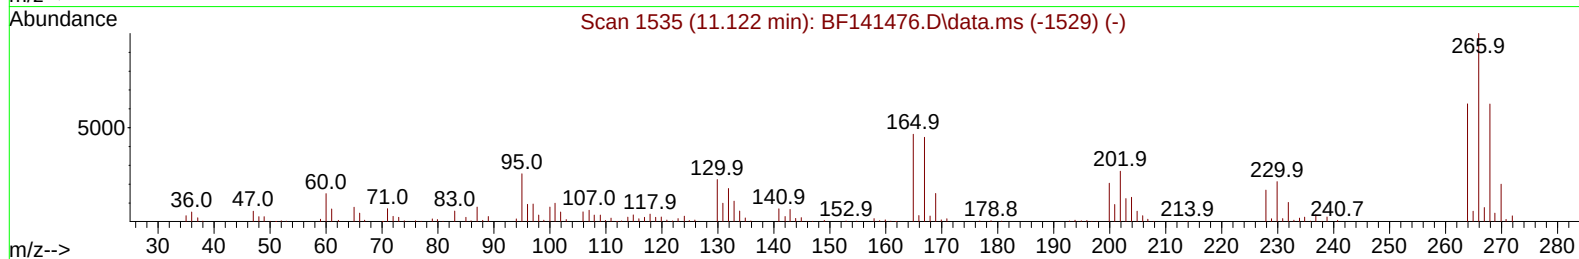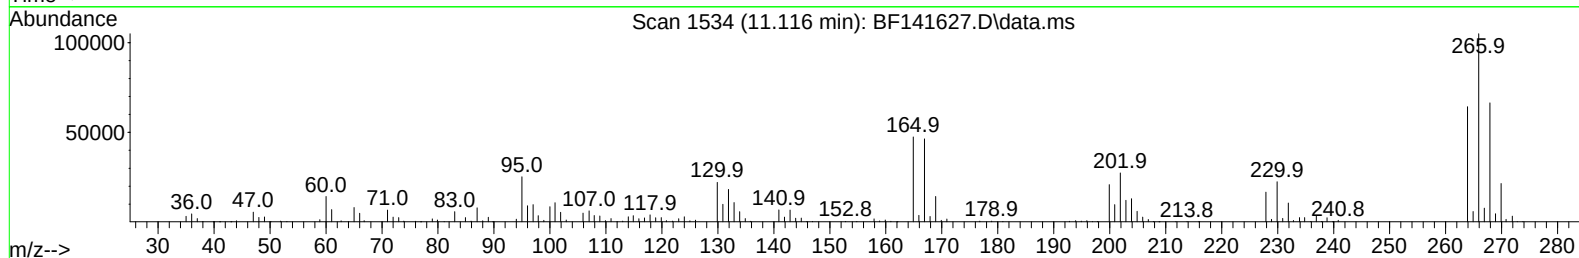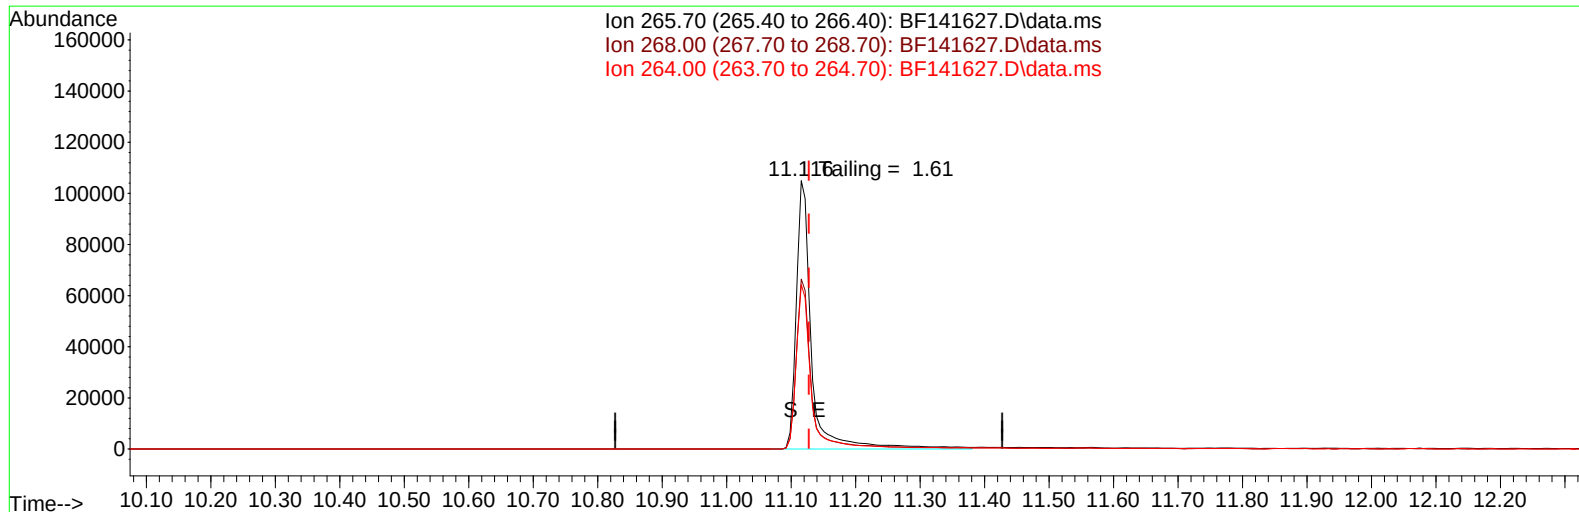

TIC: BF141627.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.012) 23053.12 ng




response 171340

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.29
264.00	62.60	61.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141627.D
Acq On : 14 Feb 2025 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 14 10:34:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

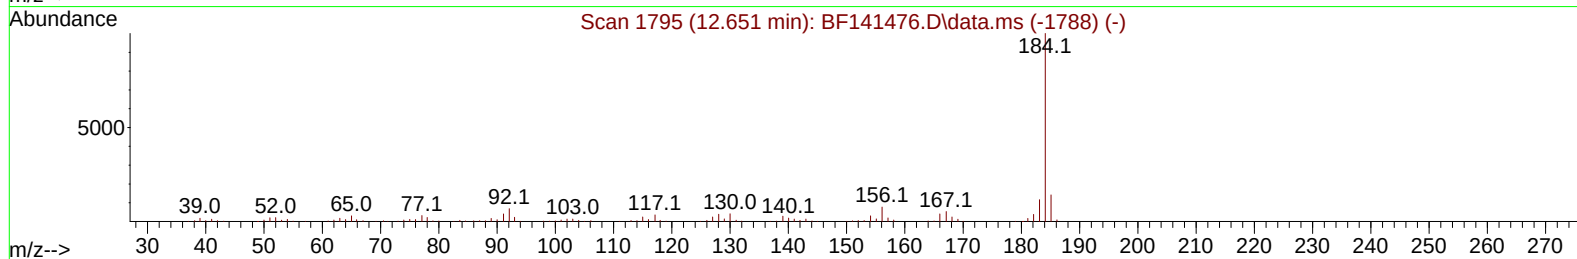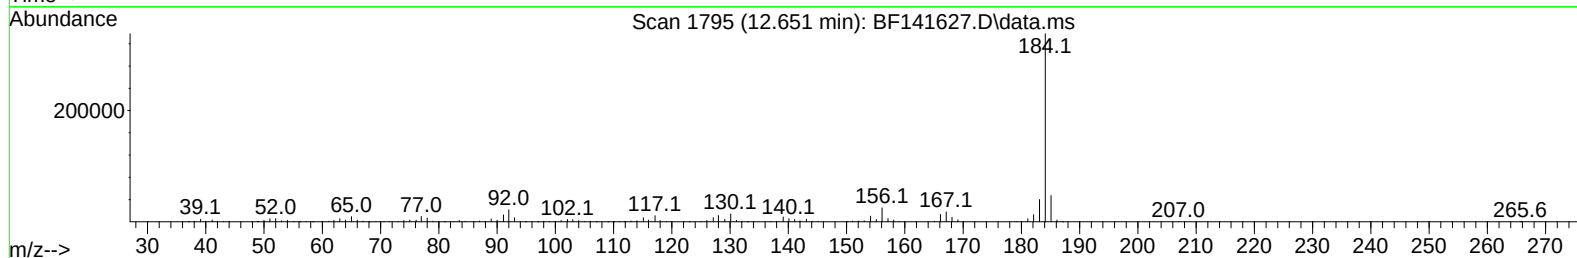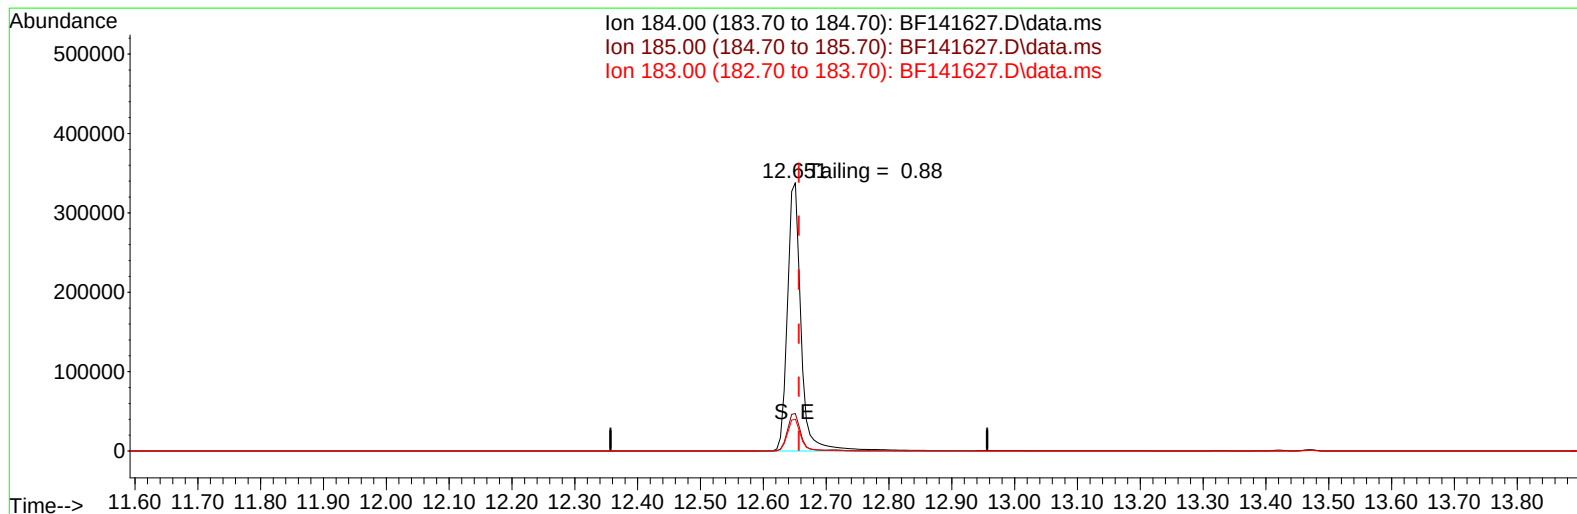

TIC: BF141627.D\data.ms

(77) Benzidine

12.651min (-0.006) 0.00 ng

response 512547

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.99
183.00	11.60	11.86
0.00	0.00	0.00