

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021425\
 Data File : VX044967.D
 Acq On : 14 Feb 2025 17:25
 Operator : JC/MD
 Sample : Q1363-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VFCC-2-021225

Quant Time: Feb 14 22:17:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 11 03:41:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	78469	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	163329	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	153346	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	68646	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	66539	57.928	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 115.860%	
35) Dibromofluoromethane	5.379	113	55153	51.938	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.880%	
50) Toluene-d8	8.647	98	205791	51.249	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.500%	
62) 4-Bromofluorobenzene	11.079	95	73777	54.500	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 109.000%	
Target Compounds						
					Qvalue	
9) 1,1,2-Trichlorotrifluo...	2.331	101	772	0.779	ug/l	96
12) 1,1-Dichloroethene	2.325	96	386	0.382	ug/l #	79
16) Acetone	2.380	43	943	2.042	ug/l	96
27) cis-1,2-Dichloroethene	4.489	96	3763	3.147	ug/l	94
30) Chloroform	5.093	83	977	0.521	ug/l	98
44) Trichloroethene	7.129	130	4393	4.017	ug/l	100
64) Tetrachloroethene	9.269	164	523	0.541	ug/l #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021425\
Data File : VX044967.D
Acq On : 14 Feb 2025 17:25
Operator : JC/MD
Sample : Q1363-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VFCC-2-021225

Quant Time: Feb 14 22:17:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 11 03:41:08 2025
Response via : Initial Calibration




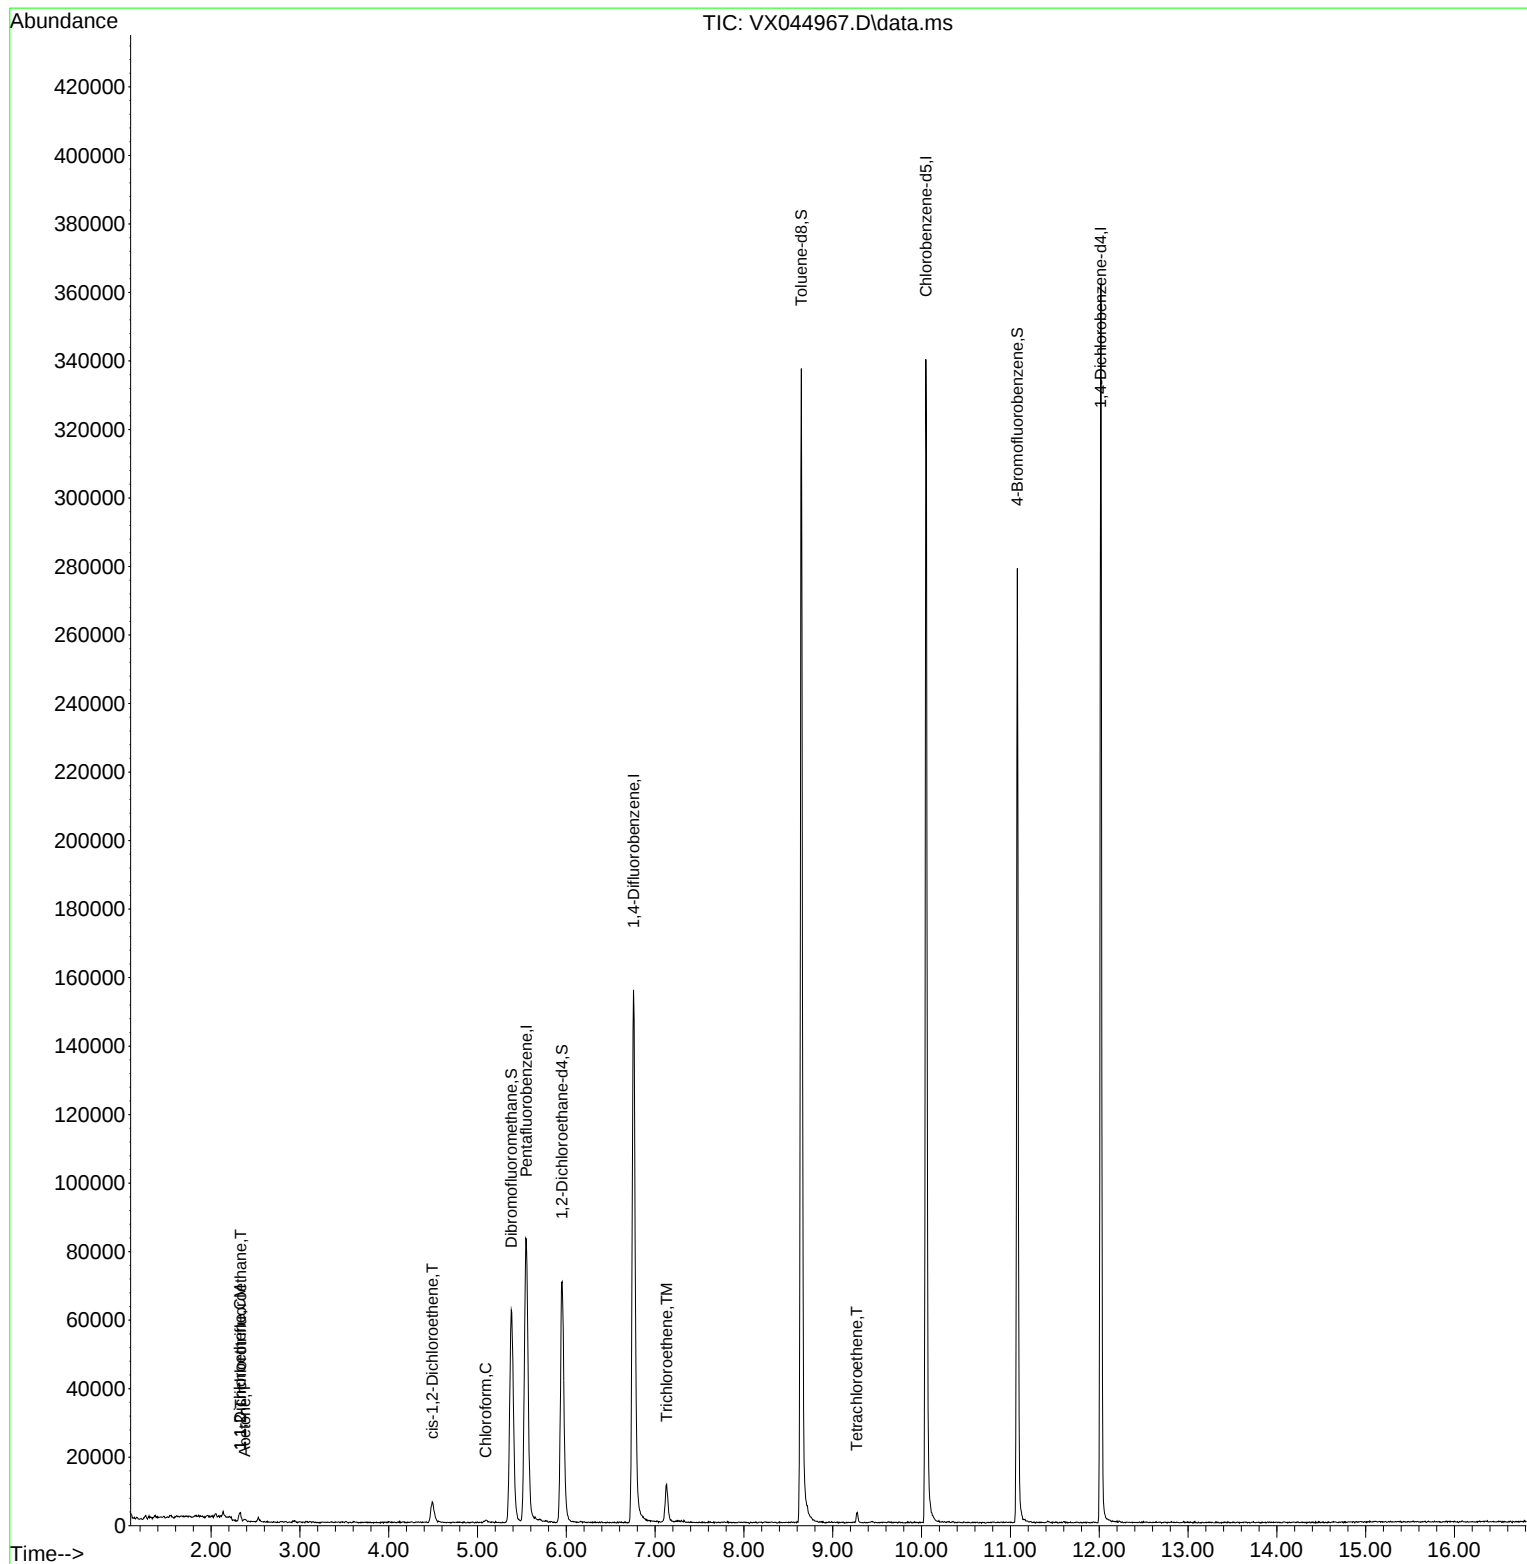


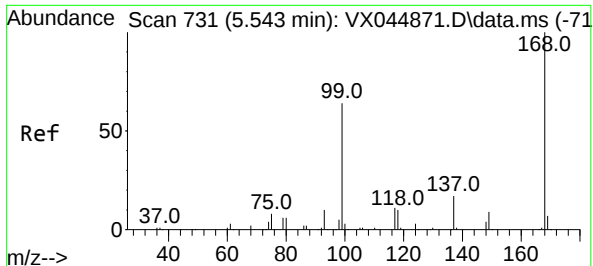

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX044967.D
Acq: 14 Feb 2025 17:25




Instrument :
MSVOA_X
ClientSampleId :
VFCC-2-021225


Tgt Ion:168 Resp: 78469
Ion Ratio Lower Upper
168 100
99 65.9 51.2 76.8

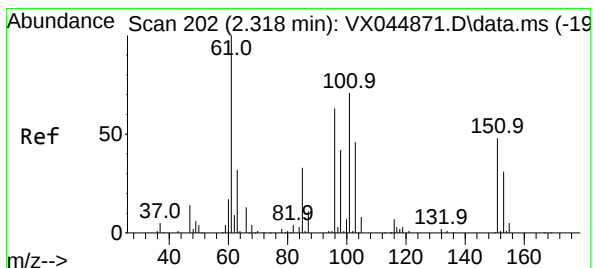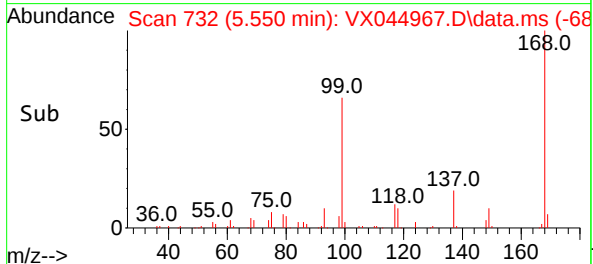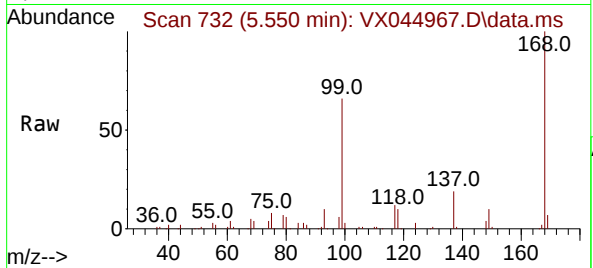

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.779 ug/l
RT: 2.331 min Scan# 204
Delta R.T. 0.013 min
Lab File: VX044967.D
Acq: 14 Feb 2025 17:25

Tgt Ion:101 Resp: 772
Ion Ratio Lower Upper
101 100
85 42.7 35.7 53.5
151 66.6 56.0 84.0

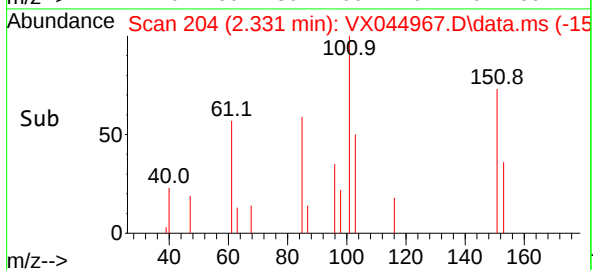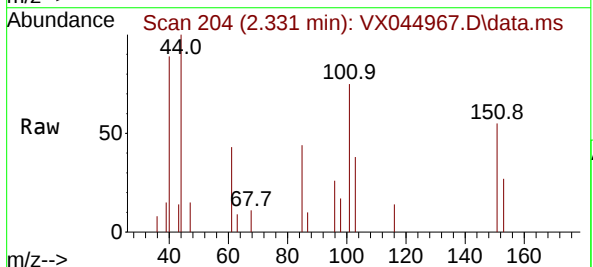

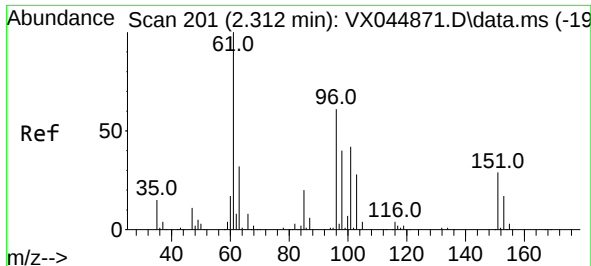

#12

1,1-Dichloroethene

Concen: 0.382 ug/l

RT: 2.325 min Scan# 201

Delta R.T. 0.013 min

Lab File: VX044967.D

Acq: 14 Feb 2025 17:25

Instrument :

MSVOA_X

ClientSampleId :

VFCC-2-021225





Tgt Ion: 96 Resp: 386

Ion Ratio Lower Upper

96 100

61 128.6 130.2 195.4#

98 71.4 52.2 78.4

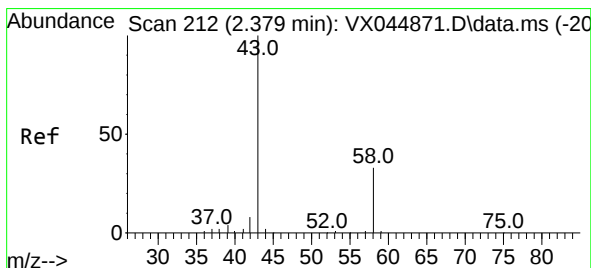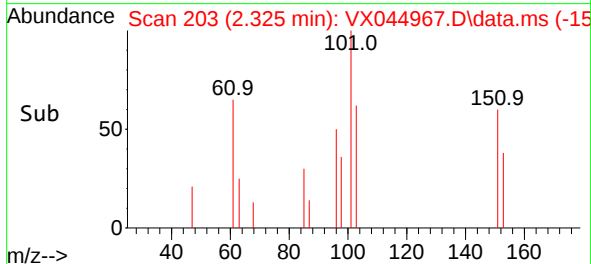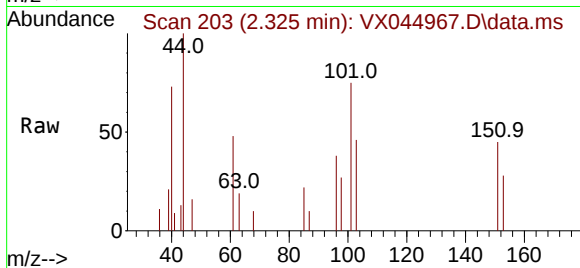

#16

Acetone

Concen: 2.042 ug/l

RT: 2.380 min Scan# 212

Delta R.T. 0.000 min

Lab File: VX044967.D




Acq: 14 Feb 2025 17:25


Tgt Ion: 43 Resp: 943

Ion Ratio Lower Upper

43 100

58 35.2 26.5 39.7

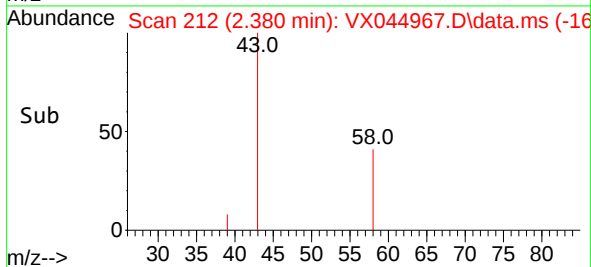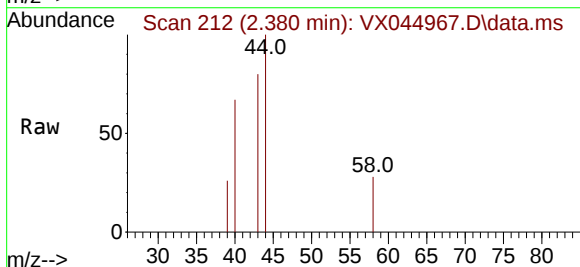

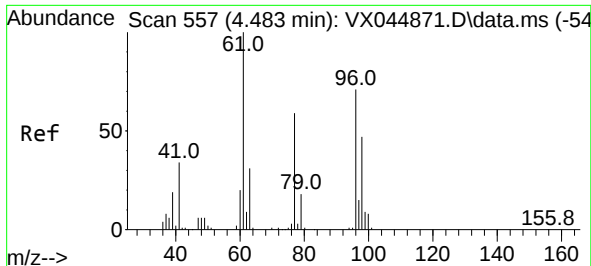

#27

cis-1,2-Dichloroethene

Concen: 3.147 ug/l

RT: 4.489 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX044967.D

Acq: 14 Feb 2025 17:25

Instrument :

MSVOA_X

ClientSampleId :

VFCC-2-021225





Tgt Ion: 96 Resp: 3763

Ion Ratio Lower Upper

96 100

61 136.2 0.0 294.0

98 66.2 0.0 131.2

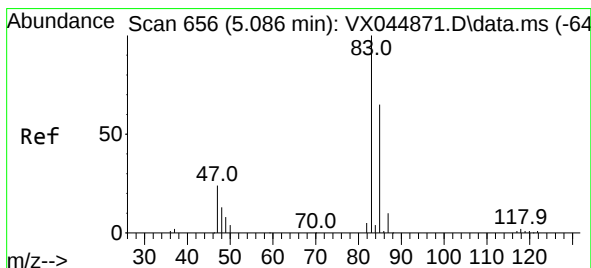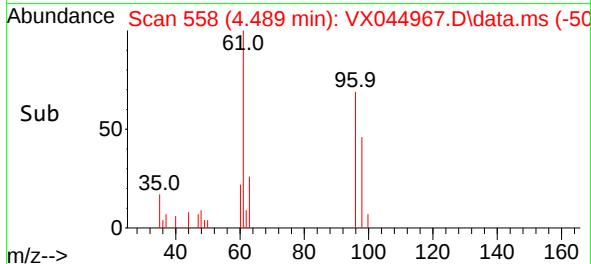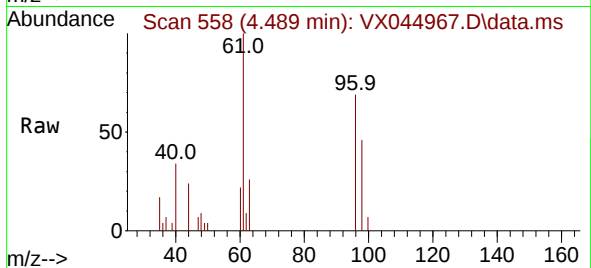

#30

Chloroform

Concen: 0.521 ug/l

RT: 5.093 min Scan# 657

Delta R.T. 0.006 min

Lab File: VX044967.D




Acq: 14 Feb 2025 17:25


Tgt Ion: 83 Resp: 977

Ion Ratio Lower Upper

83 100

85 66.5 52.1 78.1


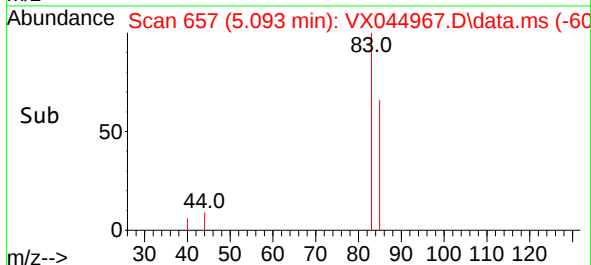

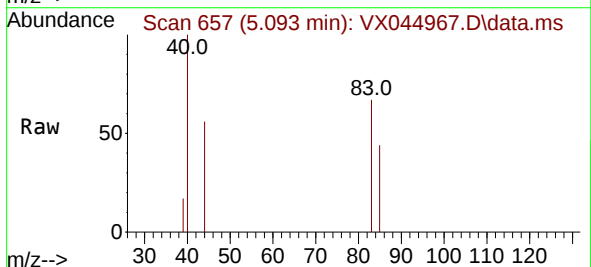


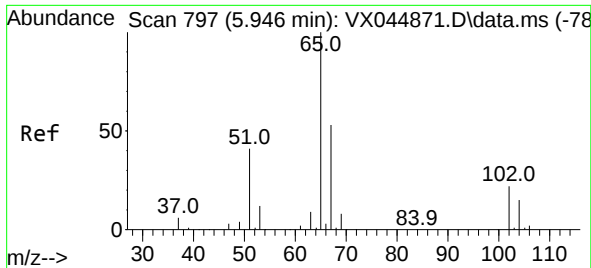

#33
 1,2-Dichloroethane-d4
 Concen: 57.928 ug/l
 RT: 5.952 min Scan# 797
 Delta R.T. 0.006 min
 Lab File: VX044967.D
 Acq: 14 Feb 2025 17:25




Instrument :
 MSVOA_X
 ClientSampleId :
 VFCC-2-021225


Tgt Ion: 65 Resp: 66539
 Ion Ratio Lower Upper
 65 100
 67 53.1 0.0 108.2

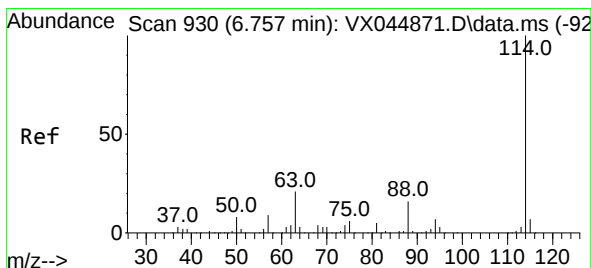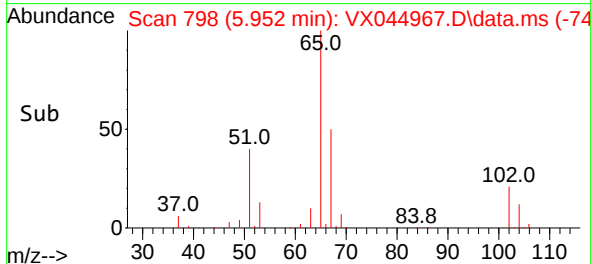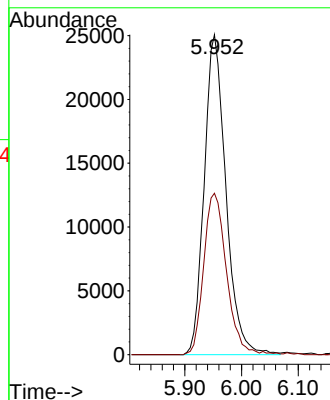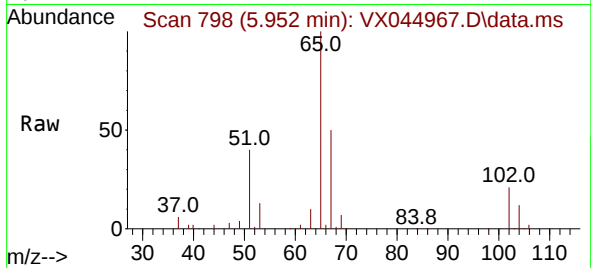

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. 0.000 min
 Lab File: VX044967.D
 Acq: 14 Feb 2025 17:25

Tgt Ion: 114 Resp: 163329
 Ion Ratio Lower Upper
 114 100
 63 21.6 0.0 42.4
 88 15.7 0.0 31.4

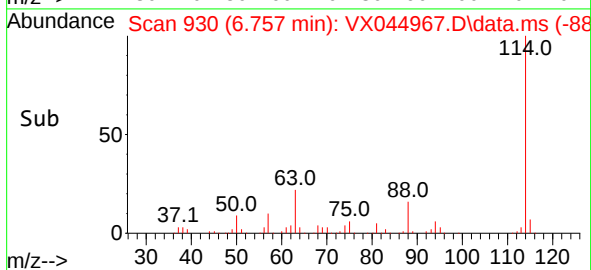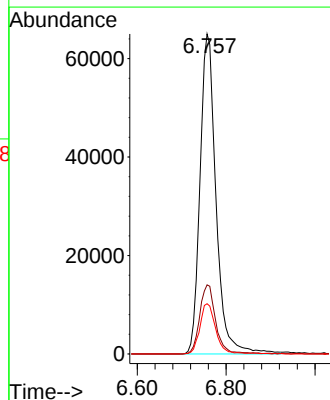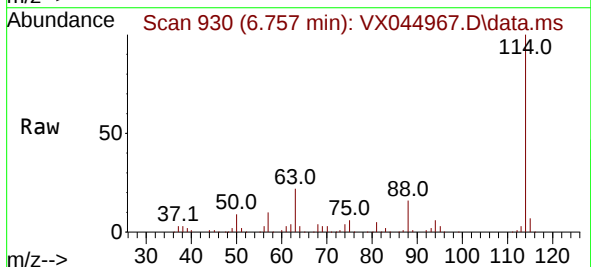

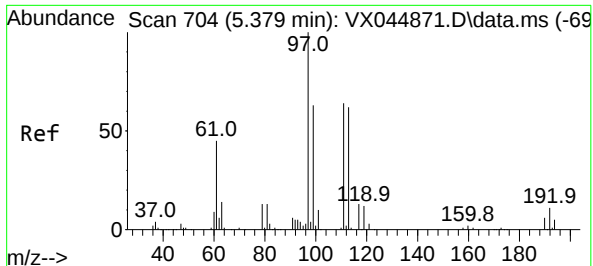

#35

Dibromofluoromethane

Concen: 51.938 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX044967.D

Acq: 14 Feb 2025 17:25

Instrument :

MSVOA_X

ClientSampleId :

VFCC-2-021225





Tgt Ion:113 Resp: 55153

Ion Ratio Lower Upper

113 100

111 103.3 83.5 125.3

192 17.6 14.4 21.6

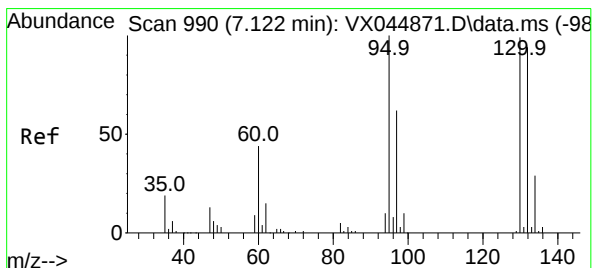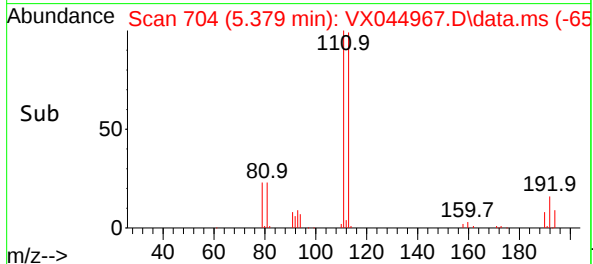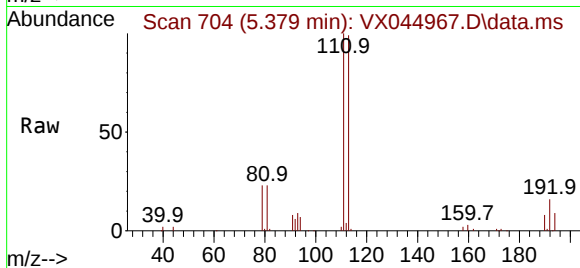

#44

Trichloroethene

Concen: 4.017 ug/l

RT: 7.129 min Scan# 991

Delta R.T. 0.006 min

Lab File: VX044967.D




Acq: 14 Feb 2025 17:25


Tgt Ion:130 Resp: 4393

Ion Ratio Lower Upper

130 100

95 100.8 0.0 202.4


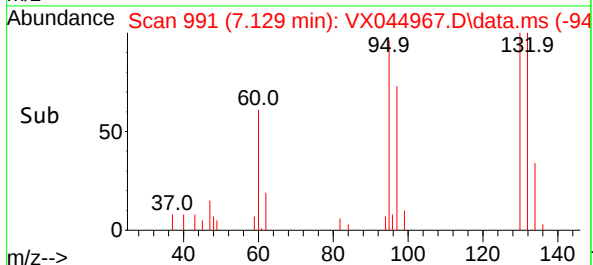

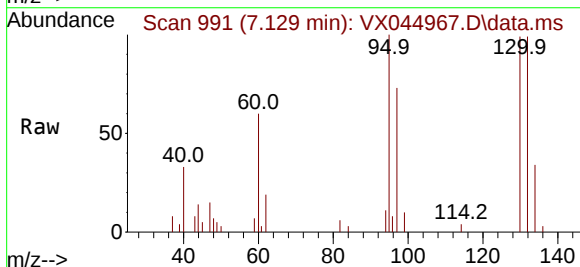


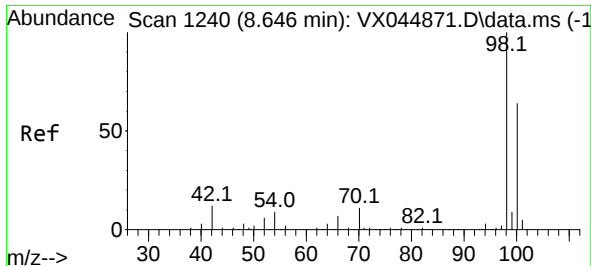

#50
Toluene-d8
Concen: 51.249 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX044967.D
Acq: 14 Feb 2025 17:25




Instrument :
MSVOA_X
ClientSampleId :
VFCC-2-021225


Tgt Ion: 98 Resp: 205791
Ion Ratio Lower Upper
98 100
100 65.3 52.7 79.1

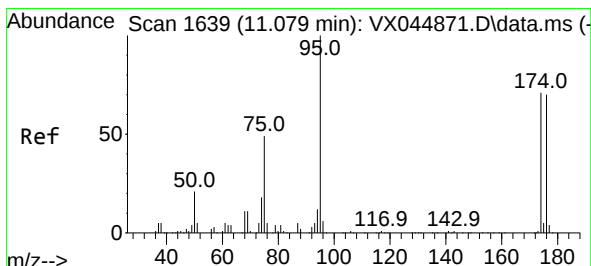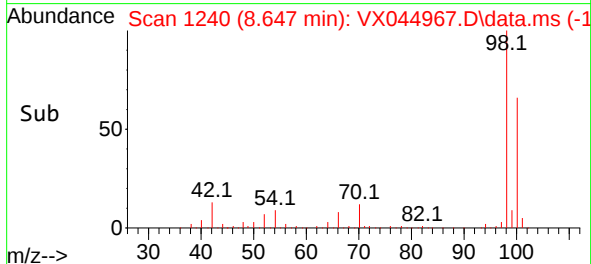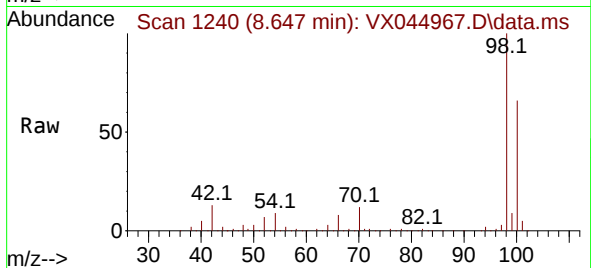

#62
4-Bromofluorobenzene
Concen: 54.500 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX044967.D
Acq: 14 Feb 2025 17:25

Tgt Ion: 95 Resp: 73777
Ion Ratio Lower Upper
95 100
174 72.0 0.0 142.6
176 69.9 0.0 141.6


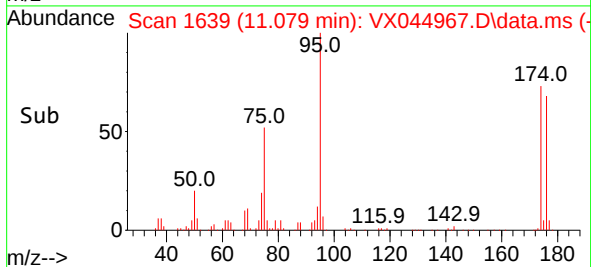

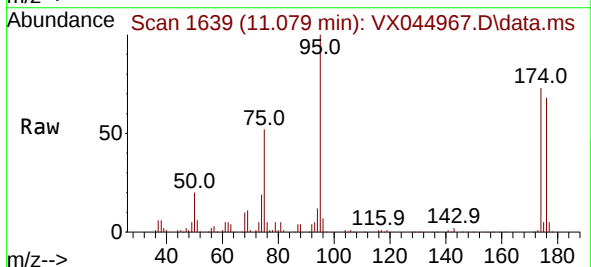


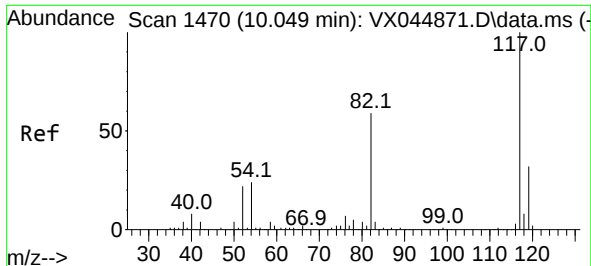

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX044967.D
Acq: 14 Feb 2025 17:25




Instrument :
MSVOA_X
ClientSampleId :
VFCC-2-021225


Tgt Ion:117 Resp: 153346
Ion Ratio Lower Upper
117 100
82 60.7 47.5 71.3
119 33.2 25.4 38.0

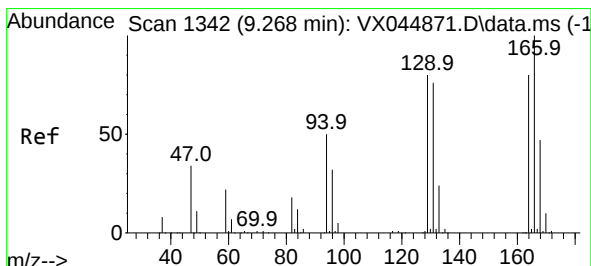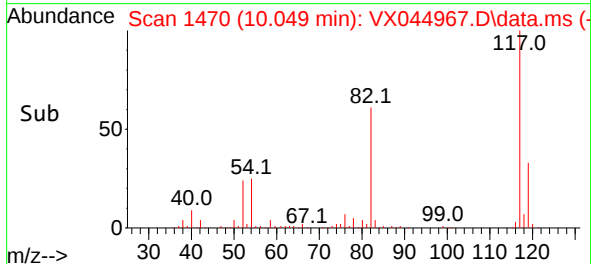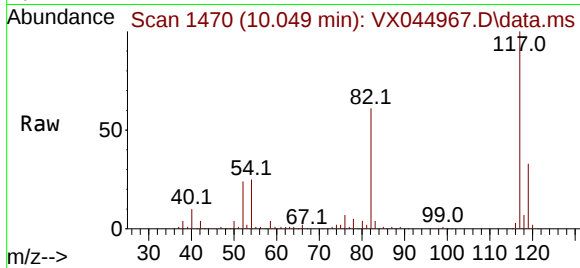

#64
Tetrachloroethene
Concen: 0.541 ug/l
RT: 9.269 min Scan# 1342
Delta R.T. 0.000 min
Lab File: VX044967.D
Acq: 14 Feb 2025 17:25


Tgt Ion:164 Resp: 523
Ion Ratio Lower Upper
164 100
166 86.7 100.4 150.6#
129 97.4 79.9 119.9
131 66.0 75.9 113.9#

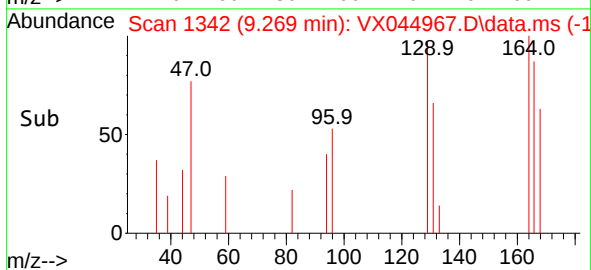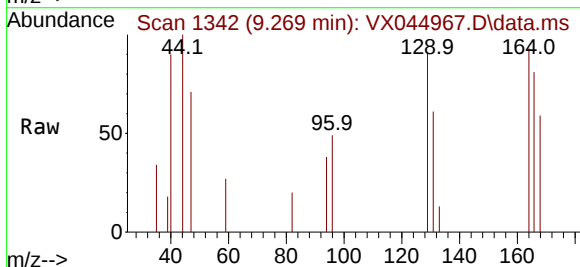

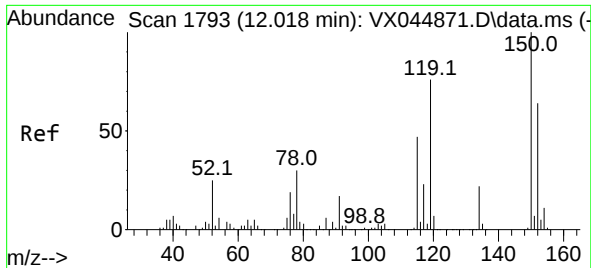

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX044967.D
 Acq: 14 Feb 2025 17:25

Instrument :
 MSVOA_X
 ClientSampleId :
 VFCC-2-021225

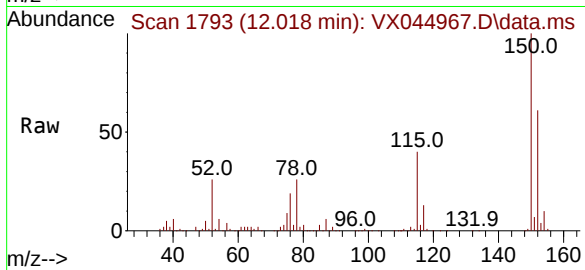

Tgt Ion:152 Resp: 68646
 Ion Ratio Lower Upper
 152 100
 115 63.6 43.4 130.1
 150 161.5 0.0 350.4

