
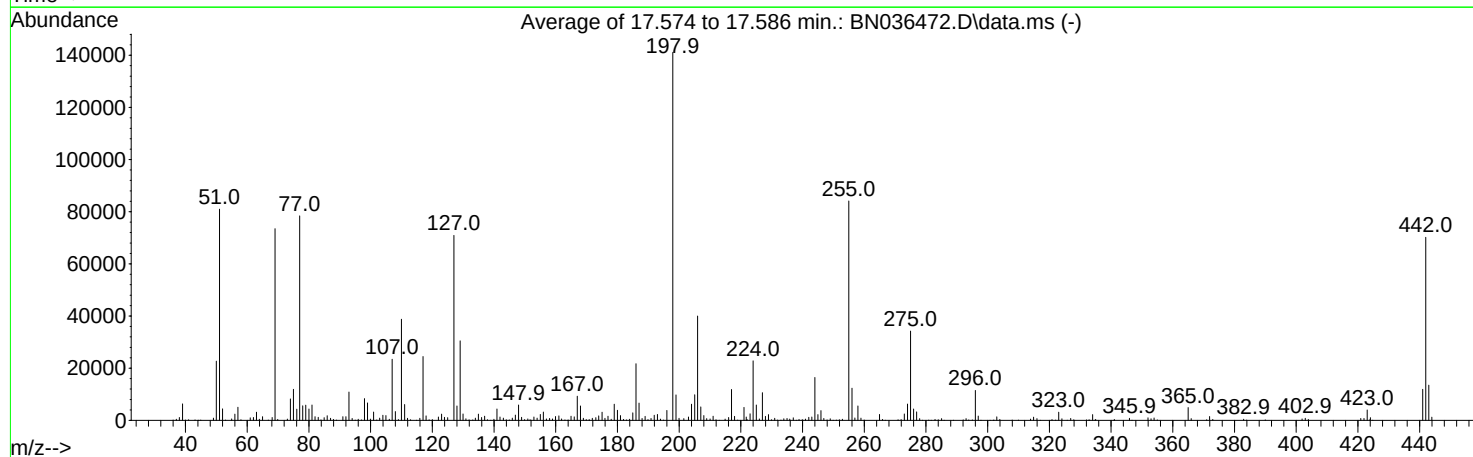


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022025\
Data File : BN036472.D
Acq On : 20 Feb 2025 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 11 01:17:14 2025

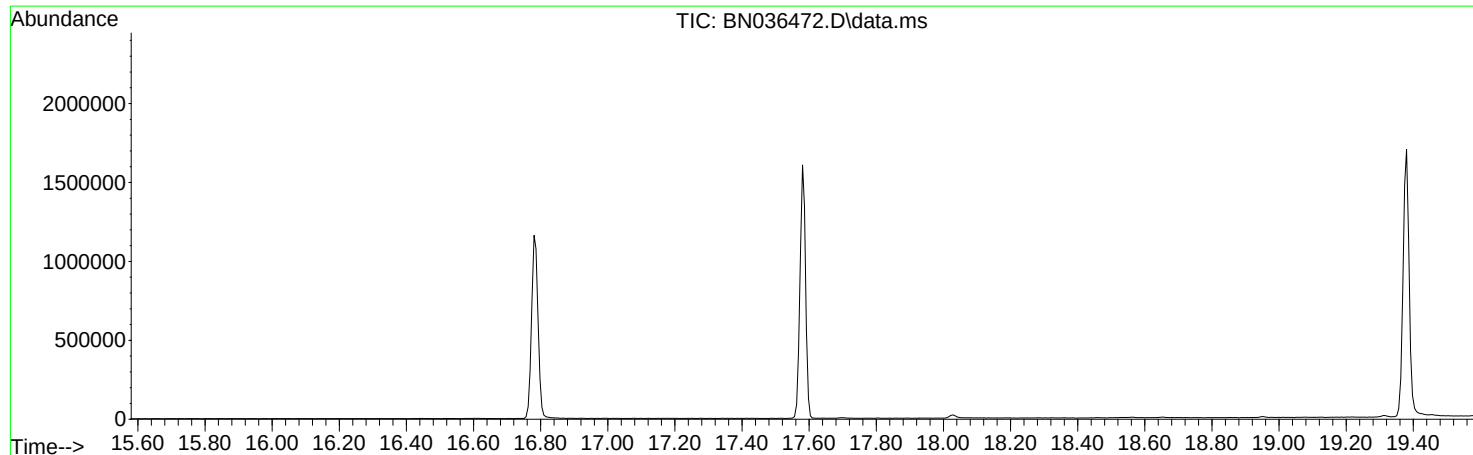

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.4	80973	PASS
68	69	0.00	2	1.5	1126	PASS
69	198	0.00	100	52.1	73475	PASS
70	69	0.00	2	0.5	370	PASS
127	198	10	80	50.3	70957	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	141053	PASS
199	198	5	9	6.9	9758	PASS
275	198	10	60	24.3	34267	PASS
365	198	1	100	3.5	4912	PASS
441	198	0.01	100	8.4	11880	PASS
442	442	50	100	100.0	70216	PASS
443	442	15	24	19.3	13522	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/20/2025	BNA_N	<u>BN036472.D</u>
Compound Name	Response	Retention Time
DDT	465194	20.621
DDD	5607	20.227
DDE	141	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5748	470942	1.22

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022025\
Data File : BN036472.D
Acq On : 20 Feb 2025 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 21 02:03:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

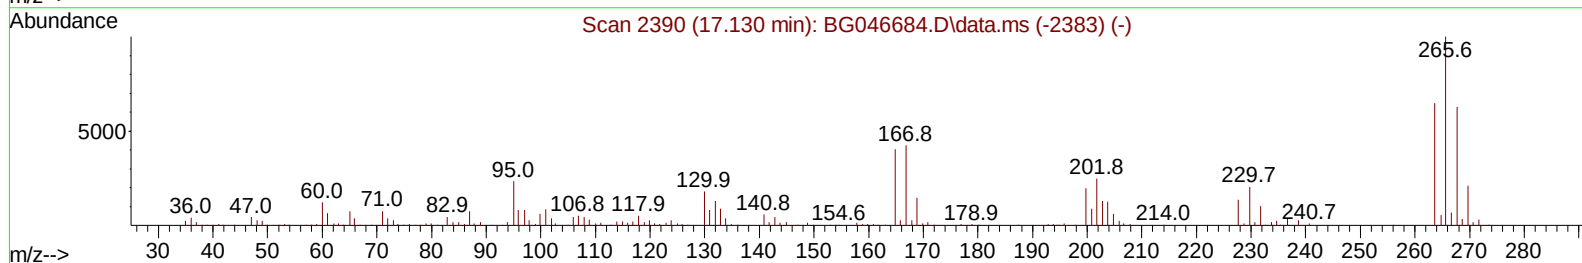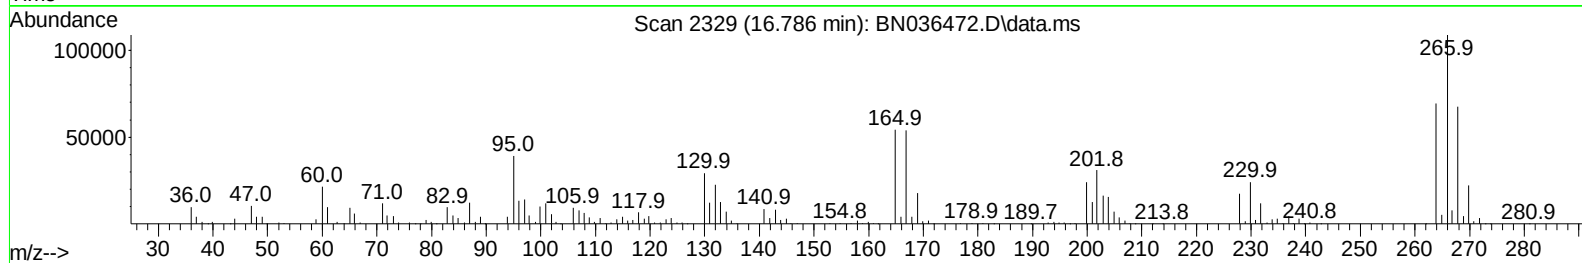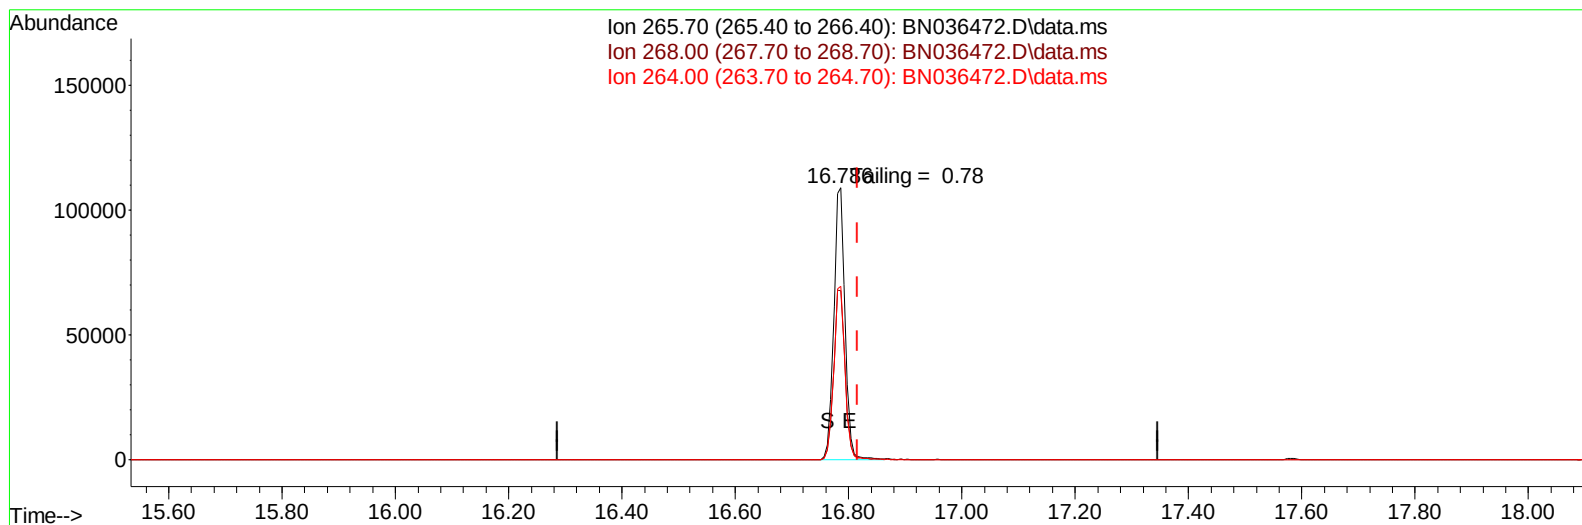

TIC: BN036472.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.030) 19225.56 ng




response 150123

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.22
264.00	61.60	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022025\
Data File : BN036472.D
Acq On : 20 Feb 2025 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 21 02:03:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

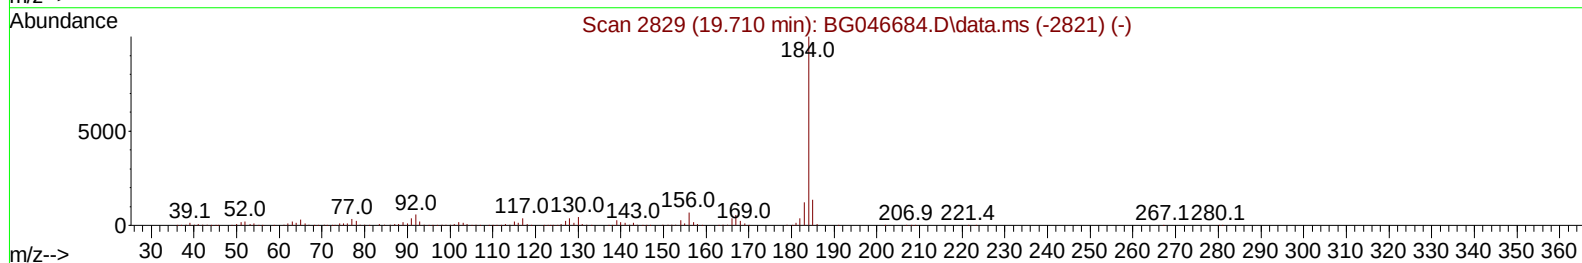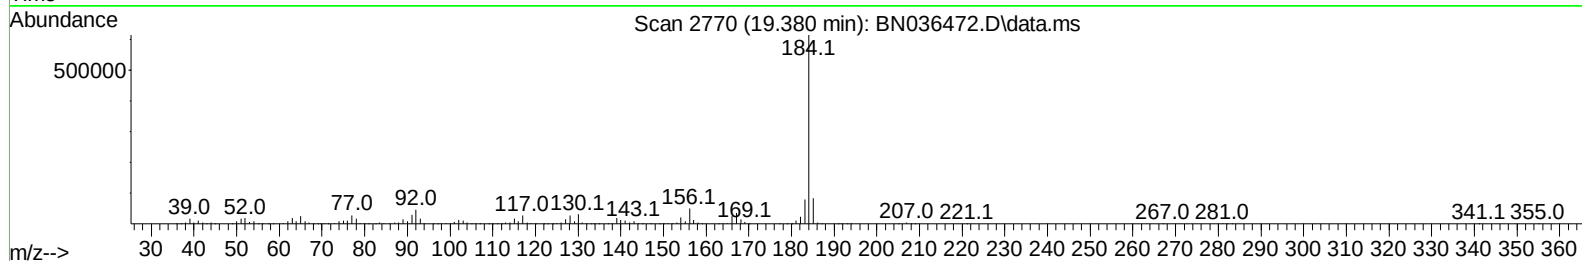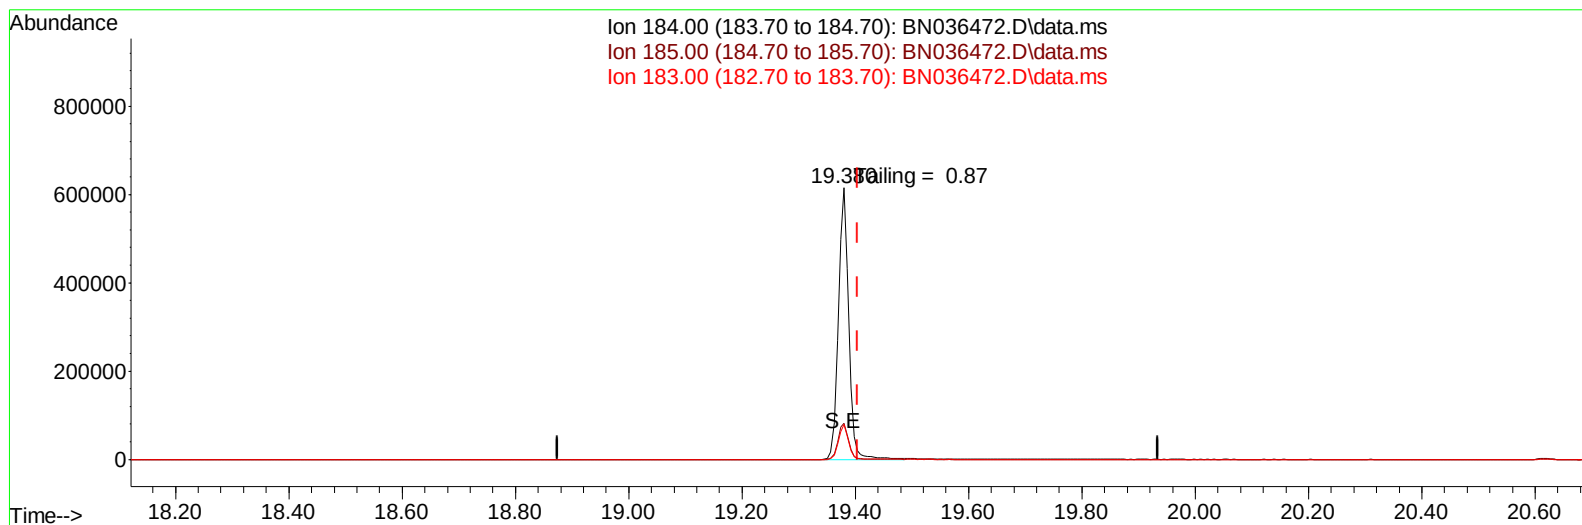

TIC: BN036472.D\data.ms

(77) Benzidine

19.380min (-0.024) 0.00 ng

response 787833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.45
183.00	13.20	12.84
0.00	0.00	0.00