
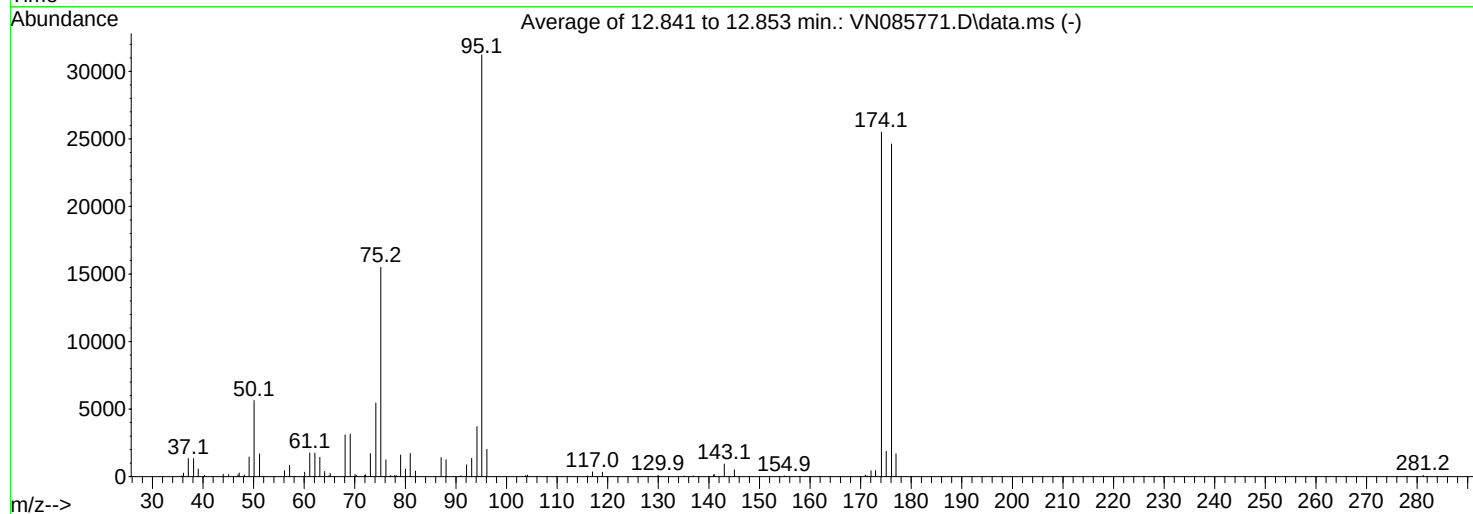


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021825\
Data File : VN085771.D
Acq On : 18 Feb 2025 10:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

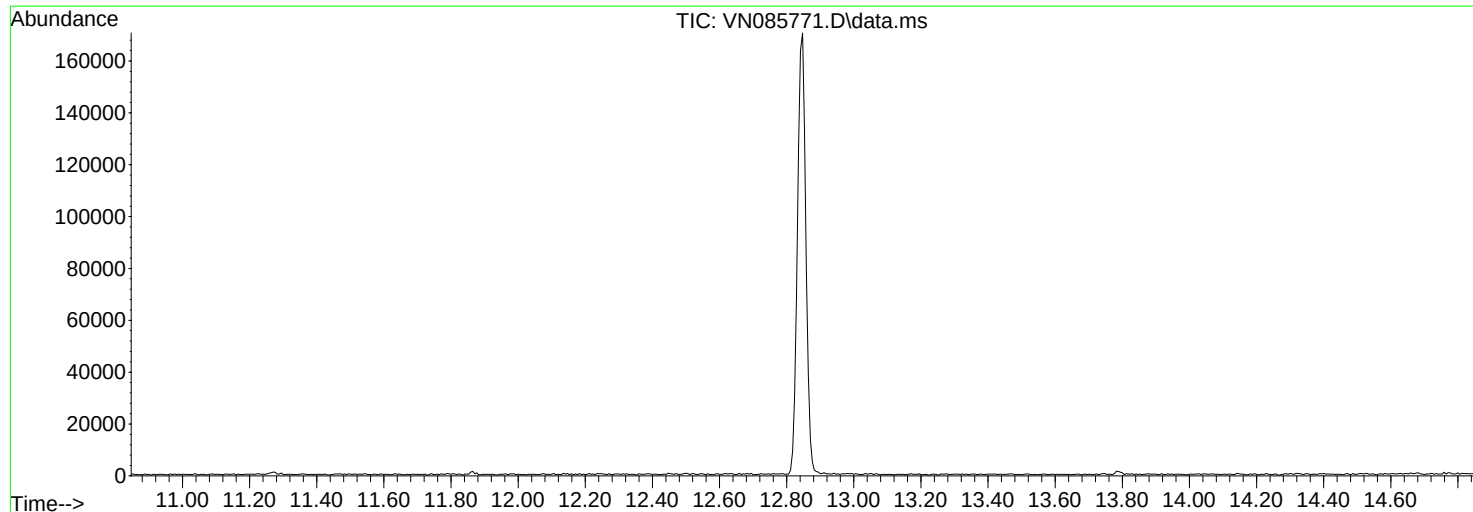

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	5643	PASS
75	95	30	60	49.7	15509	PASS
95	95	100	100	100.0	31224	PASS
96	95	5	9	6.5	2024	PASS
173	174	0.00	2	1.8	452	PASS
174	95	50	100	81.7	25509	PASS
175	174	5	9	7.4	1882	PASS
176	174	95	101	96.5	24621	PASS
177	176	5	9	6.9	1699	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	65	48.15	124	64.90	70	76.15	124
36.15	261	49.10	1454	65.15	255	77.10	80
37.10	1338	50.10	5643	68.10	3096	77.90	80
38.15	1335	51.15	1680	69.10	3155	78.20	80
39.05	560	56.10	443	70.05	161	79.05	1595
40.00	21	57.10	824	70.30	106	80.00	557
40.30	99	60.10	333	71.90	80	80.95	1716
44.00	176	61.10	1754	72.15	148	82.00	419
45.05	157	62.10	1754	73.10	1710	87.05	1414
46.90	145	63.10	1428	74.15	5444	88.05	1255
47.15	276	64.05	377	75.15	15509	91.00	59

Average of 12.841 to 12.853 min.: VN085771.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.10	882	135.10	54	174.10	25509		
93.10	1346	136.90	57	175.05	1882		
94.15	3713	140.90	114	176.10	24621		
95.10	31224	141.05	164	177.00	1699		
96.10	2024	143.05	938	281.20	112		
103.80	81	145.05	510				
104.10	121	154.90	54				
116.00	52	170.90	116				
117.00	351	171.30	58				
118.95	331	172.05	440				
129.95	112	172.95	452				

Instrument :

MSVOA_N

ClientSampleId :

BFB