

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021925\
 Data File : PL094277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2025 19:08
 Operator : AR\AJ
 Sample : Q1382-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU4-PCS-TC-08-021725

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/20/2025
 Supervised By :Ankita Jodhani 02/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 01:16:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:58:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.772	60875994	76118275	22.607m	23.319
28) SA Decachlor...	9.050	7.905	42420731	72913446	20.278	20.808

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021925\
Data File : PL094277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2025 19:08
Operator : AR\AJ
Sample : Q1382-15
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OU4-PCS-TC-08-021725


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/20/2025
Supervised By : Ankita Jodhani 02/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 01:16:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:58:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

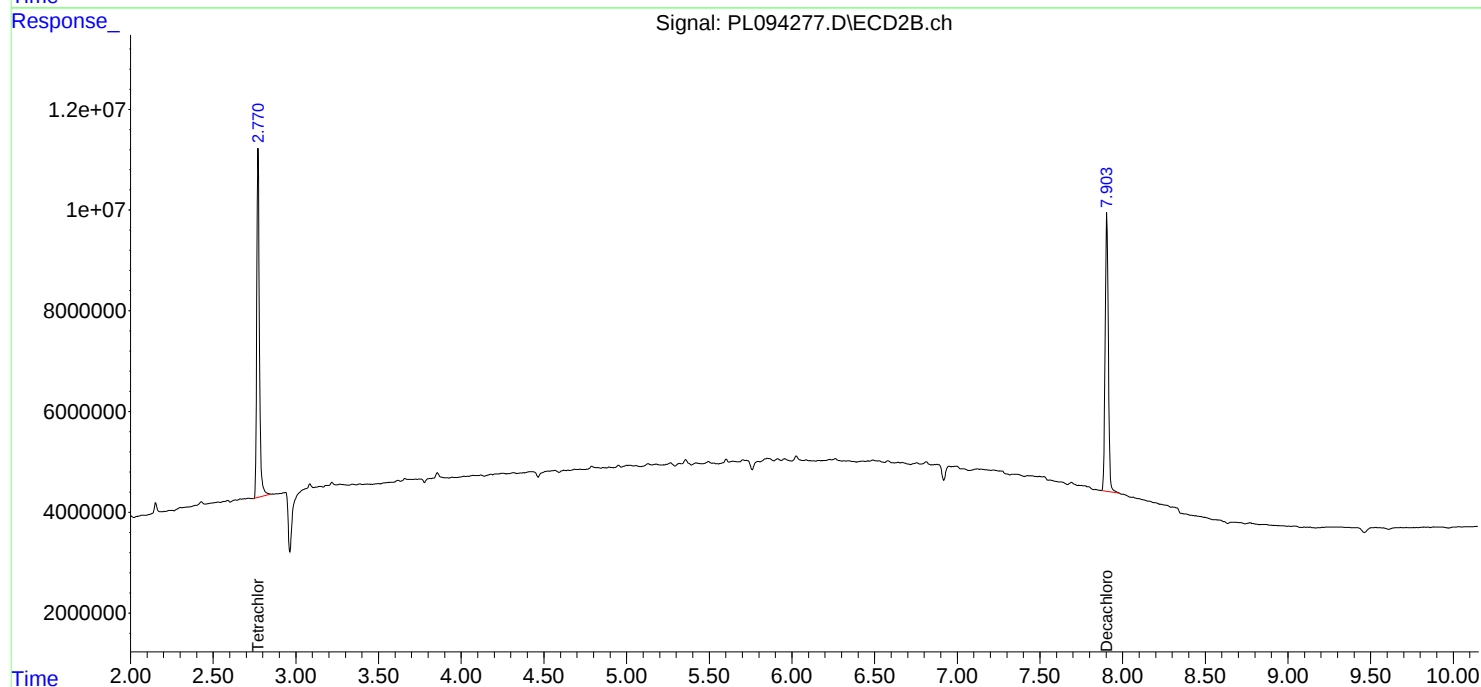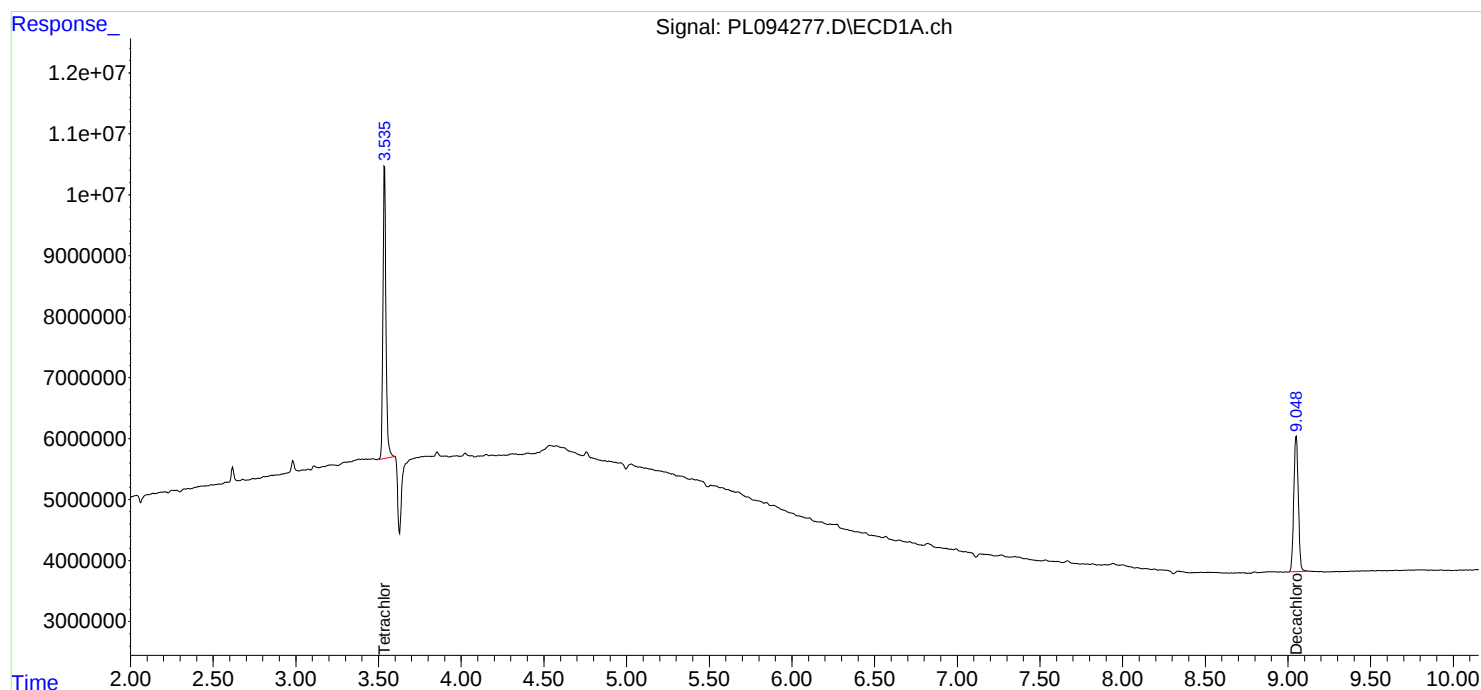

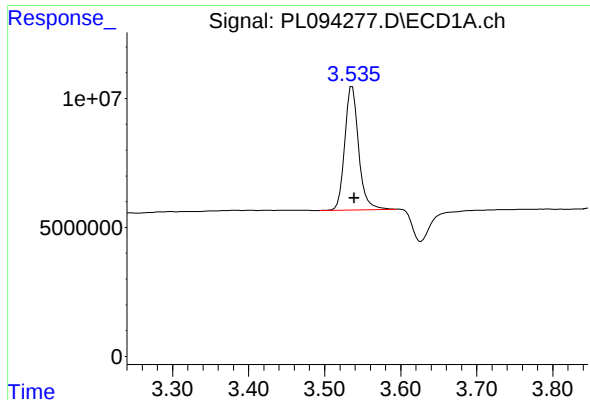


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.004 min
Response: 60875994
Conc: 22.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU4-PCS-TC-08-021725


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/20/2025
Supervised By :Ankita Jodhani 02/20/2025

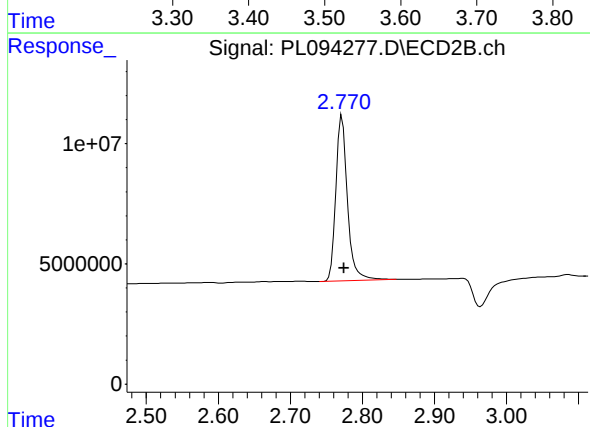


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.003 min
Response: 76118275
Conc: 23.32 ng/ml

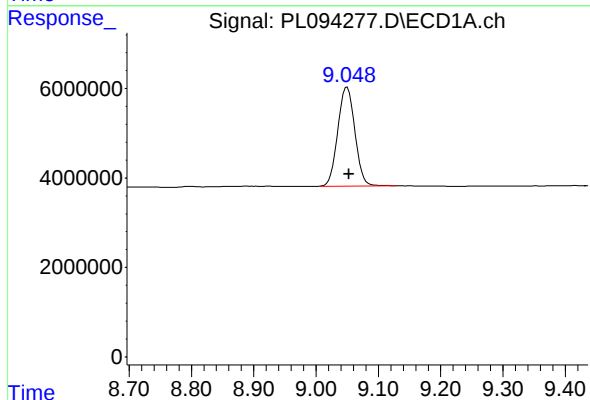

#28 Decachlorobiphenyl

R.T.: 9.050 min
Delta R.T.: -0.003 min
Response: 42420731
Conc: 20.28 ng/ml

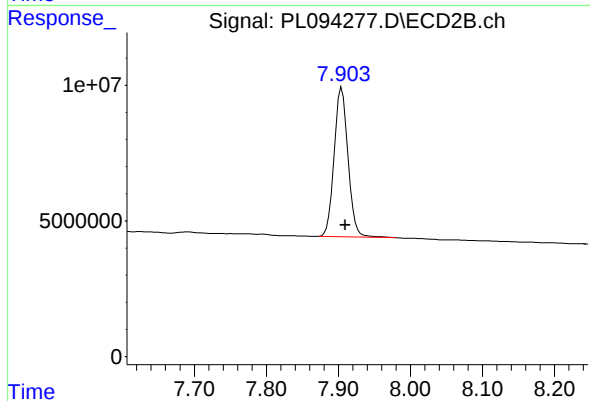

#28 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: -0.005 min
Response: 72913446
Conc: 20.81 ng/ml