

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141672.D
 Acq On : 19 Feb 2025 13:43
 Operator : RC/JU
 Sample : PB166772BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166772BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	558	563	596	rBV	1655061	2307155	81.58%	13.958%
2	6.422	730	736	756	rBV	1608256	2271693	80.32%	13.744%
3	6.781	792	797	813	rVB	367282	469085	16.59%	2.838%
4	7.345	886	893	921	rBV	1063635	1524402	53.90%	9.223%
5	8.063	1009	1015	1037	rBV	422242	611290	21.61%	3.698%
6	9.139	1192	1198	1233	rVB	2039918	2828199	100.00%	17.110%
7	9.816	1307	1313	1326	rBV	493616	678103	23.98%	4.102%
8	10.604	1442	1447	1468	rBV	1140846	1552795	54.90%	9.394%
9	11.298	1560	1565	1582	rBV	442725	631900	22.34%	3.823%
10	12.886	1829	1835	1840	rBV	1799612	2354196	83.24%	14.243%
11	13.939	2009	2014	2024	rBV	299200	417847	14.77%	2.528%
12	14.892	2168	2176	2192	rVB5	21370	86638	3.06%	0.524%
13	15.380	2253	2259	2273	rBV	236096	407175	14.40%	2.463%
14	16.321	2412	2419	2441	rVB4	19463	89988	3.18%	0.544%
15	16.668	2467	2478	2499	rVB3	56860	298655	10.56%	1.807%




Sum of corrected areas: 16529121

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141672.D
Acq On : 19 Feb 2025 13:43
Operator : RC/JU
Sample : PB166772BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166772BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

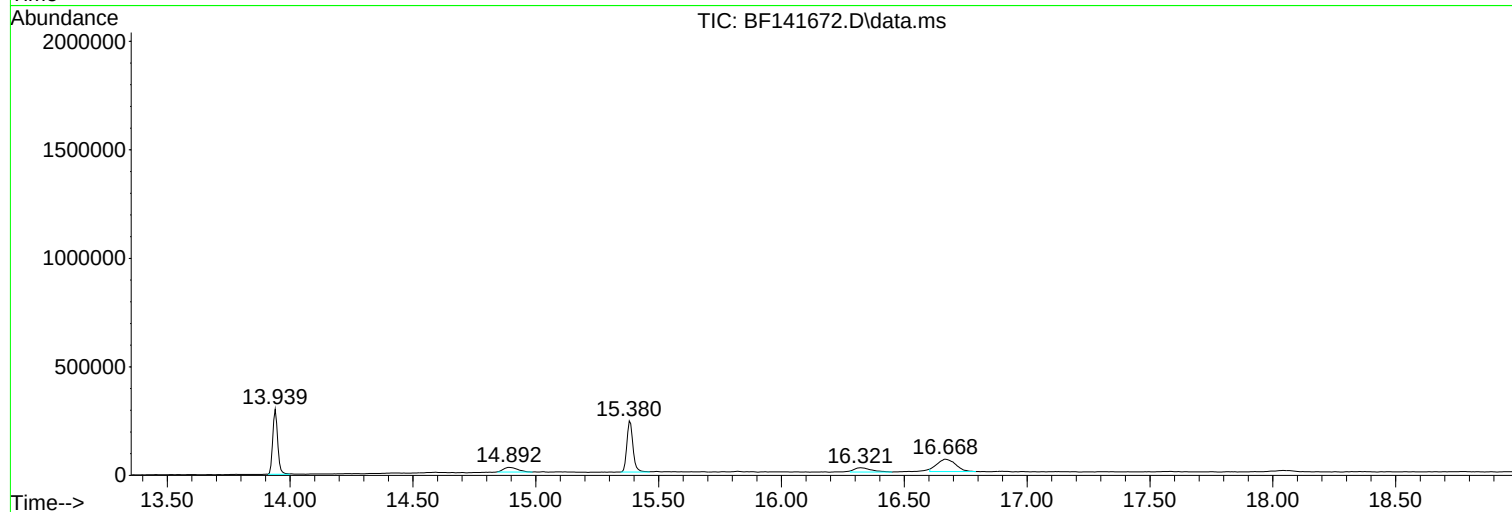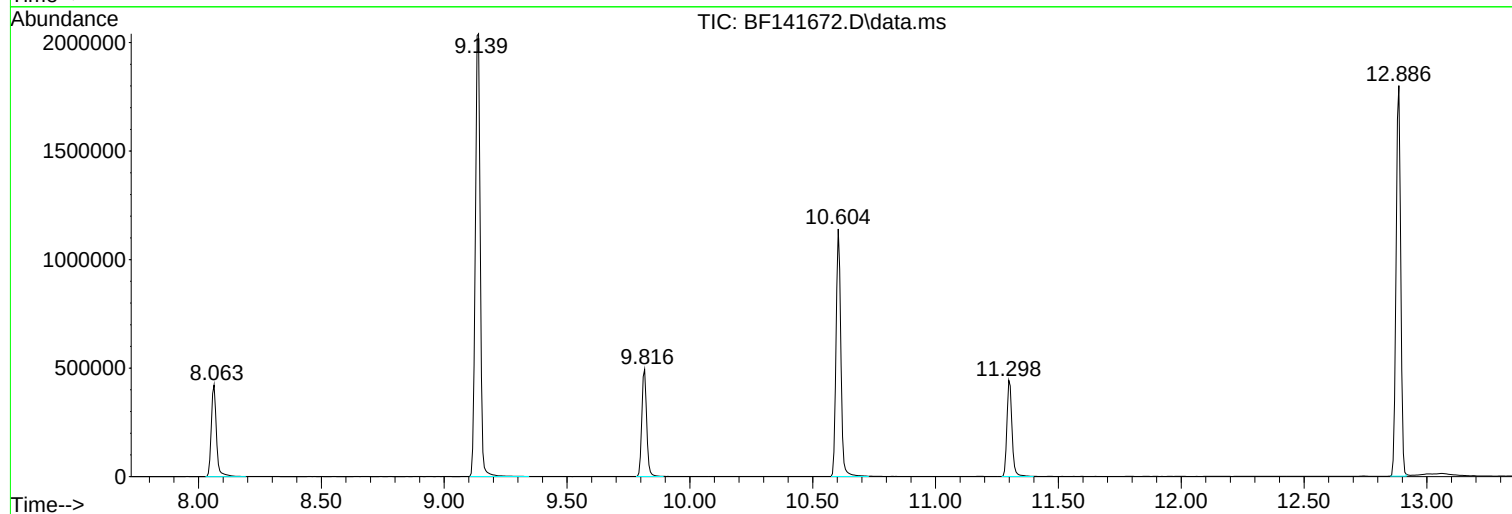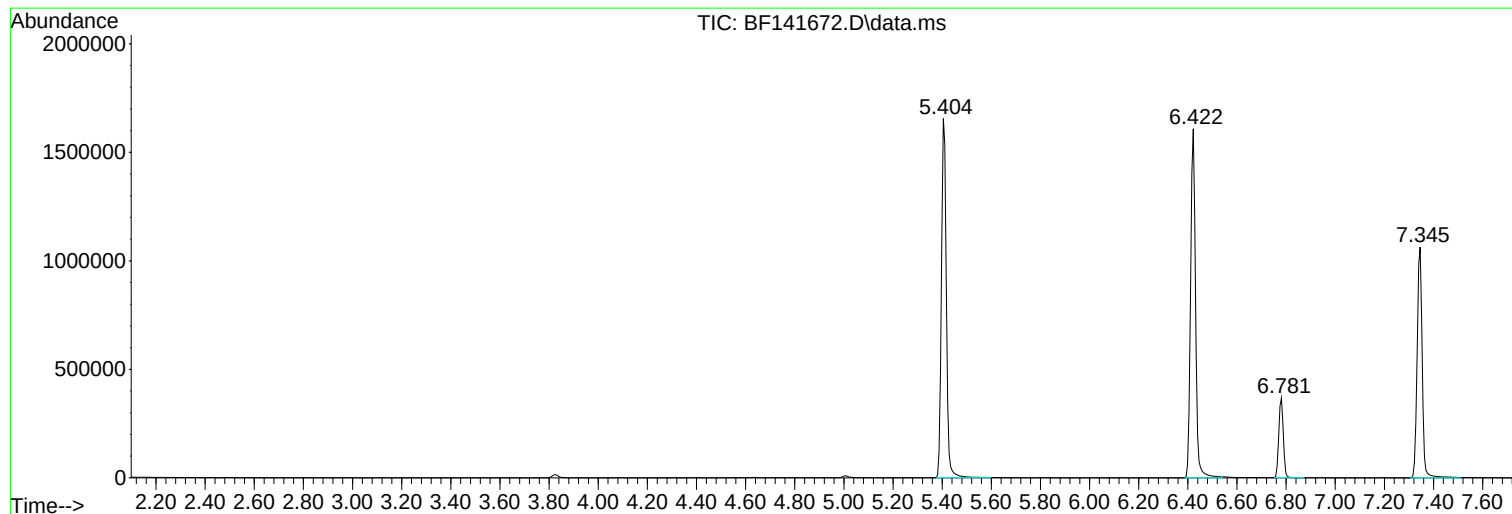

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141672.D
Acq On : 19 Feb 2025 13:43
Operator : RC/JU
Sample : PB166772BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166772BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141672.D
Acq On : 19 Feb 2025 13:43
Operator : RC/JU
Sample : PB166772BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166772BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------