

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
 Data File : BF141679.D  
 Acq On : 19 Feb 2025 17:14  
 Operator : RC/JU  
 Sample : Q1382-07  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-PCS-TC-04-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141679.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.992       | 489           | 493         | 508          | rVB      | 12031          | 22991         | 1.05%           | 0.160%        |
| 2         | 5.404       | 557           | 563         | 588          | rBV      | 1310314        | 1815553       | 82.64%          | 12.666%       |
| 3         | 6.422       | 730           | 736         | 758          | rBV      | 1282454        | 1828113       | 83.21%          | 12.754%       |
| 4         | 6.781       | 792           | 797         | 805          | rBV      | 405573         | 513792        | 23.39%          | 3.584%        |
| 5         | 7.345       | 887           | 893         | 905          | rBV      | 849967         | 1188021       | 54.08%          | 8.288%        |
| 6         | 7.610       | 933           | 938         | 955          | rBV      | 18117          | 42706         | 1.94%           | 0.298%        |
| 7         | 8.063       | 1009          | 1015        | 1034         | rBV      | 490025         | 686242        | 31.24%          | 4.788%        |
| 8         | 9.133       | 1191          | 1197        | 1208         | rBV      | 1669122        | 2196956       | 100.00%         | 15.327%       |
| 9         | 9.810       | 1307          | 1312        | 1327         | rBV      | 555158         | 765535        | 34.85%          | 5.341%        |
| 10        | 10.527      | 1429          | 1434        | 1441         | rBV      | 119173         | 154988        | 7.05%           | 1.081%        |
| 11        | 10.604      | 1441          | 1447        | 1463         | rVV      | 927223         | 1265745       | 57.61%          | 8.830%        |
| 12        | 11.298      | 1560          | 1565        | 1583         | rVB      | 559803         | 756178        | 34.42%          | 5.275%        |
| 13        | 11.827      | 1650          | 1655        | 1680         | rBV      | 87759          | 191246        | 8.71%           | 1.334%        |
| 14        | 12.880      | 1828          | 1834        | 1845         | rBV      | 1562123        | 2009939       | 91.49%          | 14.022%       |
| 15        | 13.810      | 1984          | 1992        | 1998         | rBV8     | 7627           | 29037         | 1.32%           | 0.203%        |
| 16        | 13.933      | 2008          | 2013        | 2024         | rBV      | 320822         | 461055        | 20.99%          | 3.217%        |
| 17        | 15.380      | 2253          | 2259        | 2270         | rBV      | 242060         | 405706        | 18.47%          | 2.830%        |




Sum of corrected areas: 14333803

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141679.D  
Acq On : 19 Feb 2025 17:14  
Operator : RC/JU  
Sample : Q1382-07  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-04-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

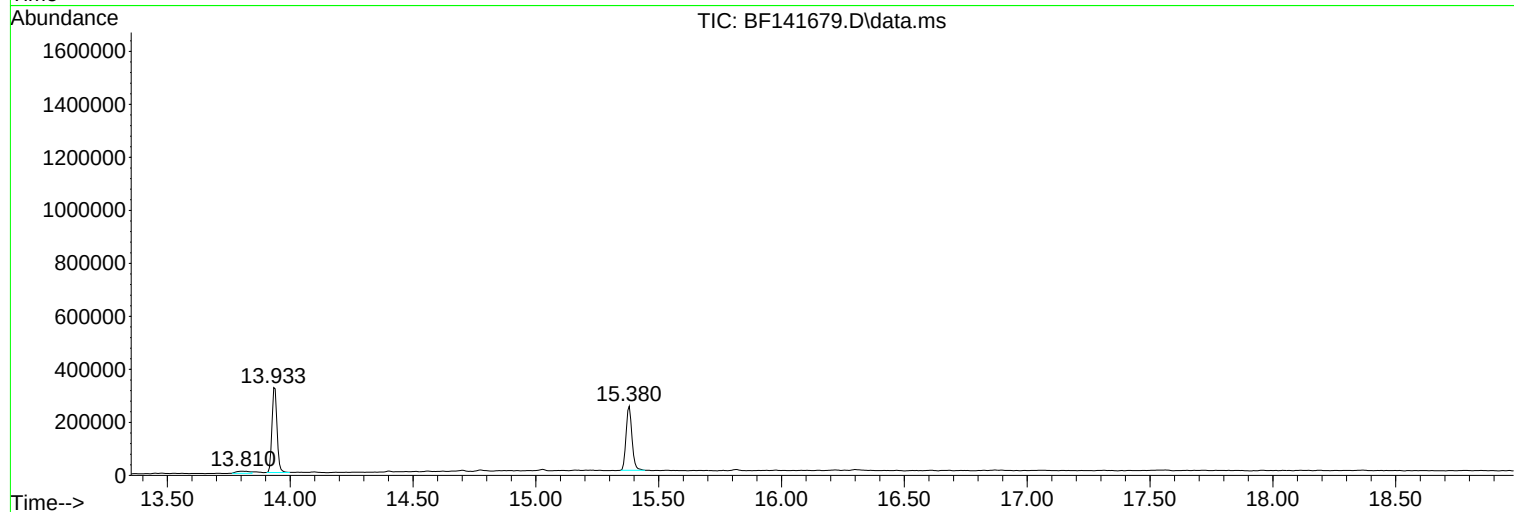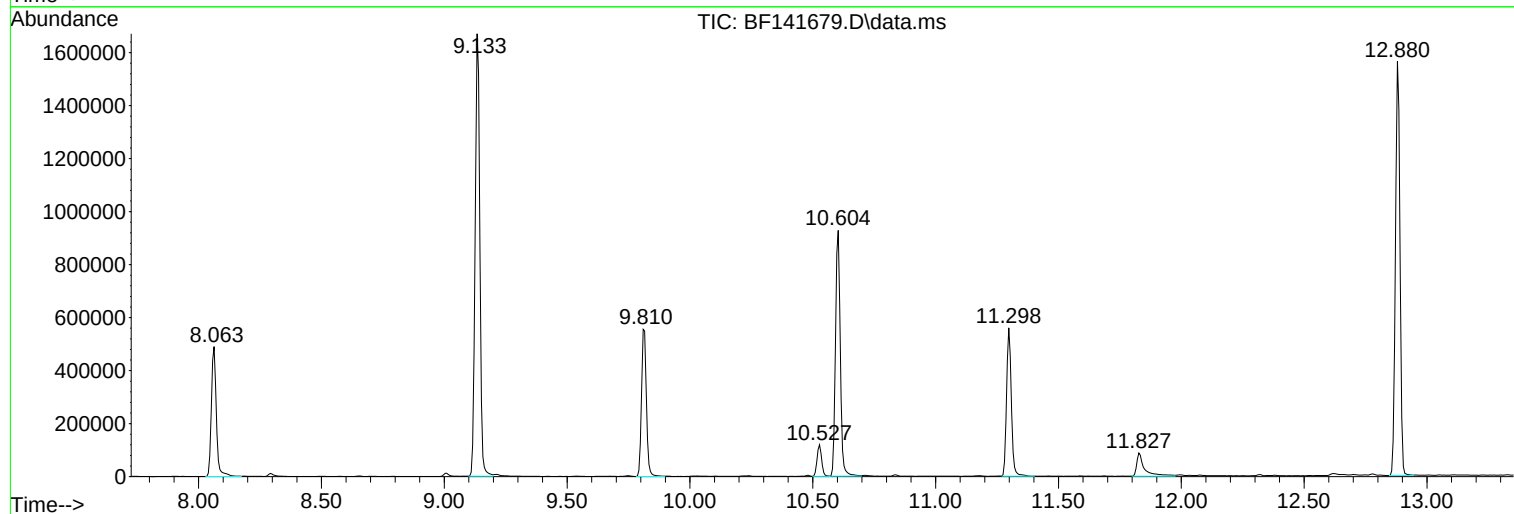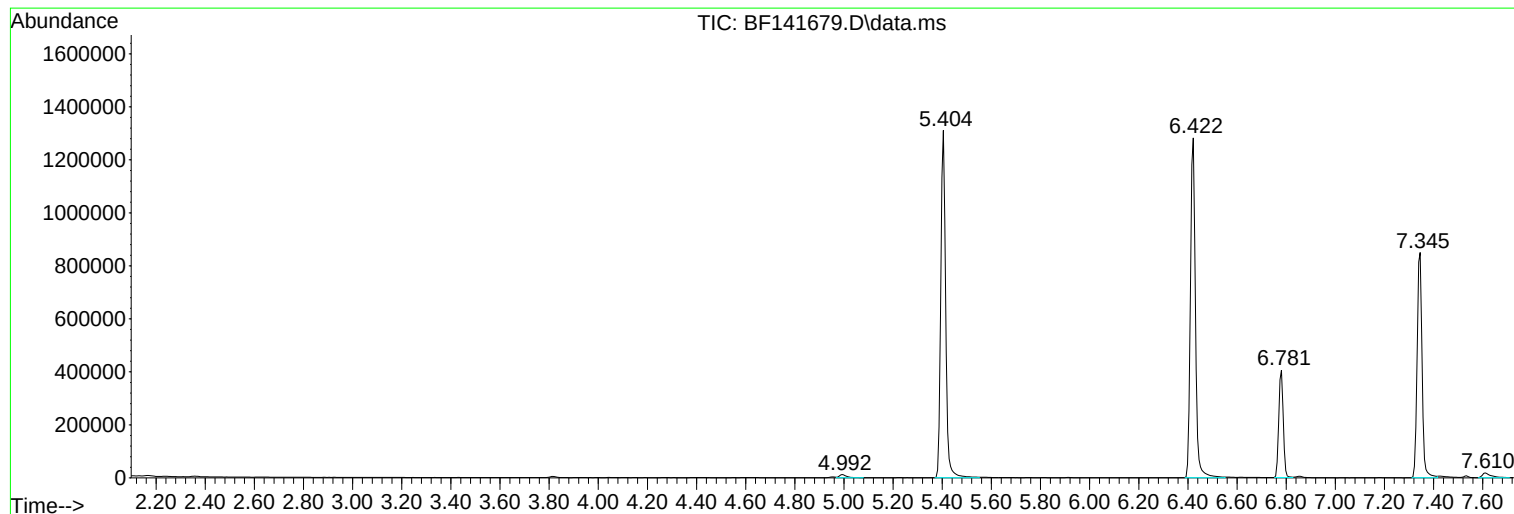

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141679.D  
Acq On : 19 Feb 2025 17:14  
Operator : RC/JU  
Sample : Q1382-07  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-04-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141679.D  
Acq On : 19 Feb 2025 17:14  
Operator : RC/JU  
Sample : Q1382-07  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-04-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|