

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141681.D
 Acq On : 19 Feb 2025 18:12
 Operator : RC/JU
 Sample : Q1382-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-06-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	557	563	589	rBV	953265	1391924	86.56%	11.762%
2	6.416	730	735	765	rBV	971405	1425917	88.68%	12.050%
3	6.781	792	797	805	rBV	423186	543407	33.79%	4.592%
4	7.339	887	892	905	rBV	624461	897880	55.84%	7.587%
5	7.622	934	940	952	rBV6	6634	19615	1.22%	0.166%
6	8.063	1009	1015	1034	rBV	509573	724384	45.05%	6.121%
7	9.133	1192	1197	1209	rBV	1247022	1608002	100.00%	13.588%
8	9.810	1307	1312	1326	rBV	589814	816807	50.80%	6.902%
9	10.527	1428	1434	1441	rBV	88901	119459	7.43%	1.009%
10	10.604	1441	1447	1463	rVV	657179	944715	58.75%	7.983%
11	11.298	1560	1565	1582	rBV	587805	796547	49.54%	6.731%
12	11.827	1650	1655	1671	rBV3	27960	64410	4.01%	0.544%
13	12.880	1828	1834	1844	rBV	1211603	1549901	96.39%	13.097%
14	13.810	1981	1992	2001	rBV7	7340	32835	2.04%	0.277%
15	13.939	2008	2014	2024	rBV	326463	469848	29.22%	3.970%
16	15.380	2253	2259	2271	rBV	254960	428122	26.62%	3.618%




Sum of corrected areas: 11833773

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141681.D
Acq On : 19 Feb 2025 18:12
Operator : RC/JU
Sample : Q1382-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-06-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

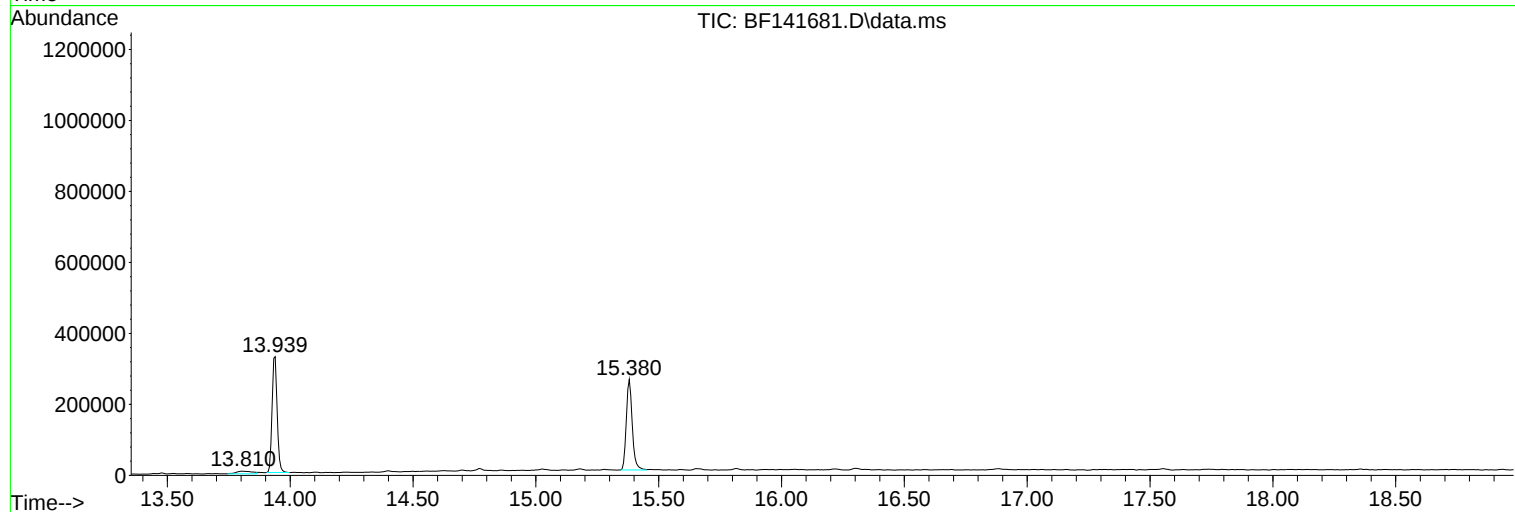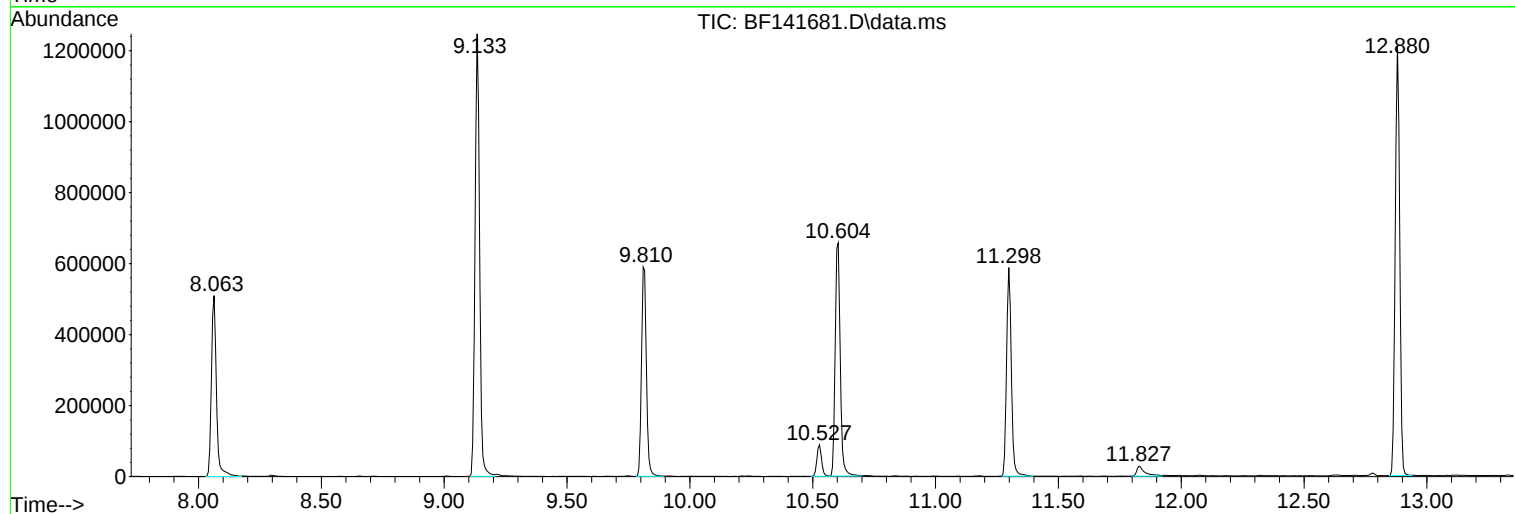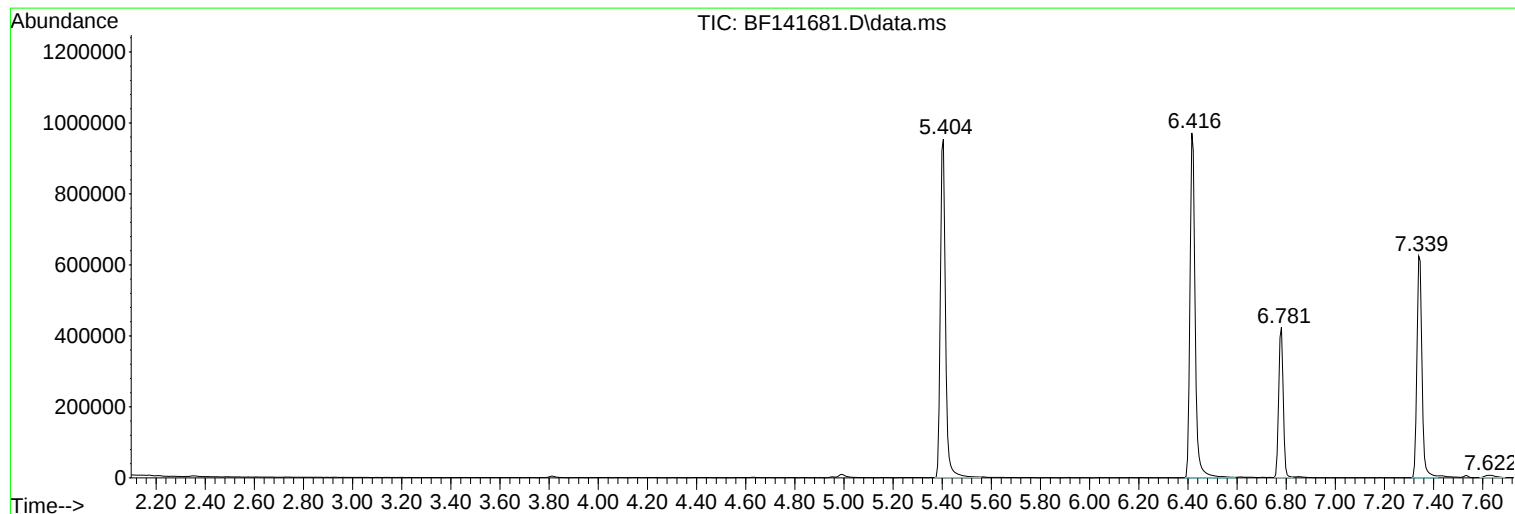

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141681.D
Acq On : 19 Feb 2025 18:12
Operator : RC/JU
Sample : Q1382-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-06-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141681.D
Acq On : 19 Feb 2025 18:12
Operator : RC/JU
Sample : Q1382-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-06-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------