


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141670.D
Acq On : 19 Feb 2025 12:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

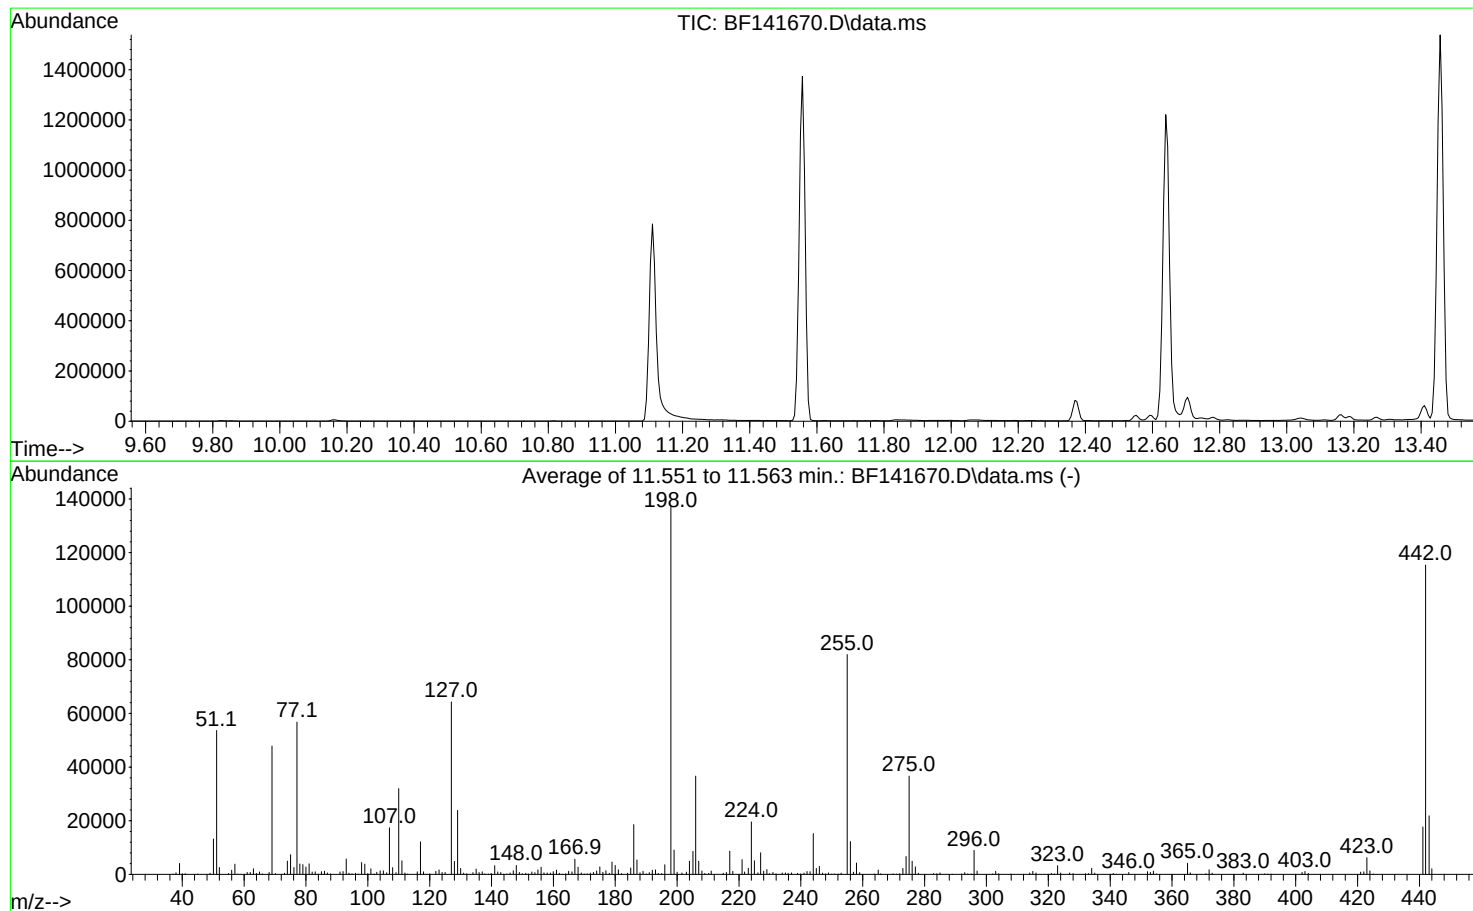

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	53635	PASS
68	69	0.00	2	1.5	716	PASS
69	198	0.00	100	34.9	47837	PASS
70	69	0.00	2	0.6	301	PASS
127	198	10	80	46.9	64312	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137187	PASS
199	198	5	9	6.6	9087	PASS
275	198	10	60	26.7	36637	PASS
365	198	1	100	3.1	4201	PASS
441	198	0.01	100	12.9	17651	PASS
442	442	50	100	100.0	115347	PASS
443	442	15	24	18.9	21851	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/19/2025	BNA_F	<u>BF141670.D</u>
Compound Name	Response	Retention Time
DDT	389402	13.457
DDD	11525	13.163
DDE	603	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12128	401530	3.02

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141670.D
Acq On : 19 Feb 2025 12:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 19 13:37:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

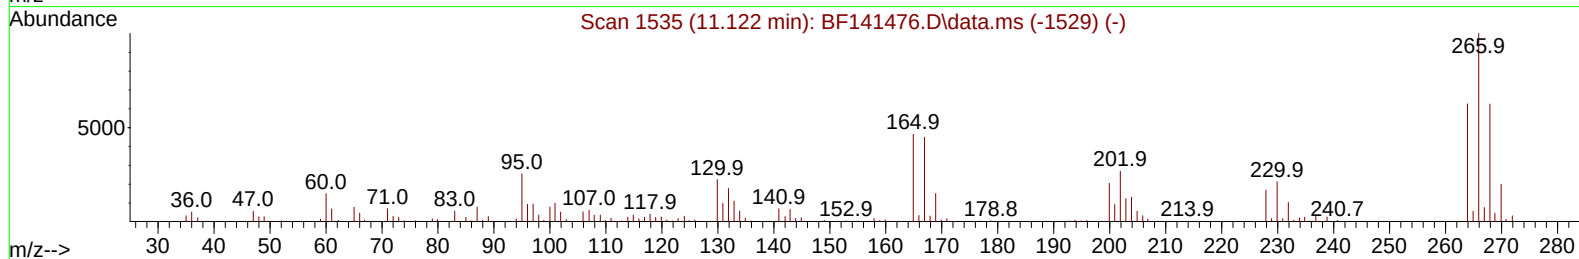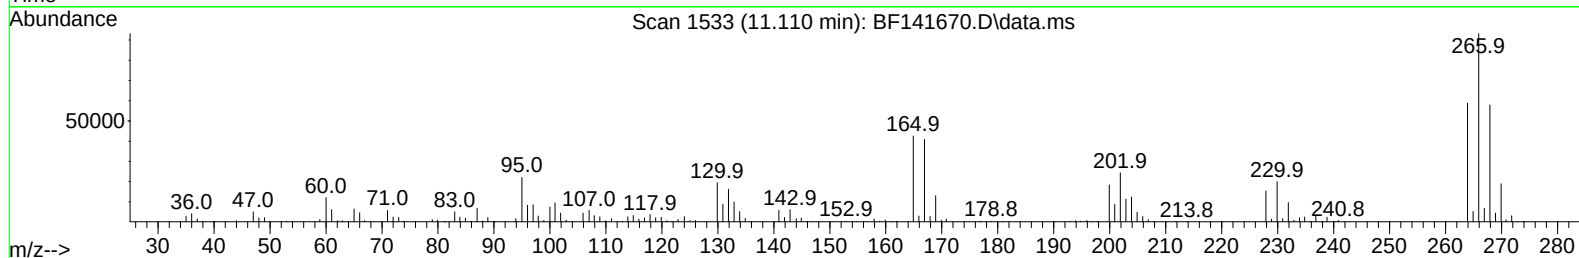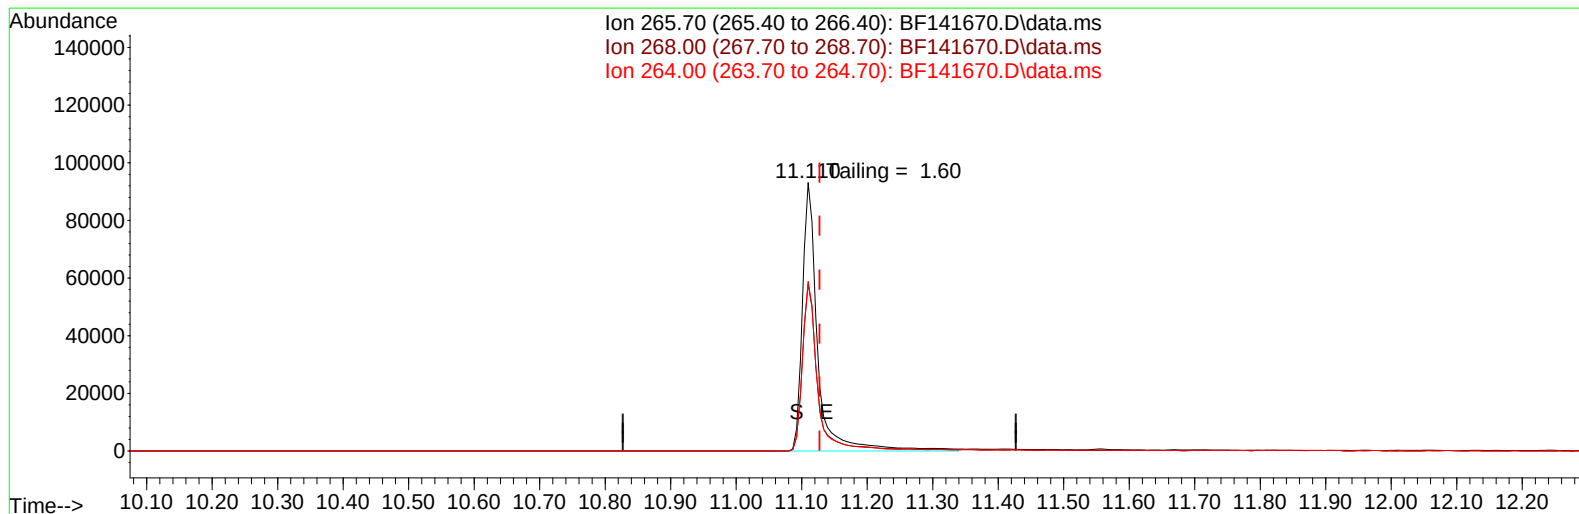

TIC: BF141670.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.017) 24620.99 ng




response 150018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.18
264.00	62.60	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141670.D
Acq On : 19 Feb 2025 12:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 19 13:37:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

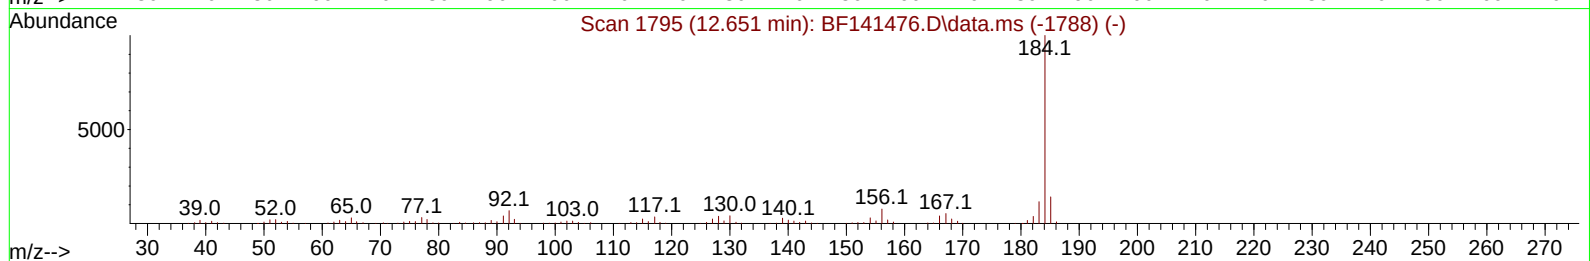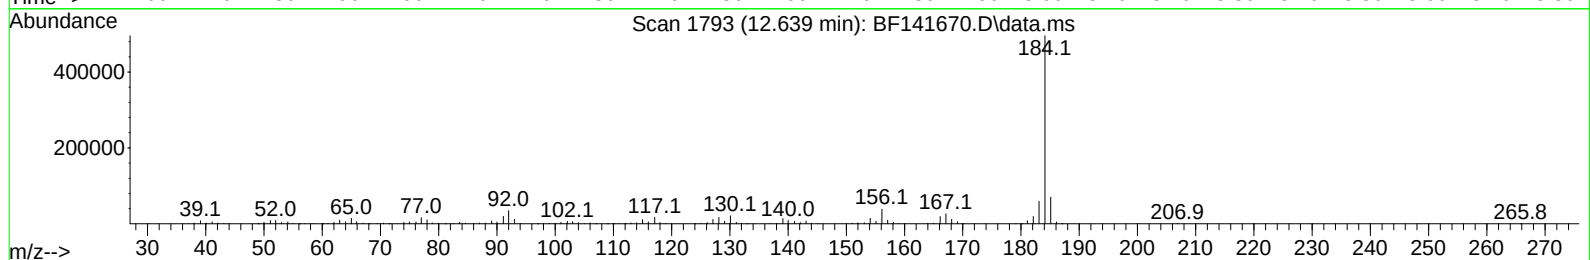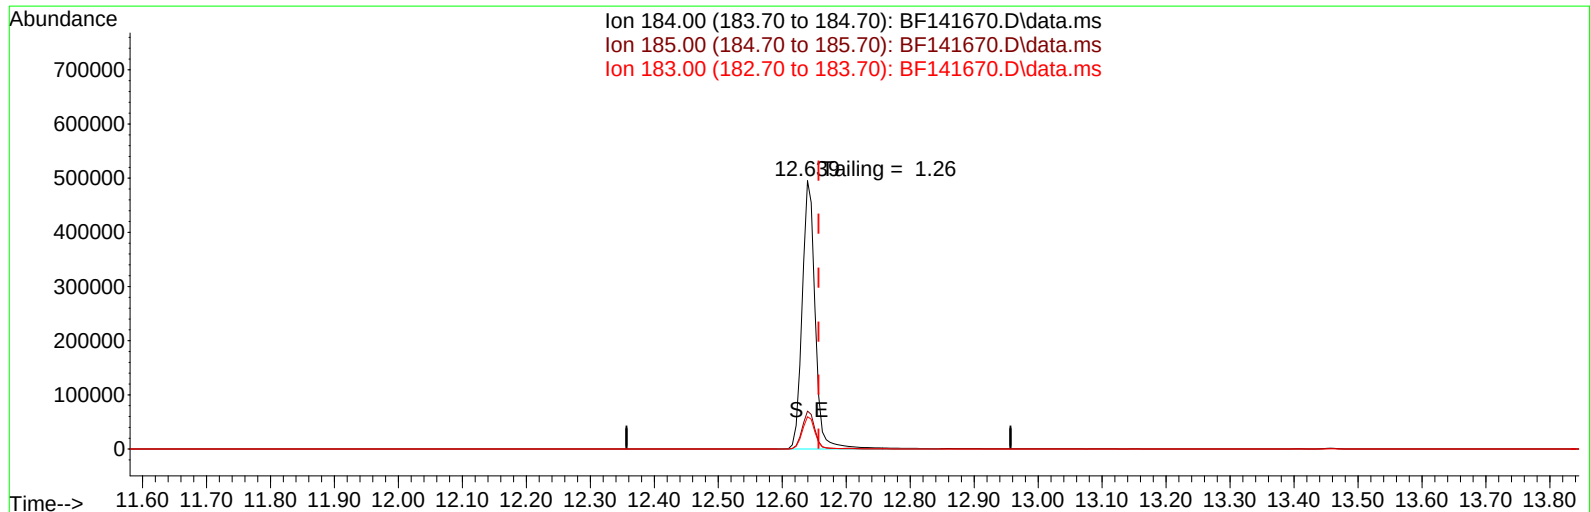

TIC: BF141670.D\data.ms

(77) Benzidine

12.639min (-0.017) 0.00 ng

response 706816

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.14
183.00	11.60	12.05
0.00	0.00	0.00