

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141690.D
 Acq On : 19 Feb 2025 22:37
 Operator : RC/JU
 Sample : Q1383-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-15-021725

Quant Time: Feb 20 00:16:04 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 06 16:58:59 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	93977	20.000	ng	-0.01
21) Naphthalene-d8	8.063	136	374022	20.000	ng	-0.01
39) Acenaphthene-d10	9.810	164	200098	20.000	ng	-0.02
64) Phenanthrene-d10	11.298	188	336579	20.000	ng	-0.02
76) Chrysene-d12	13.933	240	182552	20.000	ng	-0.03
86) Perylene-d12	15.380	264	183803	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.404	112	673535	112.360	ng	0.00
7) Phenol-d6	6.422	99	839637	110.822	ng	-0.02
23) Nitrobenzene-d5	7.345	82	547127	76.298	ng	-0.02
42) 2,4,6-Tribromophenol	10.604	330	225226	112.049	ng	-0.02
45) 2-Fluorobiphenyl	9.133	172	1041995	80.228	ng	-0.02
79) Terphenyl-d14	12.880	244	1043224	96.473	ng	-0.02


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141690.D
Acq On : 19 Feb 2025 22:37
Operator : RC/JU
Sample : Q1383-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-15-021725

Quant Time: Feb 20 00:16:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration



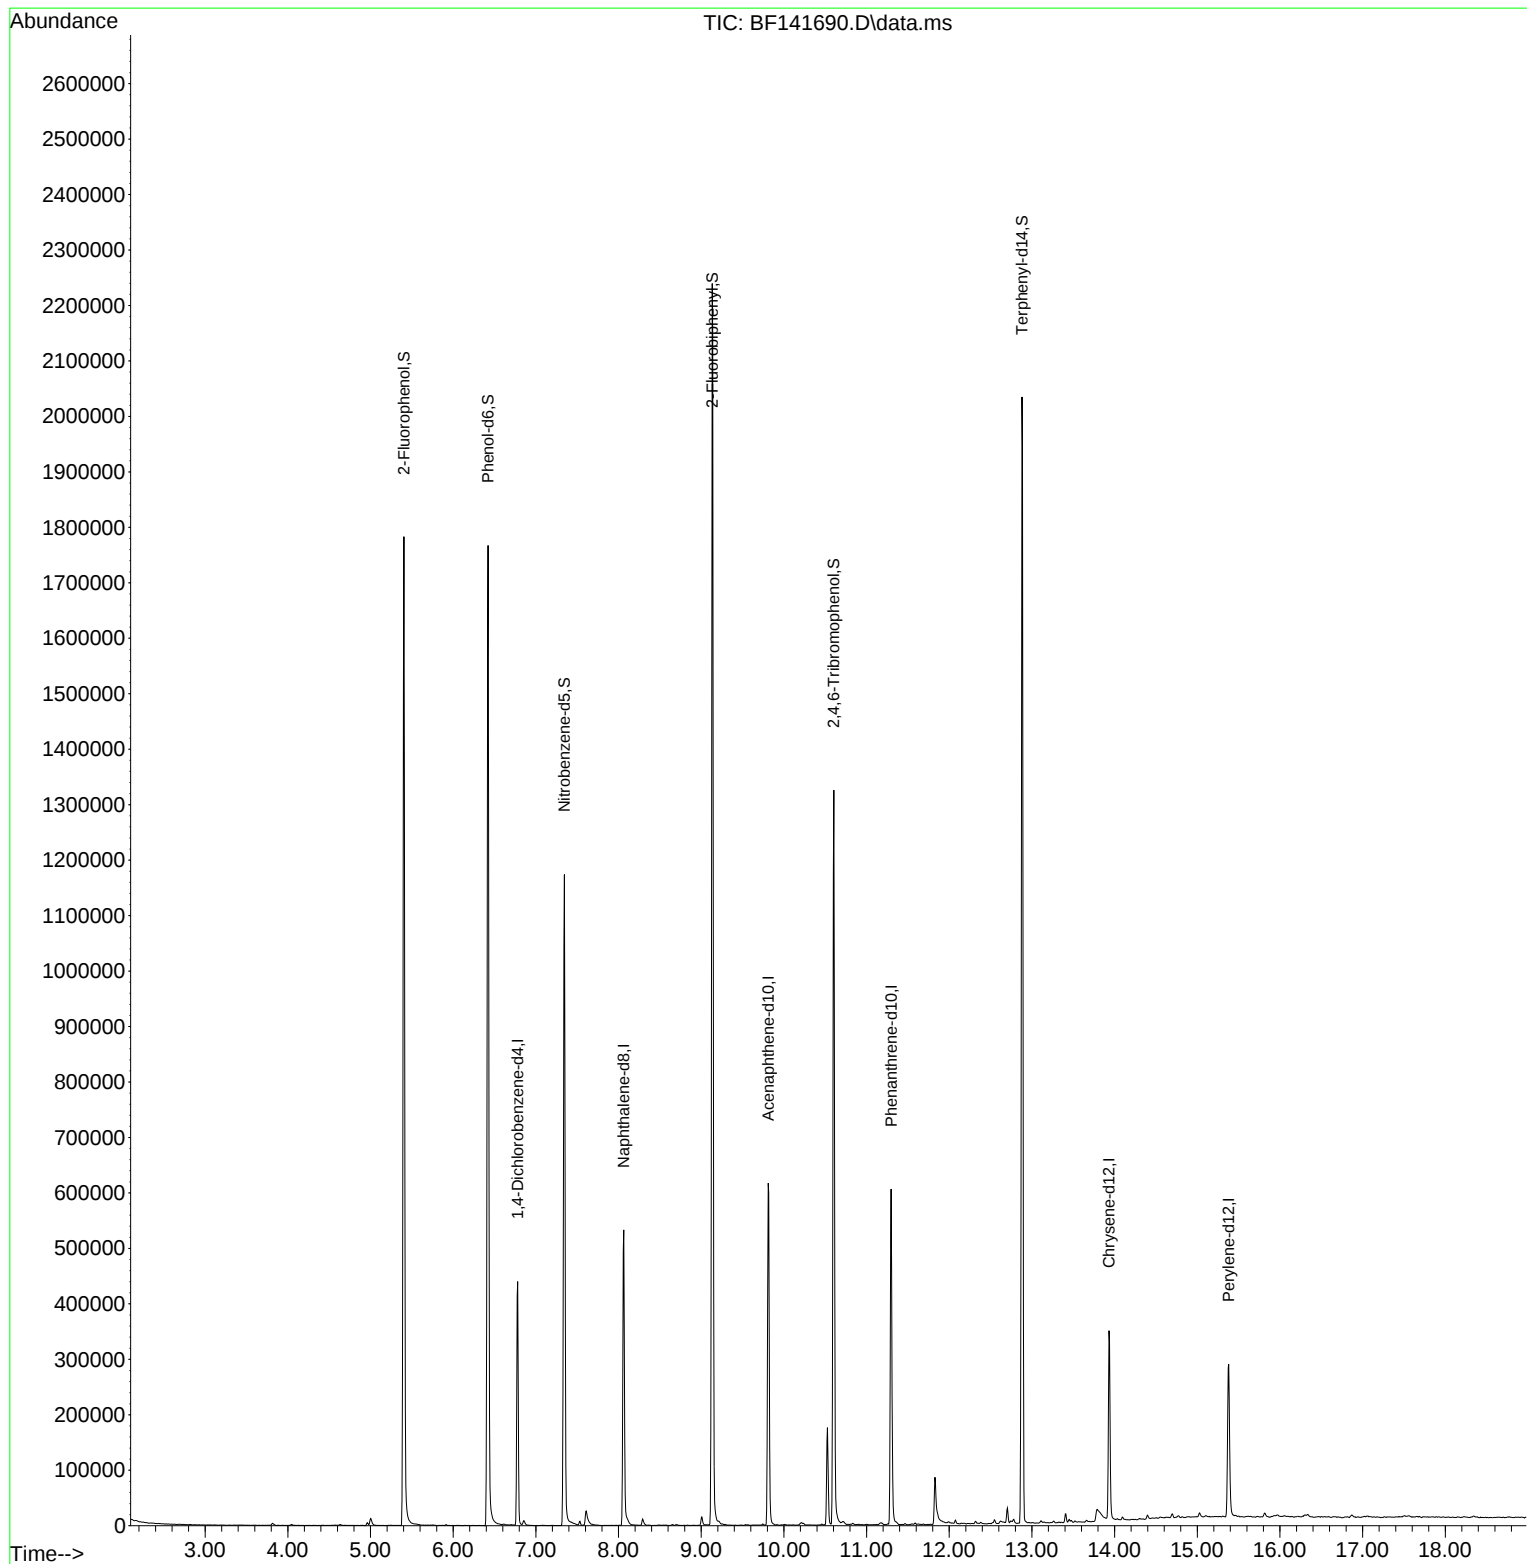




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.781 min Scan# 798
Delta R.T. -0.011 min
Lab File: BF141690.D
Acq: 19 Feb 2025 22:37




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-15-021725

Tgt Ion:152 Resp: 93977
Ion Ratio Lower Upper
152 100
150 155.2 125.0 187.4
115 63.4 53.6 80.4

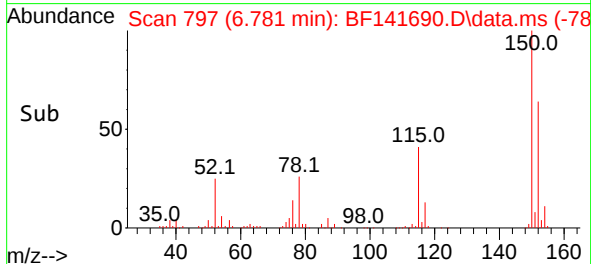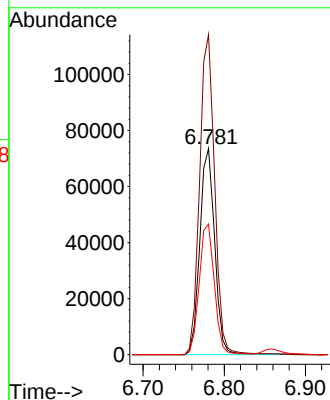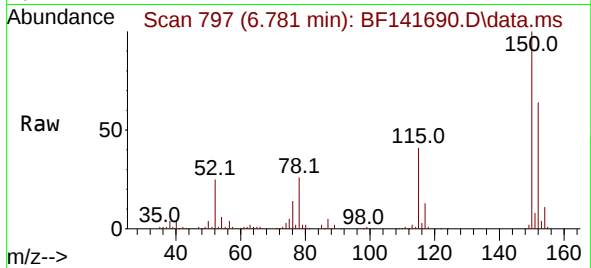

#5
2-Fluorophenol
Concen: 112.360 ng
RT: 5.404 min Scan# 563
Delta R.T. -0.006 min
Lab File: BF141690.D
Acq: 19 Feb 2025 22:37

Tgt Ion:112 Resp: 673535
Ion Ratio Lower Upper
112 100
64 61.1 51.1 76.7
63 32.9 28.4 42.6


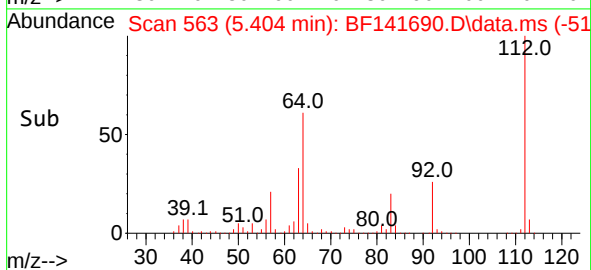
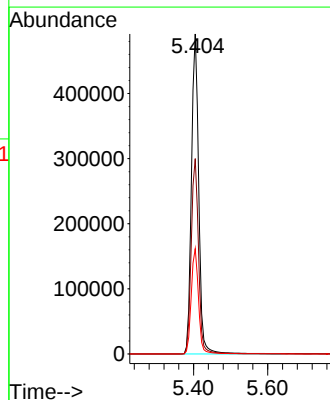
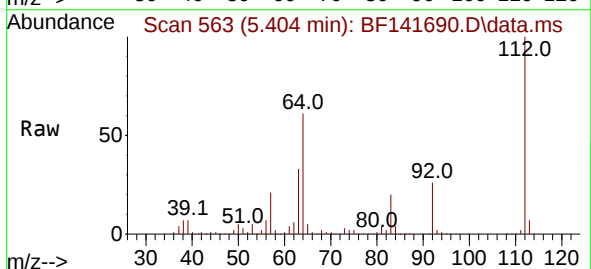




#7
Phenol-d6
Concen: 110.822 ng
RT: 6.422 min Scan# 71
Delta R.T. -0.018 min
Lab File: BF141690.D
Acq: 19 Feb 2025 22:37




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-15-021725

Tgt Ion: 99 Resp: 839637
Ion Ratio Lower Upper
99 100
42 20.9 19.1 28.7
71 36.6 31.1 46.7

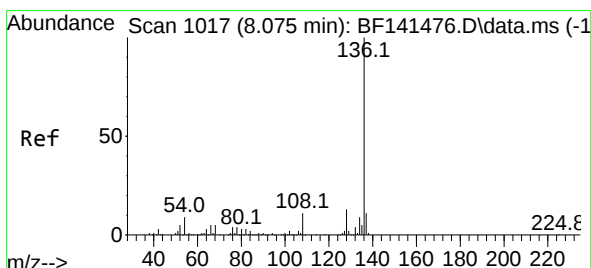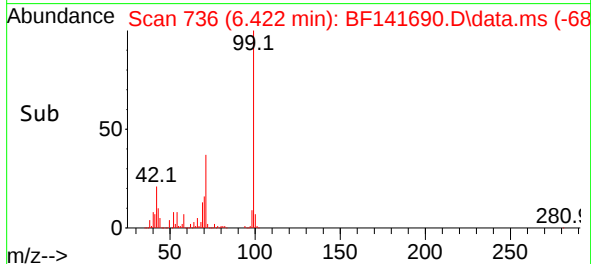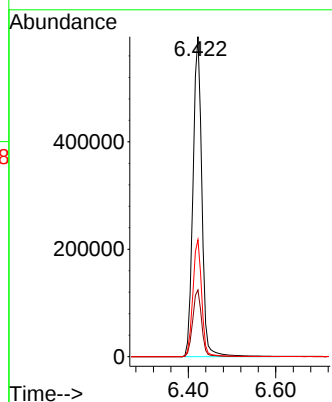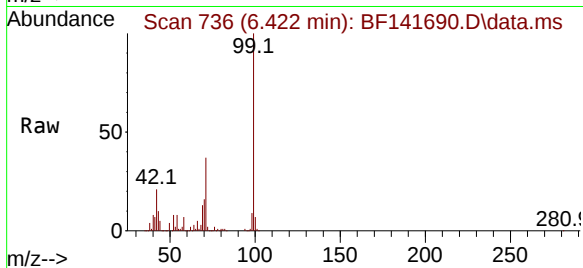

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.063 min Scan# 1015
Delta R.T. -0.012 min
Lab File: BF141690.D
Acq: 19 Feb 2025 22:37

Tgt Ion: 136 Resp: 374022
Ion Ratio Lower Upper
136 100
137 10.5 8.6 13.0
54 8.4 7.2 10.8
68 4.6 3.7 5.5


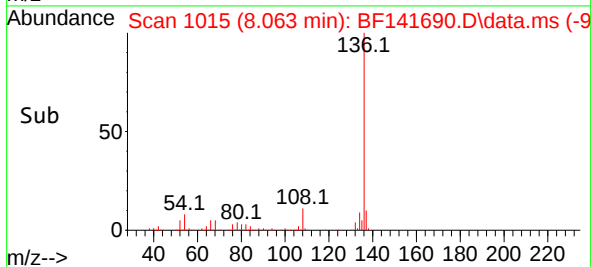
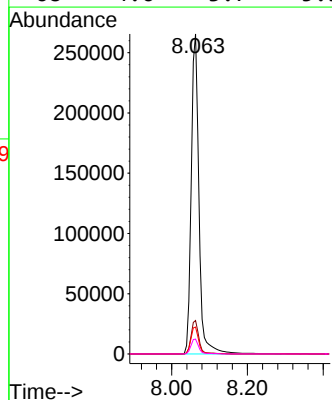
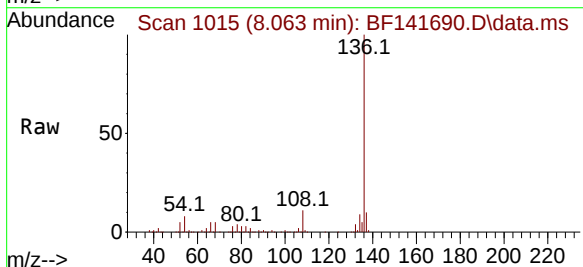




#23
Nitrobenzene-d5
Concen: 76.298 ng
RT: 7.345 min Scan# 89
Delta R.T. -0.018 min
Lab File: BF141690.D
Acq: 19 Feb 2025 22:37




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-15-021725

Tgt Ion: 82 Resp: 547127
Ion Ratio Lower Upper
82 100
128 45.2 34.8 52.2
54 56.3 48.2 72.4

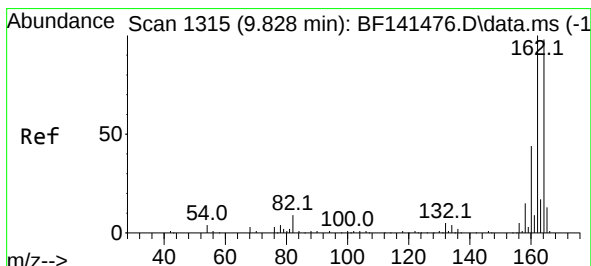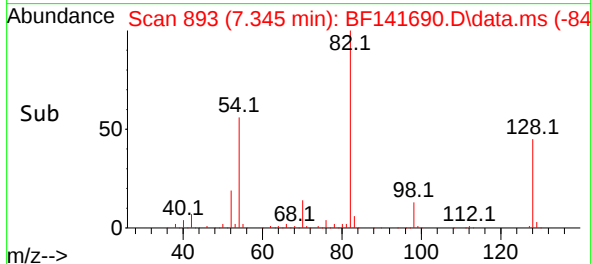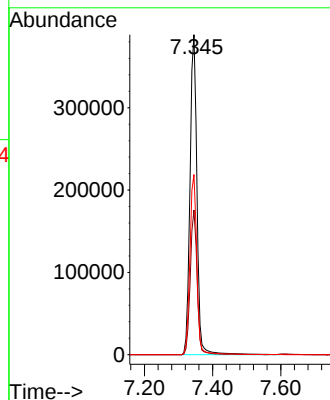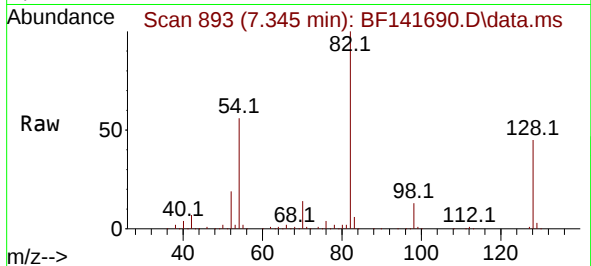

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.810 min Scan# 1312
Delta R.T. -0.024 min
Lab File: BF141690.D
Acq: 19 Feb 2025 22:37

Tgt Ion:164 Resp: 200098
Ion Ratio Lower Upper
164 100
162 102.9 81.3 121.9
160 45.4 35.9 53.9

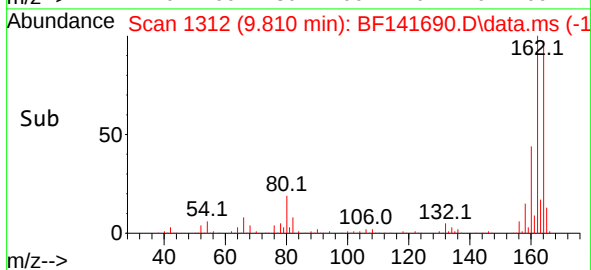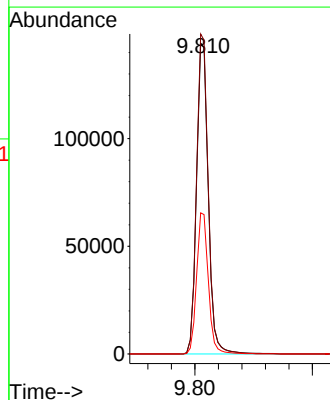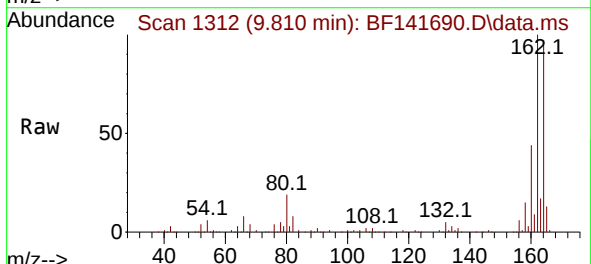



#42

2,4,6-Tribromophenol

Concen: 112.049 ng

RT: 10.604 min Scan# 1447

Delta R.T. -0.024 min

Lab File: BF141690.D


Acq: 19 Feb 2025 22:37

Instrument :

BNA_F

ClientSampleId :

OU4-PCS-TC-15-021725

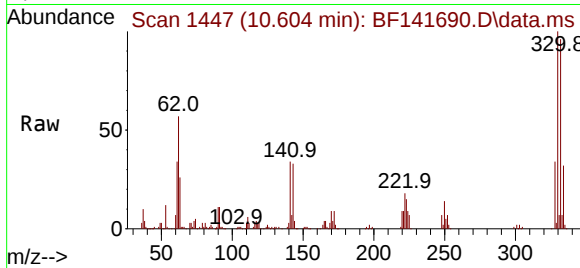



Tgt Ion:330 Resp: 225226

Ion Ratio Lower Upper

330 100

332 95.7 78.5 117.7

141 35.3 31.0 46.4

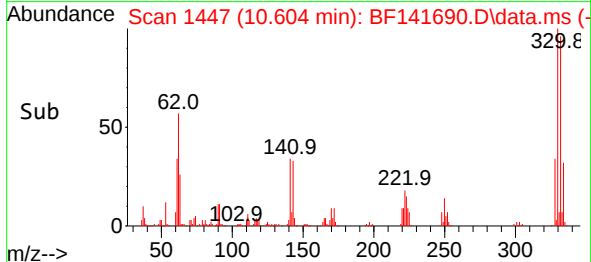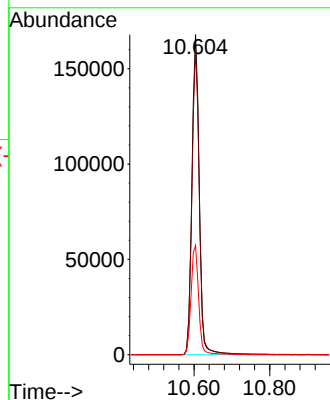

#45

2-Fluorobiphenyl

Concen: 80.228 ng

RT: 9.133 min Scan# 1197

Delta R.T. -0.018 min

Lab File: BF141690.D

Acq: 19 Feb 2025 22:37




Tgt Ion:172 Resp: 1041995

Ion Ratio Lower Upper

172 100

171 35.4 28.7 43.1

170 23.5 18.9 28.3

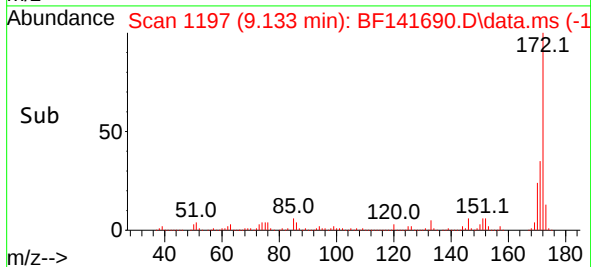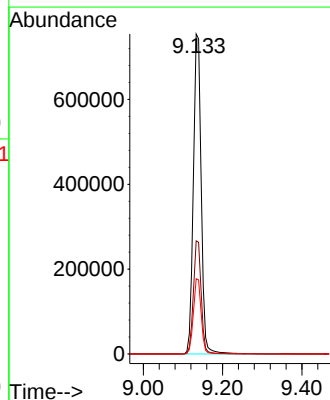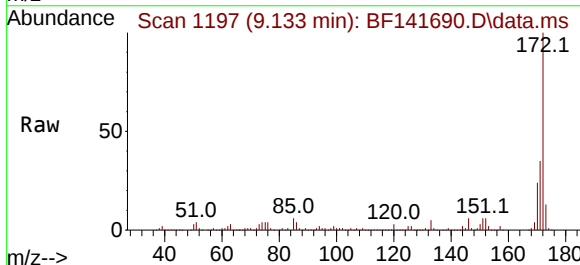



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.298 min Scan# 1

Delta R.T. -0.018 min

Lab File: BF141690.D

Acq: 19 Feb 2025 22:37

Instrument :

BNA_F

ClientSampleId :

OU4-PCS-TC-15-021725





Tgt Ion:188 Resp: 336579

Ion Ratio Lower Upper

188 100

94 8.4 6.6 10.0

80 9.3 7.3 10.9

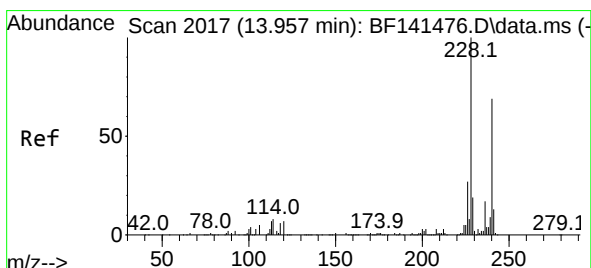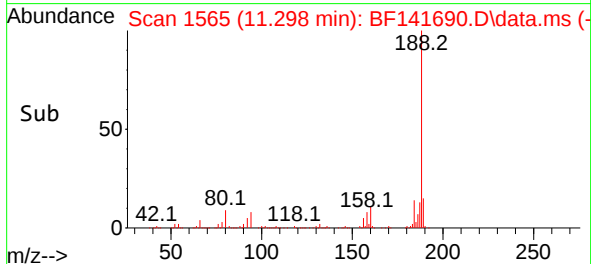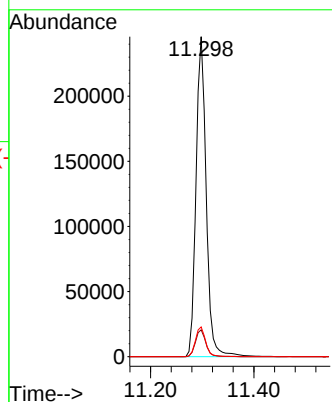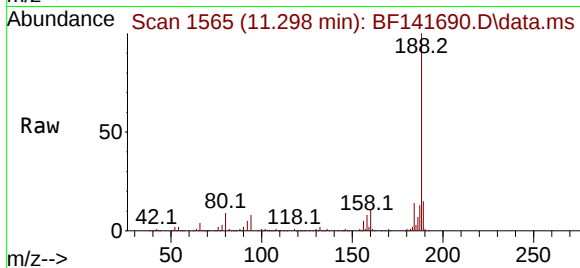

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.933 min Scan# 2013

Delta R.T. -0.029 min

Lab File: BF141690.D

Acq: 19 Feb 2025 22:37




Tgt Ion:240 Resp: 182552


Ion Ratio Lower Upper

240 100

120 10.7 8.0 12.0

236 25.1 19.8 29.8


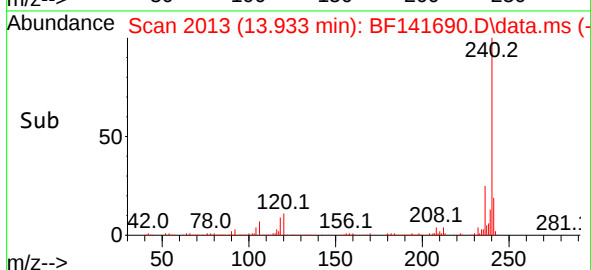
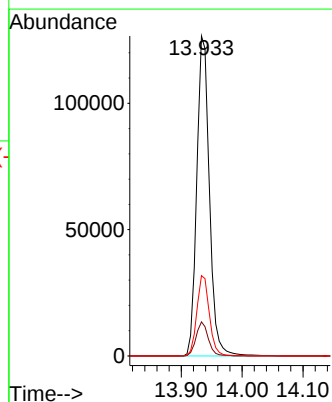
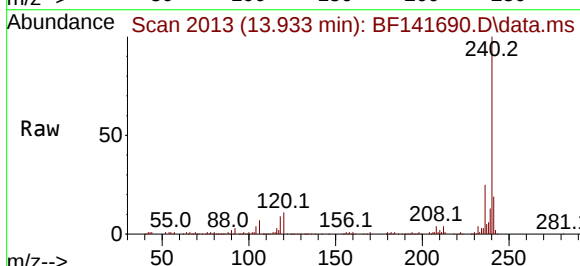


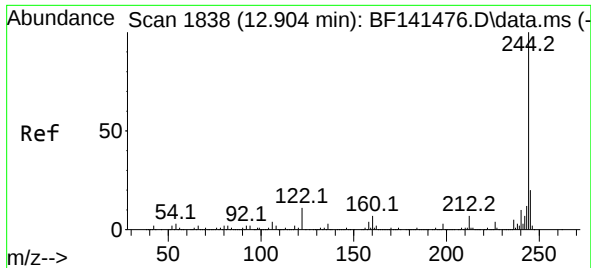

#79
 Terphenyl-d14
 Concen: 96.473 ng
 RT: 12.880 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: BF141690.D
 Acq: 19 Feb 2025 22:37

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-15-021725

Tgt Ion:244 Resp: 1043224
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.6 8.4
 122 11.2 8.4 12.6

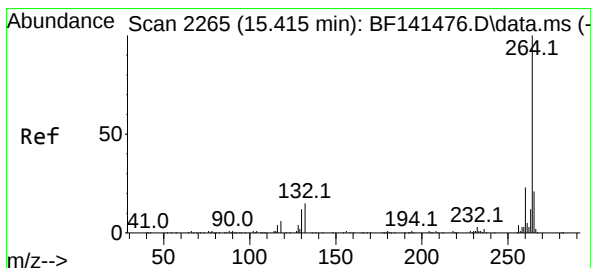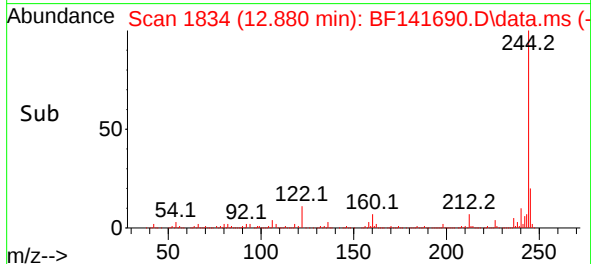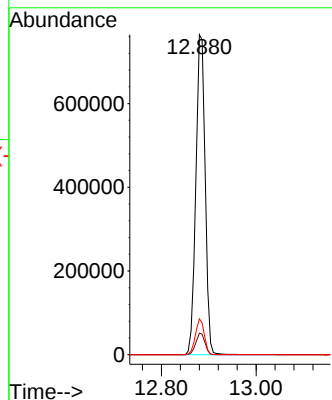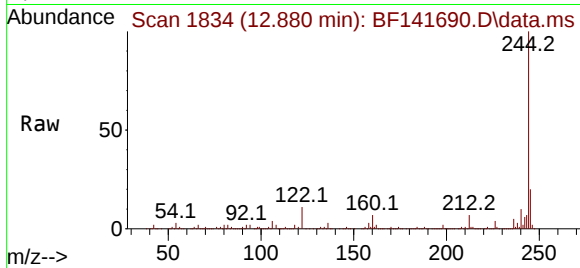

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.380 min Scan# 2259
 Delta R.T. -0.035 min
 Lab File: BF141690.D
 Acq: 19 Feb 2025 22:37

Tgt Ion:264 Resp: 183803
 Ion Ratio Lower Upper
 264 100
 260 23.2 18.6 28.0
 265 21.2 17.0 25.4

