

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
 Data File : BF141702.D
 Acq On : 20 Feb 2025 14:36
 Operator : RC/JU
 Sample : Q1383-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-18-021725

Quant Time: Feb 20 14:56:41 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 06 16:58:59 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.775	152	84665	20.000	ng	-0.02
21) Naphthalene-d8	8.063	136	329153	20.000	ng	-0.01
39) Acenaphthene-d10	9.810	164	174135	20.000	ng	-0.02
64) Phenanthrene-d10	11.298	188	300993	20.000	ng	-0.02
76) Chrysene-d12	13.933	240	190107	20.000	ng	-0.03
86) Perylene-d12	15.374	264	159816	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.399	112	479827	88.850	ng	-0.01
7) Phenol-d6	6.416	99	599553	87.837	ng	-0.02
23) Nitrobenzene-d5	7.340	82	380295	60.262	ng	-0.02
42) 2,4,6-Tribromophenol	10.604	330	149623	85.535	ng	-0.02
45) 2-Fluorobiphenyl	9.134	172	718368	63.557	ng	-0.02
79) Terphenyl-d14	12.880	244	778501	69.132	ng	-0.02


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141702.D
Acq On : 20 Feb 2025 14:36
Operator : RC/JU
Sample : Q1383-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-18-021725

Quant Time: Feb 20 14:56:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration



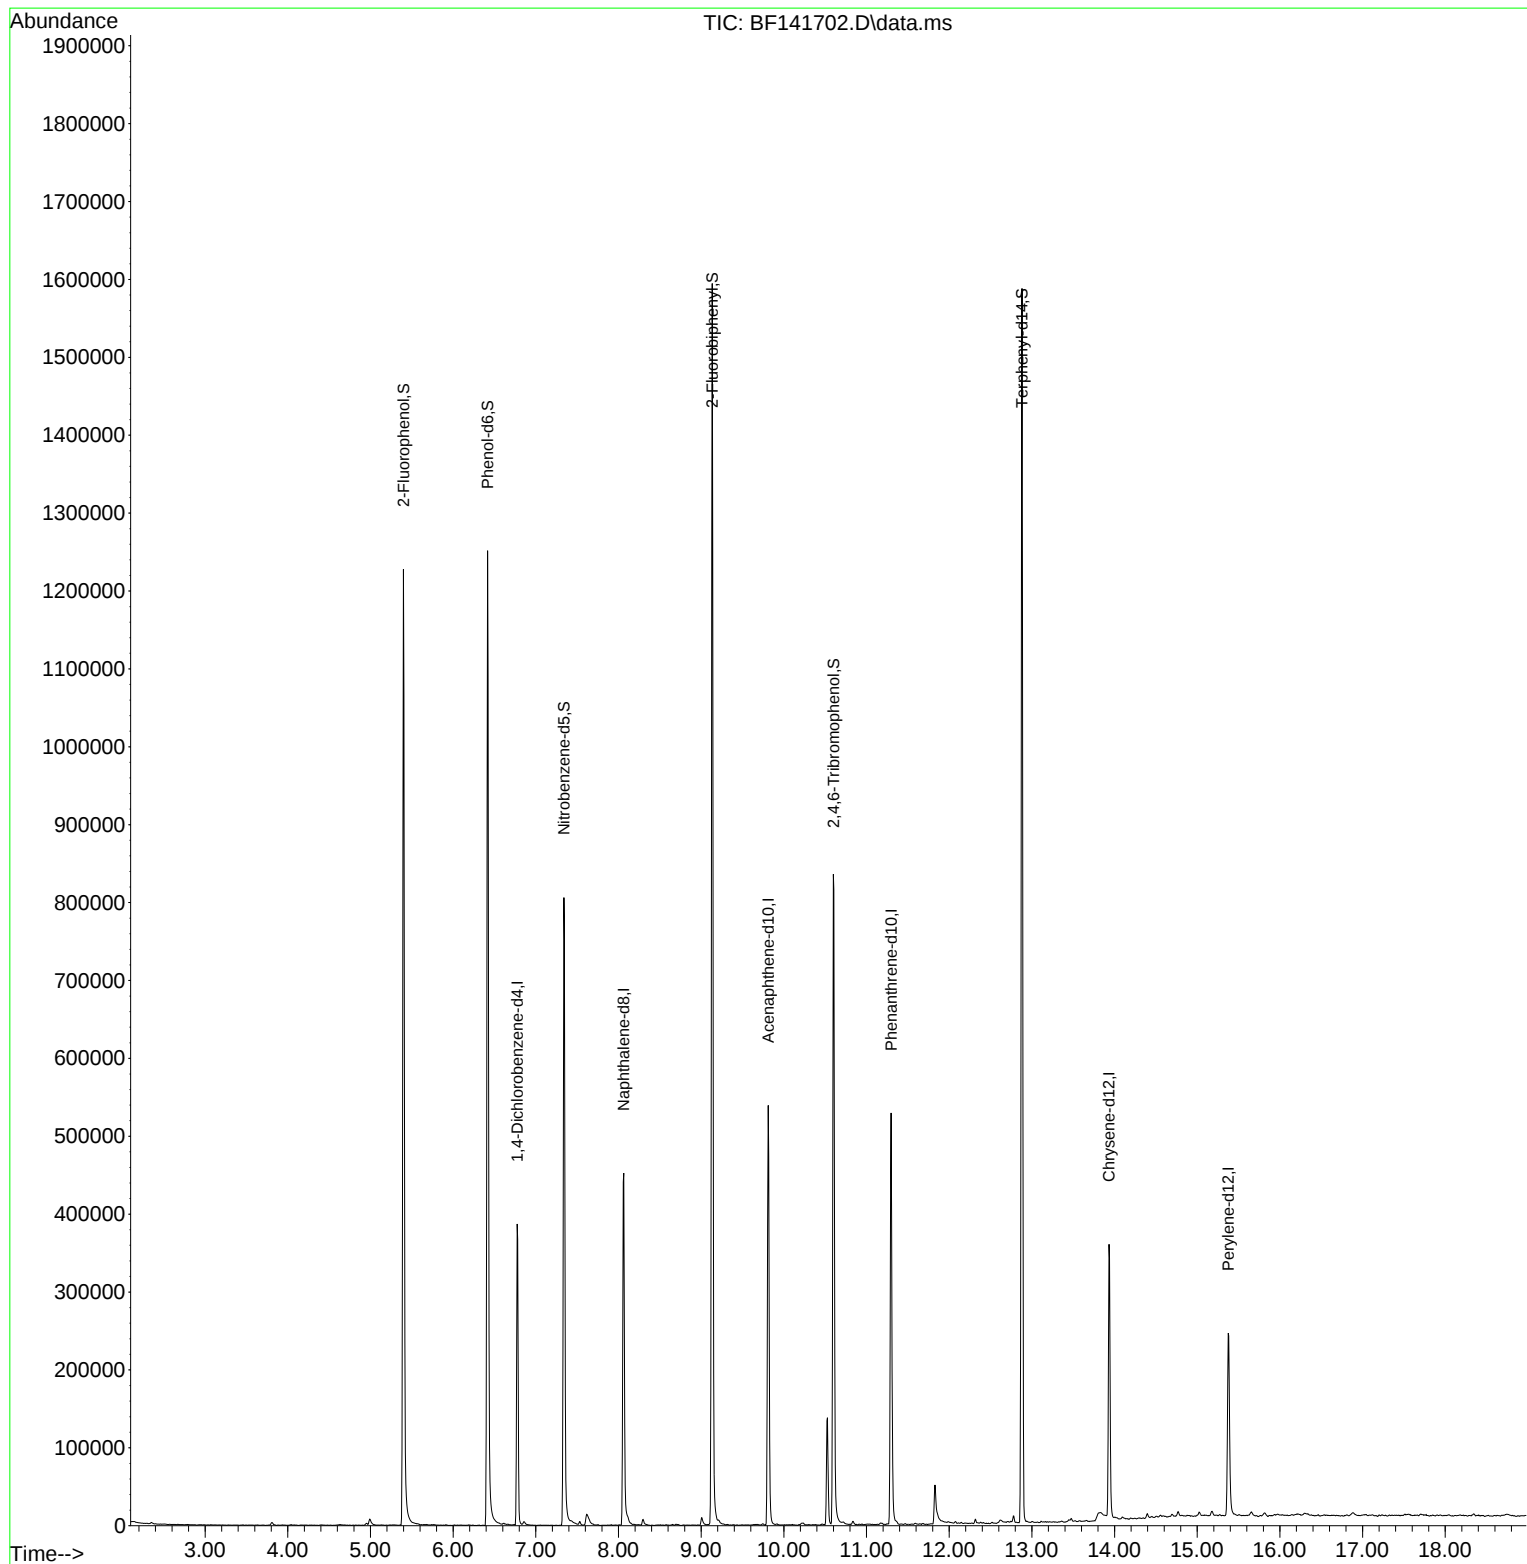


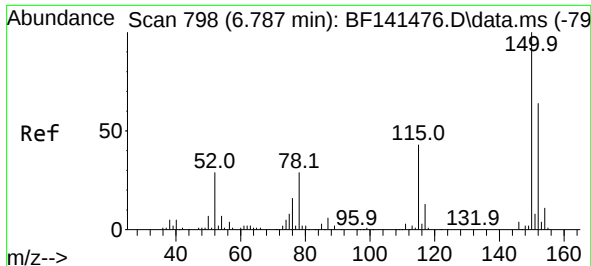

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.775 min Scan# 798
Delta R.T. -0.017 min
Lab File: BF141702.D
Acq: 20 Feb 2025 14:36




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-18-021725

Tgt Ion:152 Resp: 84665
Ion Ratio Lower Upper
152 100
150 155.1 125.0 187.4
115 64.4 53.6 80.4

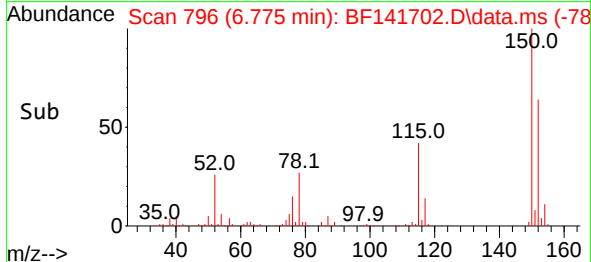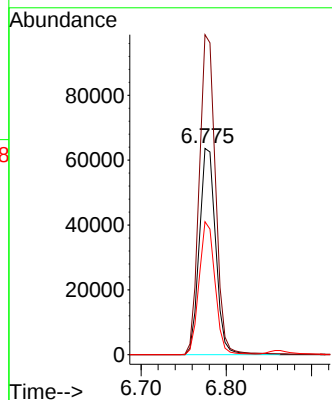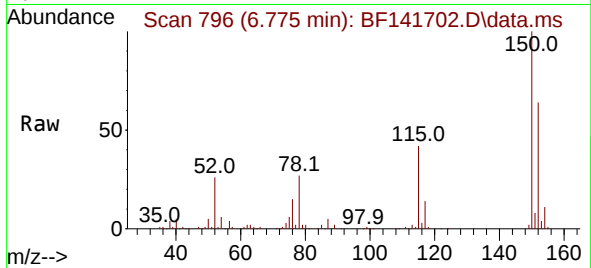

#5
2-Fluorophenol
Concen: 88.850 ng
RT: 5.399 min Scan# 562
Delta R.T. -0.012 min
Lab File: BF141702.D
Acq: 20 Feb 2025 14:36

Tgt Ion:112 Resp: 479827
Ion Ratio Lower Upper
112 100
64 61.2 51.1 76.7
63 33.0 28.4 42.6

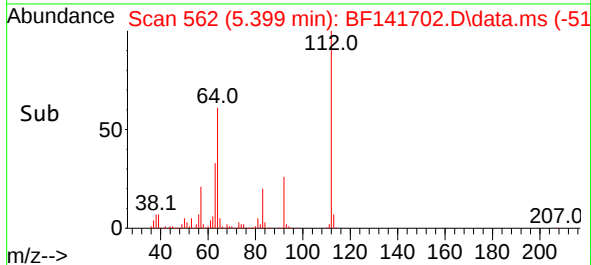
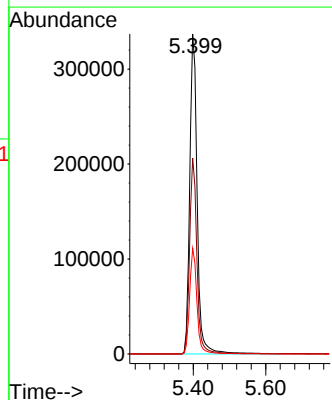
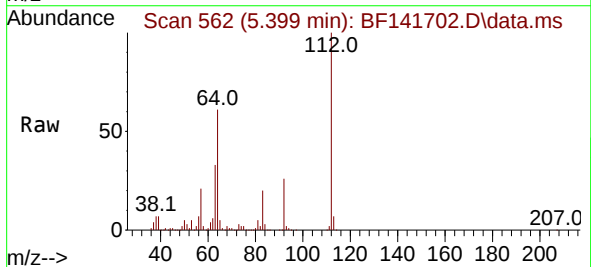




#7
Phenol-d6
Concen: 87.837 ng
RT: 6.416 min Scan# 71
Delta R.T. -0.023 min
Lab File: BF141702.D
Acq: 20 Feb 2025 14:36




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-18-021725

Tgt Ion: 99 Resp: 599553
Ion Ratio Lower Upper
99 100
42 21.1 19.1 28.7
71 36.3 31.1 46.7

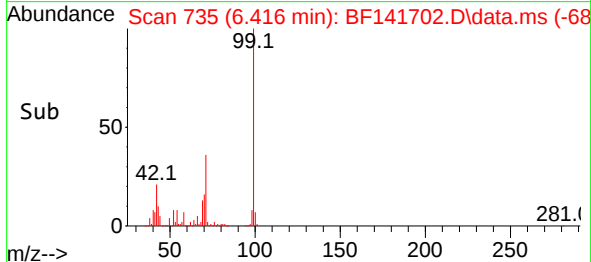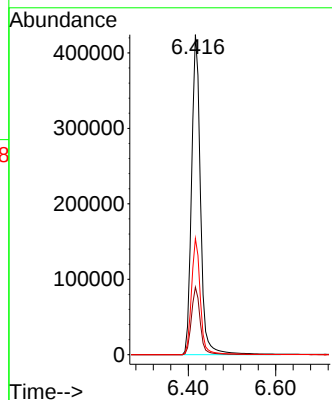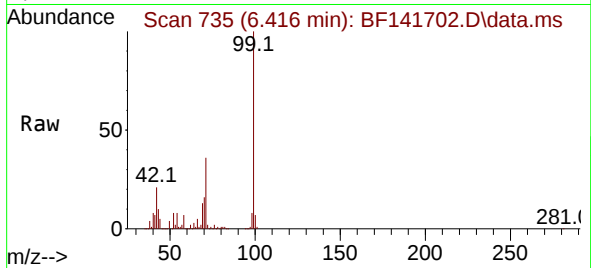

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.063 min Scan# 1015
Delta R.T. -0.012 min
Lab File: BF141702.D
Acq: 20 Feb 2025 14:36

Tgt Ion: 136 Resp: 329153
Ion Ratio Lower Upper
136 100
137 10.7 8.6 13.0
54 8.6 7.2 10.8
68 4.7 3.7 5.5

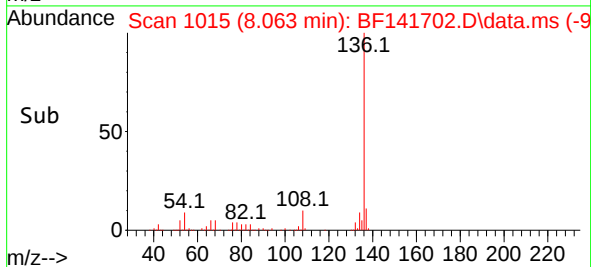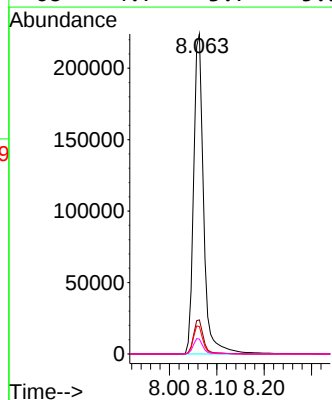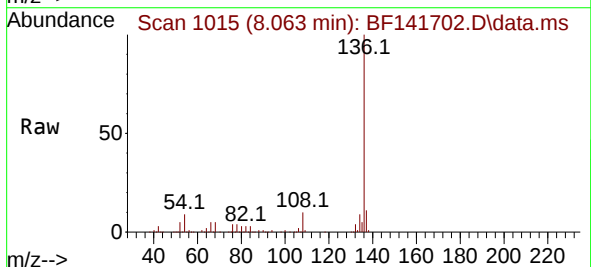



#23

Nitrobenzene-d5

Concen: 60.262 ng

RT: 7.340 min Scan# 895

Delta R.T. -0.023 min

Lab File: BF141702.D

Acq: 20 Feb 2025 14:36

Instrument :

BNA_F

ClientSampleId :

OU4-PCS-TC-18-021725





Tgt Ion: 82 Resp: 380295

Ion Ratio Lower Upper

82 100

128 43.7 34.8 52.2

54 57.4 48.2 72.4

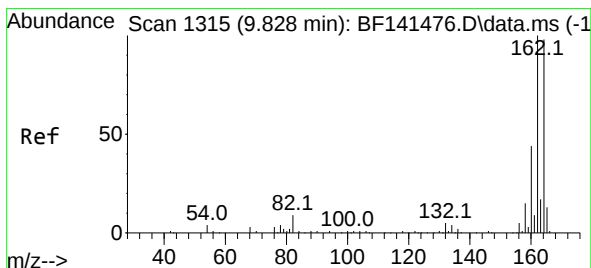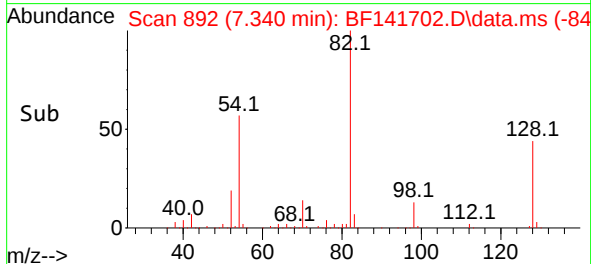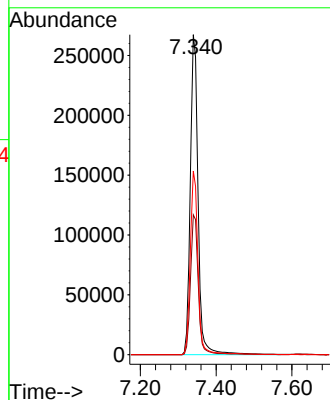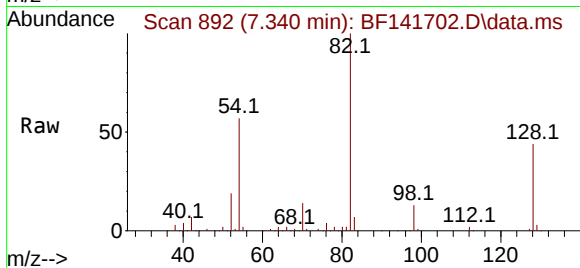

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.810 min Scan# 1312

Delta R.T. -0.023 min

Lab File: BF141702.D

Acq: 20 Feb 2025 14:36




Tgt Ion:164 Resp: 174135

Ion Ratio Lower Upper

164 100

162 102.7 81.3 121.9

160 45.5 35.9 53.9

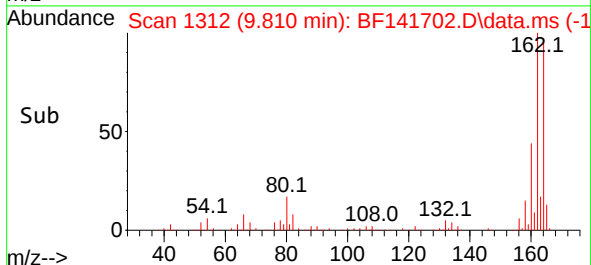
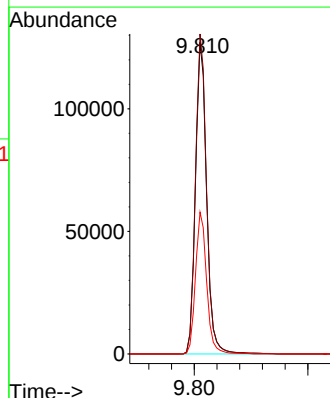
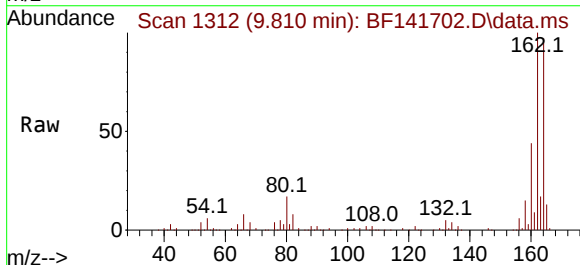




#42
2,4,6-Tribromophenol
Concen: 85.535 ng
RT: 10.604 min Scan# 1450
Delta R.T. -0.023 min
Lab File: BF141702.D
Acq: 20 Feb 2025 14:36




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-18-021725

Tgt Ion:330 Resp: 149623
Ion Ratio Lower Upper
330 100
332 96.1 78.5 117.7
141 35.2 31.0 46.4

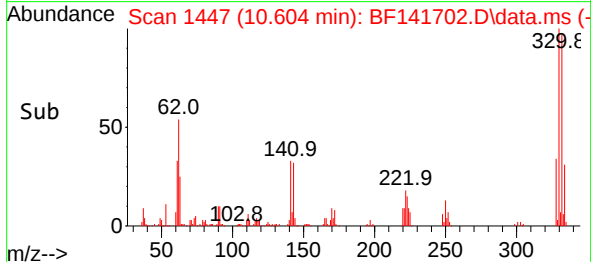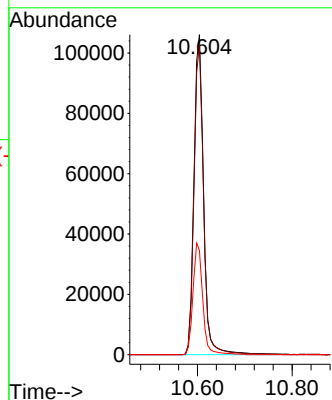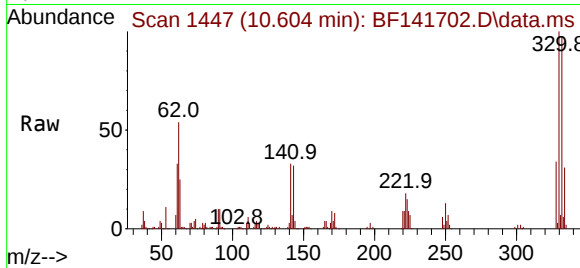

#45
2-Fluorobiphenyl
Concen: 63.557 ng
RT: 9.134 min Scan# 1197
Delta R.T. -0.017 min
Lab File: BF141702.D
Acq: 20 Feb 2025 14:36

Tgt Ion:172 Resp: 718368
Ion Ratio Lower Upper
172 100
171 35.4 28.7 43.1
170 23.0 18.9 28.3


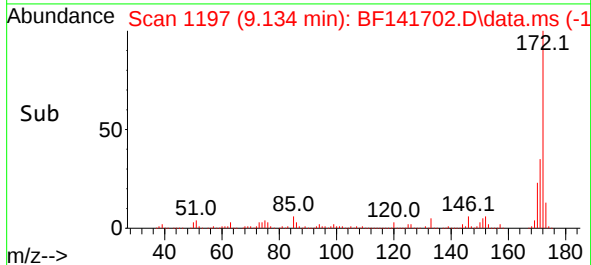
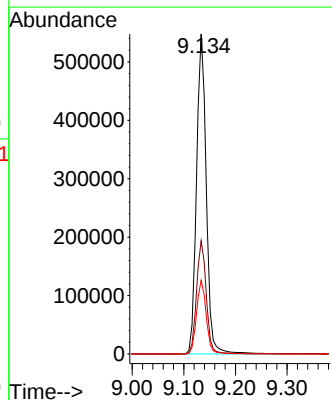
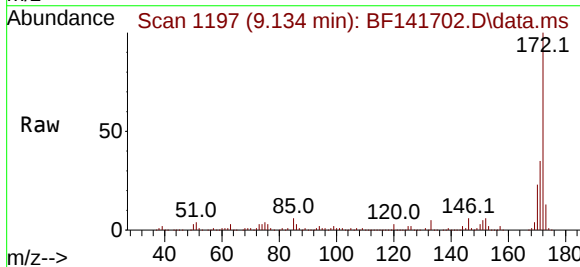




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.298 min Scan# 11
Delta R.T. -0.017 min
Lab File: BF141702.D
Acq: 20 Feb 2025 14:36




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-18-021725


Tgt Ion:188 Resp: 300993
Ion Ratio Lower Upper
188 100
94 8.6 6.6 10.0
80 8.8 7.3 10.9

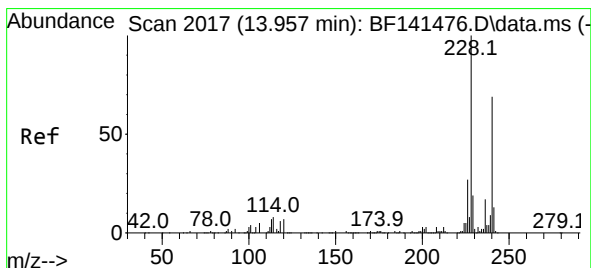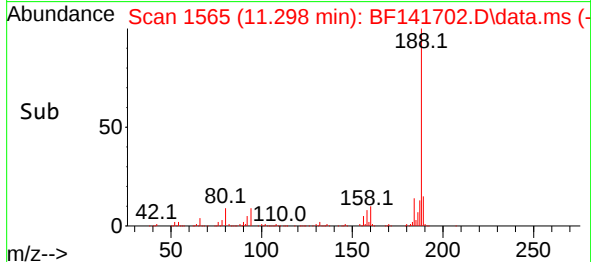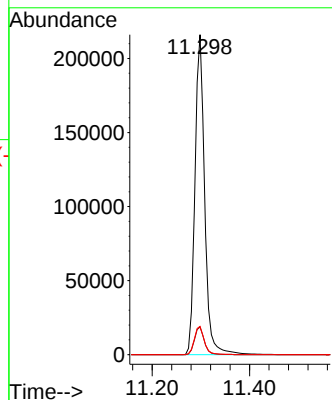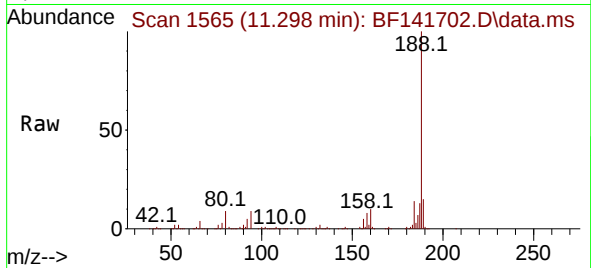

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.933 min Scan# 2013
Delta R.T. -0.029 min
Lab File: BF141702.D
Acq: 20 Feb 2025 14:36


Tgt Ion:240 Resp: 190107
Ion Ratio Lower Upper
240 100
120 10.7 8.0 12.0
236 25.2 19.8 29.8

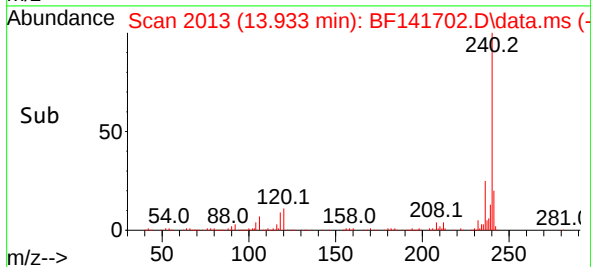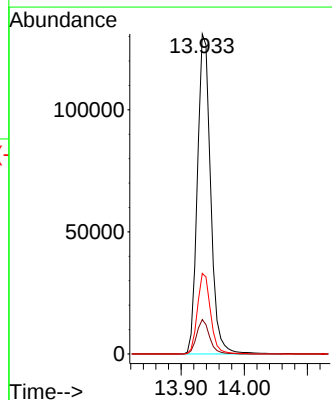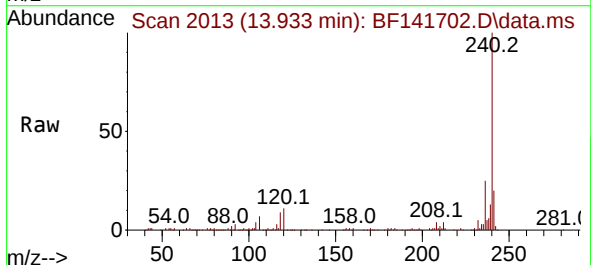



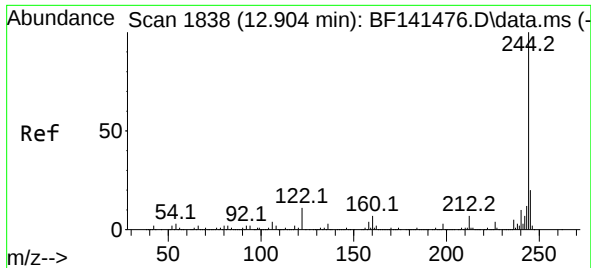


#79
 Terphenyl-d14
 Concen: 69.132 ng
 RT: 12.880 min Scan# 11
 Delta R.T. -0.023 min
 Lab File: BF141702.D
 Acq: 20 Feb 2025 14:36

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-18-021725

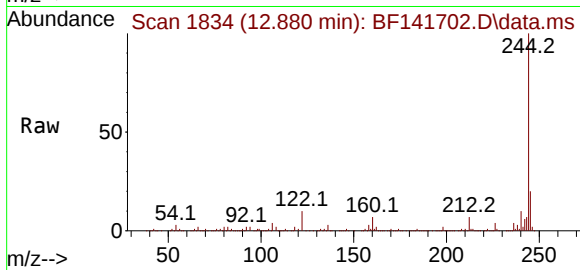

Tgt Ion:244 Resp: 778501
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.6 8.4
 122 10.4 8.4 12.6

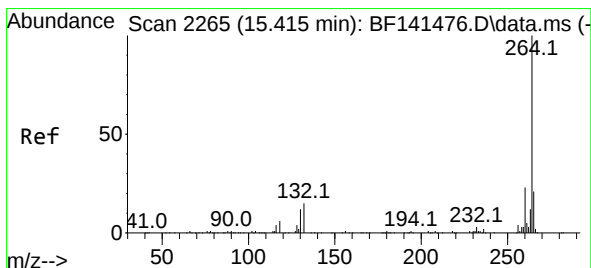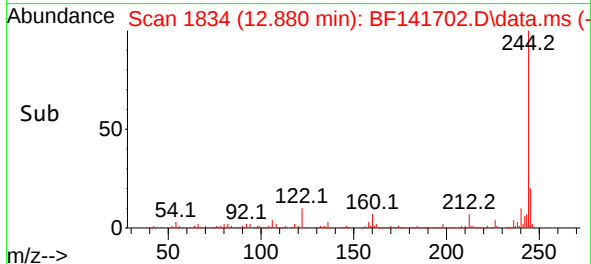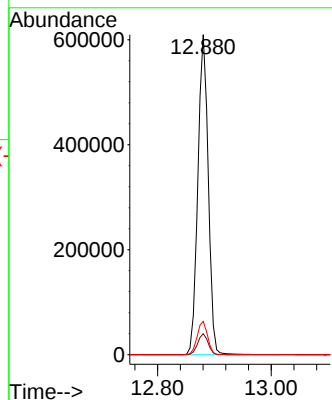

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.374 min Scan# 2258
 Delta R.T. -0.041 min
 Lab File: BF141702.D
 Acq: 20 Feb 2025 14:36

Tgt Ion:264 Resp: 159816
 Ion Ratio Lower Upper
 264 100
 260 22.9 18.6 28.0
 265 21.9 17.0 25.4

