

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
 Data File : BF141686.D  
 Acq On : 19 Feb 2025 20:39  
 Operator : RC/JU  
 Sample : Q1383-01  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 OU4-PCS-TC-11-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141686.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.404       | 557           | 563         | 587          | rBV      | 1176160        | 1660890       | 77.08%          | 12.204%       |
| 2         | 6.416       | 730           | 735         | 763          | rBV      | 1176469        | 1693077       | 78.58%          | 12.440%       |
| 3         | 6.781       | 791           | 797         | 805          | rBV      | 409859         | 528005        | 24.50%          | 3.880%        |
| 4         | 7.339       | 887           | 892         | 905          | rBV      | 774359         | 1095433       | 50.84%          | 8.049%        |
| 5         | 7.610       | 933           | 938         | 950          | rBV2     | 11703          | 32053         | 1.49%           | 0.236%        |
| 6         | 8.063       | 1009          | 1015        | 1033         | rBV      | 495452         | 707583        | 32.84%          | 5.199%        |
| 7         | 9.004       | 1170          | 1175        | 1185         | rBV      | 47090          | 66481         | 3.09%           | 0.488%        |
| 8         | 9.133       | 1190          | 1197        | 1215         | rVV      | 1613695        | 2154703       | 100.00%         | 15.832%       |
| 9         | 9.810       | 1307          | 1312        | 1329         | rBV      | 577894         | 793400        | 36.82%          | 5.830%        |
| 10        | 10.528      | 1429          | 1434        | 1441         | rBV      | 242786         | 309771        | 14.38%          | 2.276%        |
| 11        | 10.604      | 1441          | 1447        | 1463         | rVV      | 826739         | 1129409       | 52.42%          | 8.298%        |
| 12        | 11.298      | 1560          | 1565        | 1583         | rVB      | 566078         | 773632        | 35.90%          | 5.684%        |
| 13        | 11.827      | 1650          | 1655        | 1659         | rBV2     | 17447          | 30210         | 1.40%           | 0.222%        |
| 14        | 12.880      | 1828          | 1834        | 1842         | rBV      | 1368391        | 1735478       | 80.54%          | 12.752%       |
| 15        | 13.933      | 2008          | 2013        | 2024         | rVB      | 309490         | 444826        | 20.64%          | 3.268%        |
| 16        | 15.380      | 2252          | 2259        | 2274         | rBV      | 259841         | 454933        | 21.11%          | 3.343%        |




Sum of corrected areas: 13609884

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141686.D  
Acq On : 19 Feb 2025 20:39  
Operator : RC/JU  
Sample : Q1383-01  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-11-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

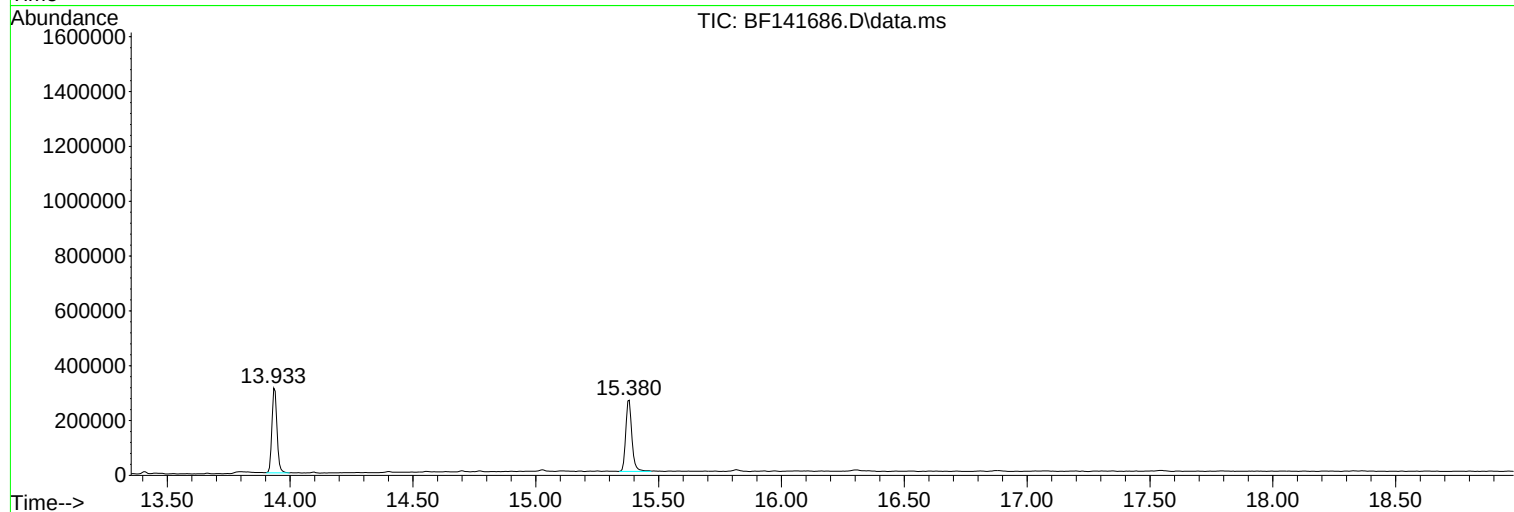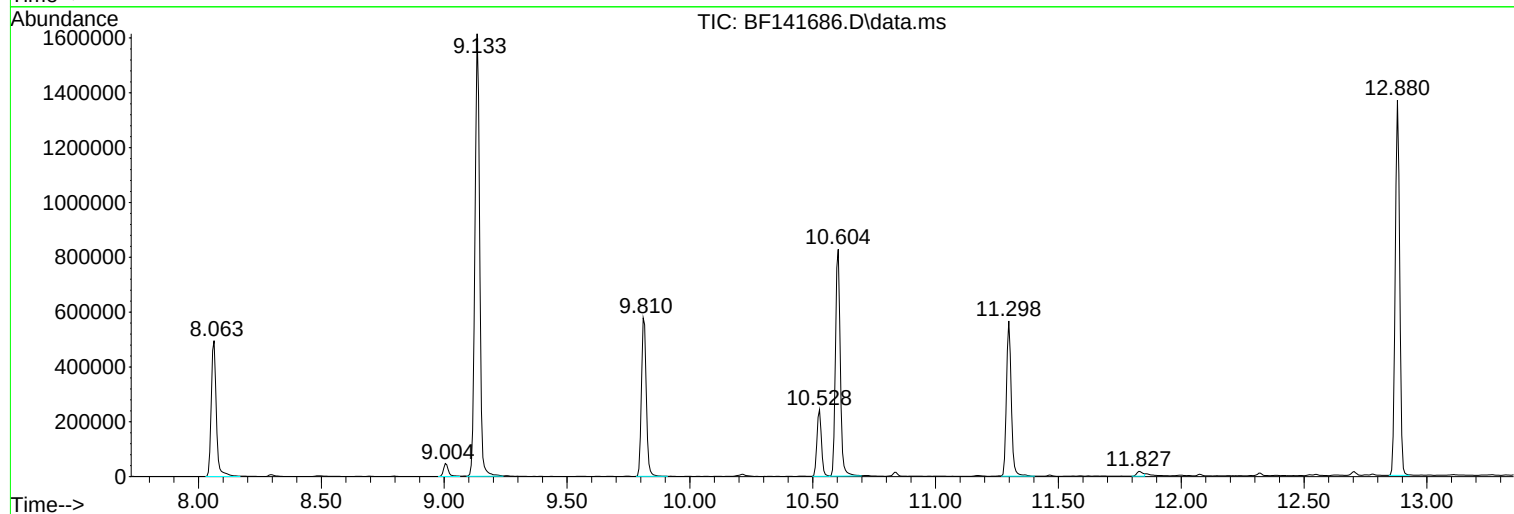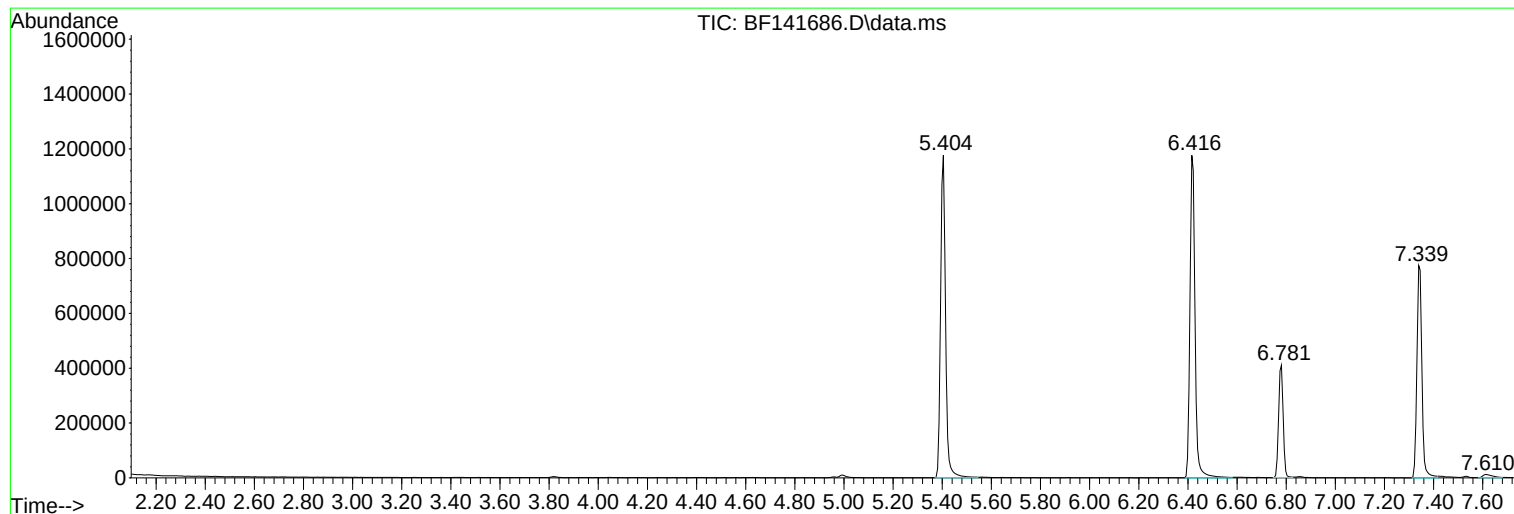

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141686.D  
Acq On : 19 Feb 2025 20:39  
Operator : RC/JU  
Sample : Q1383-01  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-11-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021925\  
Data File : BF141686.D  
Acq On : 19 Feb 2025 20:39  
Operator : RC/JU  
Sample : Q1383-01  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
OU4-PCS-TC-11-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----