

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
 Data File : BF141700.D
 Acq On : 20 Feb 2025 13:36
 Operator : RC/JU
 Sample : Q1383-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-16-021725

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.399	556	562	582	rBV	1047945	1489567	82.28%	11.950%
2	6.416	730	735	765	rBV	1084486	1550444	85.64%	12.439%
3	6.775	791	796	806	rBV	377997	492263	27.19%	3.949%
4	7.340	887	892	906	rBV	701726	975135	53.86%	7.823%
5	7.610	933	938	952	rBV	12900	35684	1.97%	0.286%
6	8.063	1009	1015	1041	rBV	443714	643112	35.52%	5.160%
7	9.134	1191	1197	1208	rBV	1394992	1805679	99.74%	14.486%
8	9.810	1307	1312	1328	rBV	521033	695553	38.42%	5.580%
9	10.528	1429	1434	1441	rBV	91361	124637	6.88%	1.000%
10	10.598	1441	1446	1464	rVV	735016	1035403	57.19%	8.307%
11	11.298	1559	1565	1585	rVB	494830	692120	38.23%	5.553%
12	11.828	1648	1655	1676	rBV2	83690	180722	9.98%	1.450%
13	12.616	1782	1789	1800	rBV5	12311	35127	1.94%	0.282%
14	12.880	1828	1834	1844	rBV	1415149	1810356	100.00%	14.524%
15	13.933	2006	2013	2023	rVB	360209	519564	28.70%	4.168%
16	15.374	2252	2258	2272	rVB	211676	379232	20.95%	3.042%




Sum of corrected areas: 12464598

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141700.D
Acq On : 20 Feb 2025 13:36
Operator : RC/JU
Sample : Q1383-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-16-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

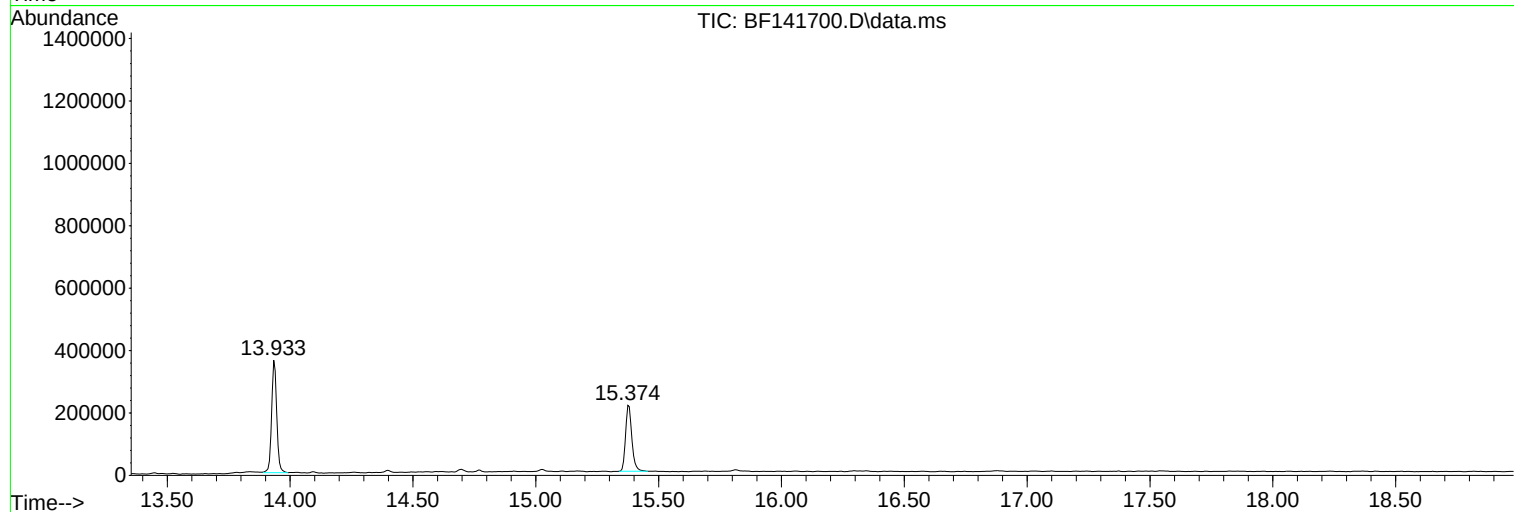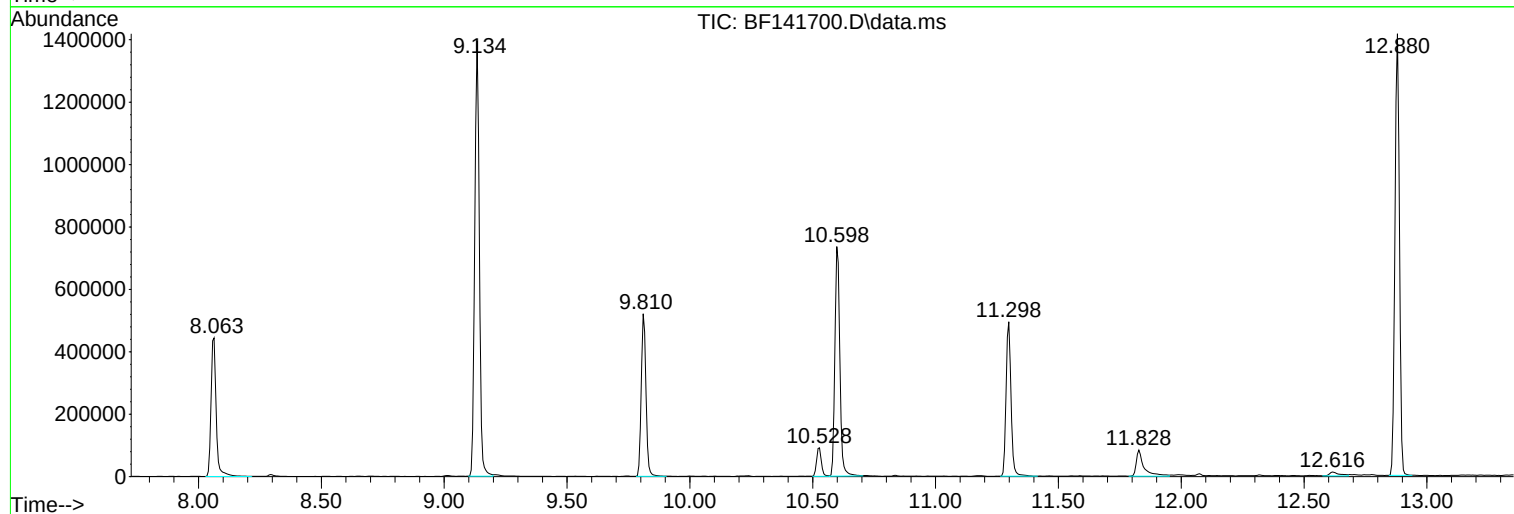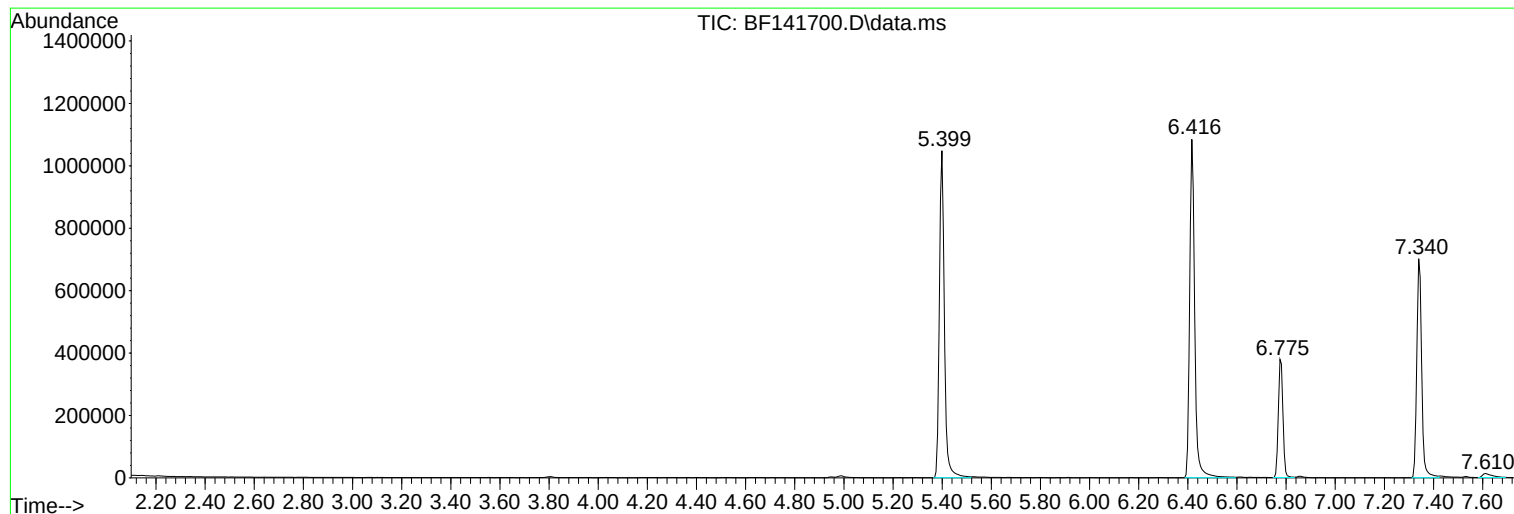

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141700.D
Acq On : 20 Feb 2025 13:36
Operator : RC/JU
Sample : Q1383-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-16-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141700.D
Acq On : 20 Feb 2025 13:36
Operator : RC/JU
Sample : Q1383-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-16-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------