

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
 Data File : BF141701.D
 Acq On : 20 Feb 2025 14:06
 Operator : RC/JU
 Sample : Q1383-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-17-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	557	562	587	rBV	1057050	1491178	82.67%	12.035%
2	6.416	730	735	761	rBV	1093966	1543536	85.57%	12.457%
3	6.775	791	796	806	rBV	374278	494220	27.40%	3.989%
4	7.339	887	892	907	rBV	692412	974262	54.01%	7.863%
5	7.628	935	941	958	rBV2	10297	33365	1.85%	0.269%
6	8.063	1009	1015	1038	rBV	442813	651378	36.11%	5.257%
7	9.133	1192	1197	1209	rBV	1386271	1803737	100.00%	14.558%
8	9.810	1307	1312	1333	rBV	515421	716234	39.71%	5.781%
9	10.527	1428	1434	1441	rBV	90876	123117	6.83%	0.994%
10	10.598	1441	1446	1463	rVV	701138	1019754	56.54%	8.230%
11	11.298	1559	1565	1584	rBV	514342	716421	39.72%	5.782%
12	11.827	1650	1655	1671	rBV2	34403	79590	4.41%	0.642%
13	12.880	1828	1834	1849	rBV	1414553	1801935	99.90%	14.543%
14	13.821	1984	1994	1996	rBV4	7688	21230	1.18%	0.171%
15	13.933	2008	2013	2025	rVB	357073	513964	28.49%	4.148%
16	15.380	2253	2259	2272	rBV	227512	406496	22.54%	3.281%




Sum of corrected areas: 12390417

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141701.D
Acq On : 20 Feb 2025 14:06
Operator : RC/JU
Sample : Q1383-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-17-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

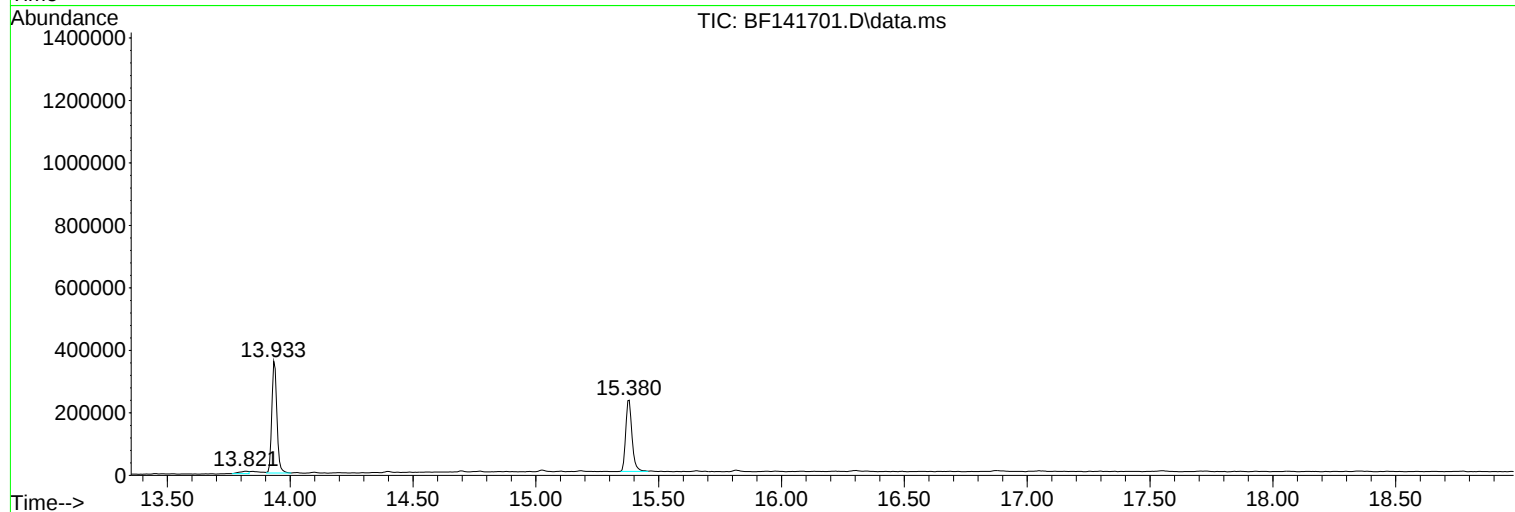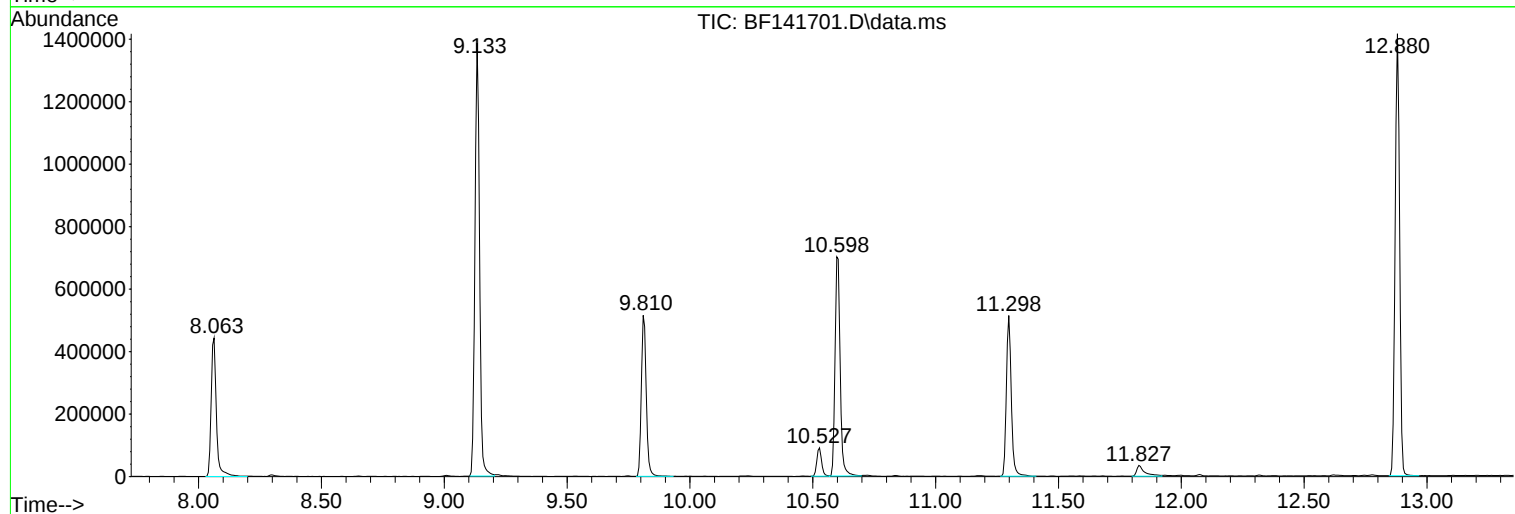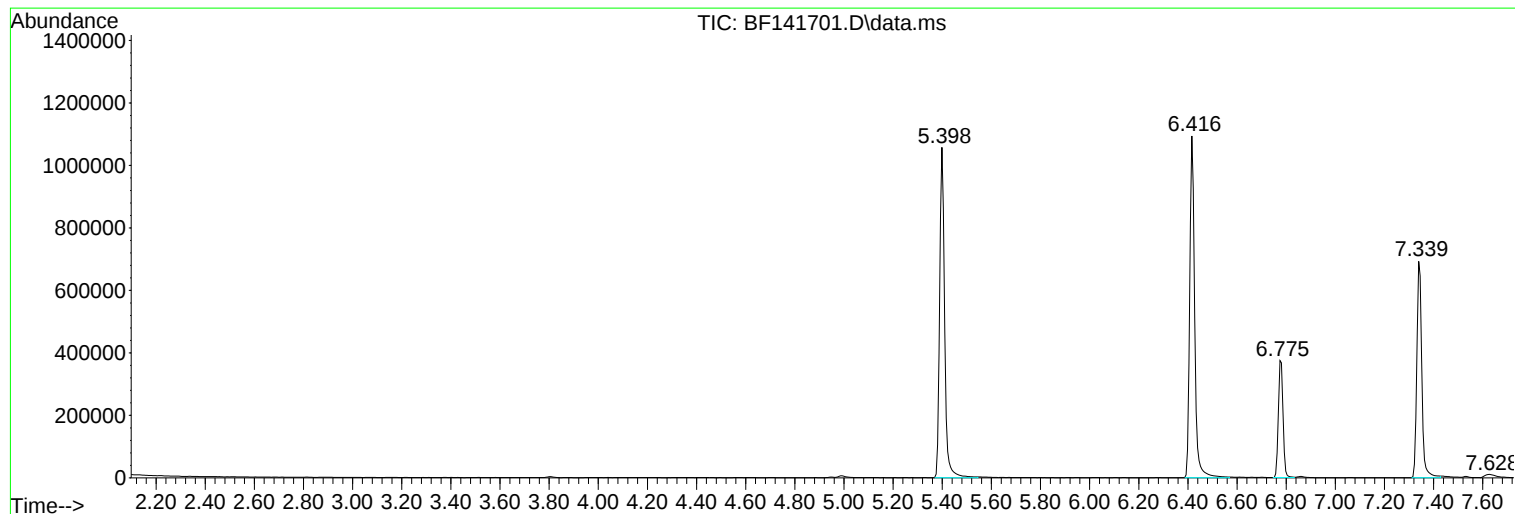

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141701.D
Acq On : 20 Feb 2025 14:06
Operator : RC/JU
Sample : Q1383-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-17-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141701.D
Acq On : 20 Feb 2025 14:06
Operator : RC/JU
Sample : Q1383-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-17-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------