

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
 Data File : BF141702.D
 Acq On : 20 Feb 2025 14:36
 Operator : RC/JU
 Sample : Q1383-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-18-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.399	557	562	596	rBV	1227264	1722934	83.00%	12.428%
2	6.416	730	735	758	rBV	1251440	1786377	86.06%	12.886%
3	6.775	792	796	805	rBV	386258	498460	24.01%	3.596%
4	7.340	887	892	921	rBV	805773	1138381	54.84%	8.212%
5	7.616	931	939	955	rBV3	13837	41691	2.01%	0.301%
6	8.063	1009	1015	1034	rBV	451904	660153	31.80%	4.762%
7	9.134	1191	1197	1208	rBV	1592808	2075764	100.00%	14.973%
8	9.810	1307	1312	1327	rBV	539059	731301	35.23%	5.275%
9	10.528	1429	1434	1441	rBV	137339	185338	8.93%	1.337%
10	10.598	1441	1446	1463	rVV	834118	1189765	57.32%	8.582%
11	11.298	1559	1565	1581	rVB	528102	730763	35.20%	5.271%
12	11.828	1650	1655	1676	rBV2	50192	112982	5.44%	0.815%
13	12.880	1828	1834	1843	rBV	1584582	2017825	97.21%	14.555%
14	13.827	1984	1995	2003	rBV	10677	53287	2.57%	0.384%
15	13.933	2008	2013	2023	rVB	351201	502442	24.21%	3.624%
16	15.374	2252	2258	2270	rBV	234068	415684	20.03%	2.998%




Sum of corrected areas: 13863147

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141702.D
Acq On : 20 Feb 2025 14:36
Operator : RC/JU
Sample : Q1383-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-18-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

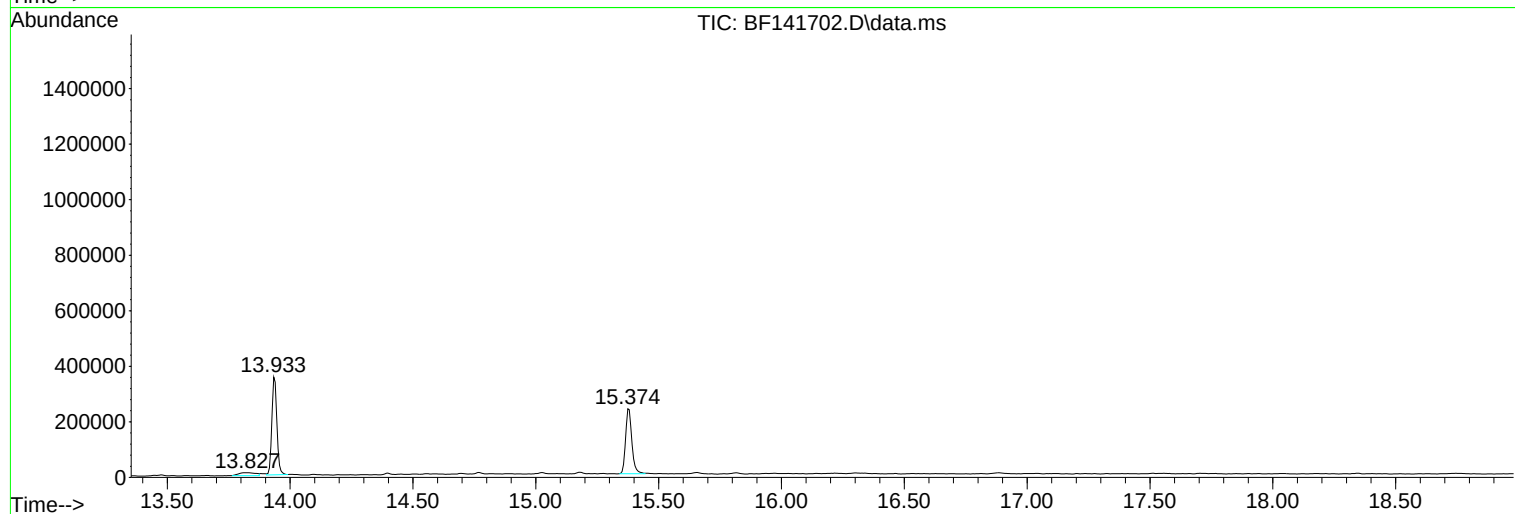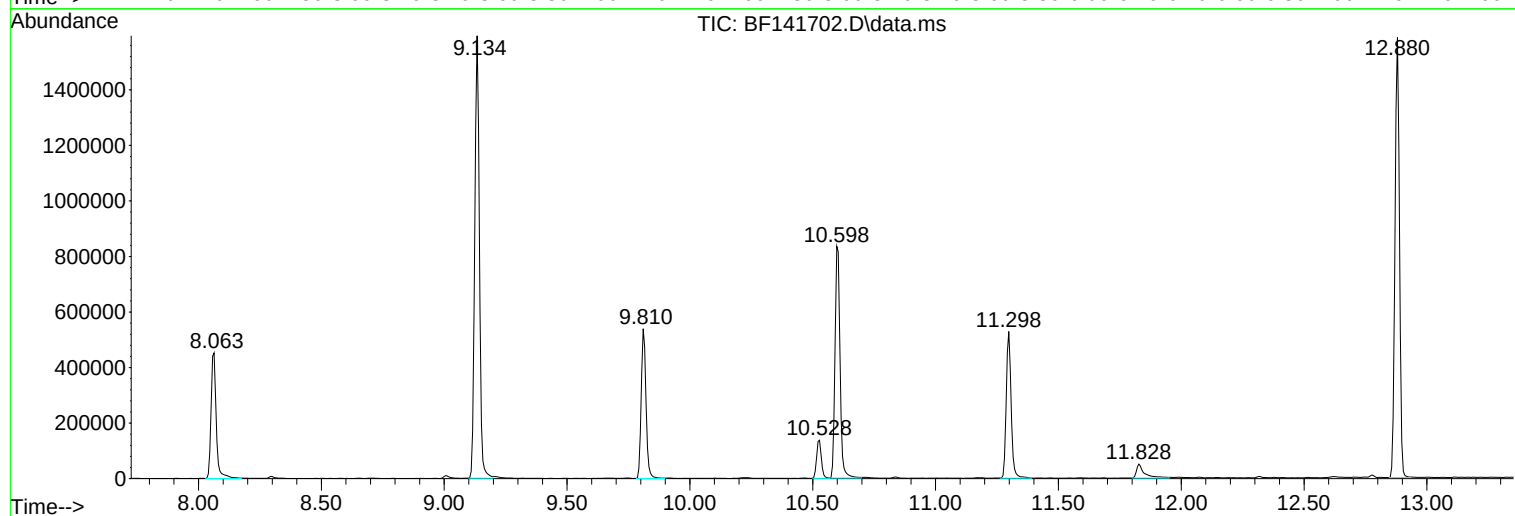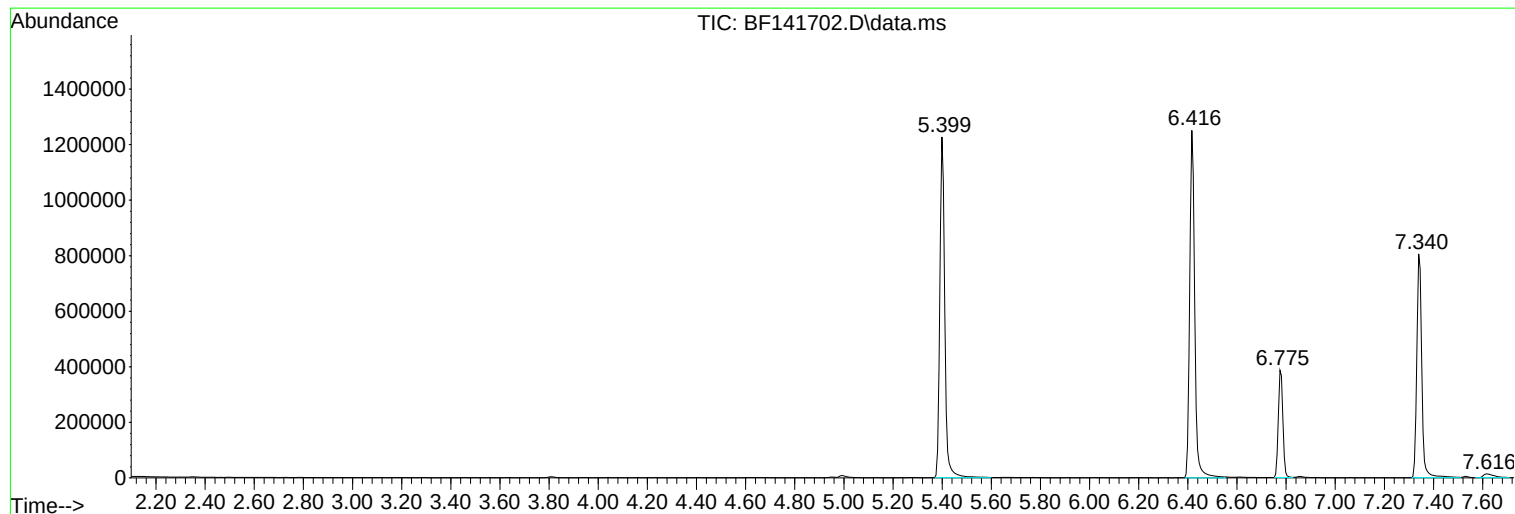

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141702.D
Acq On : 20 Feb 2025 14:36
Operator : RC/JU
Sample : Q1383-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-18-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022025\
Data File : BF141702.D
Acq On : 20 Feb 2025 14:36
Operator : RC/JU
Sample : Q1383-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-18-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------