
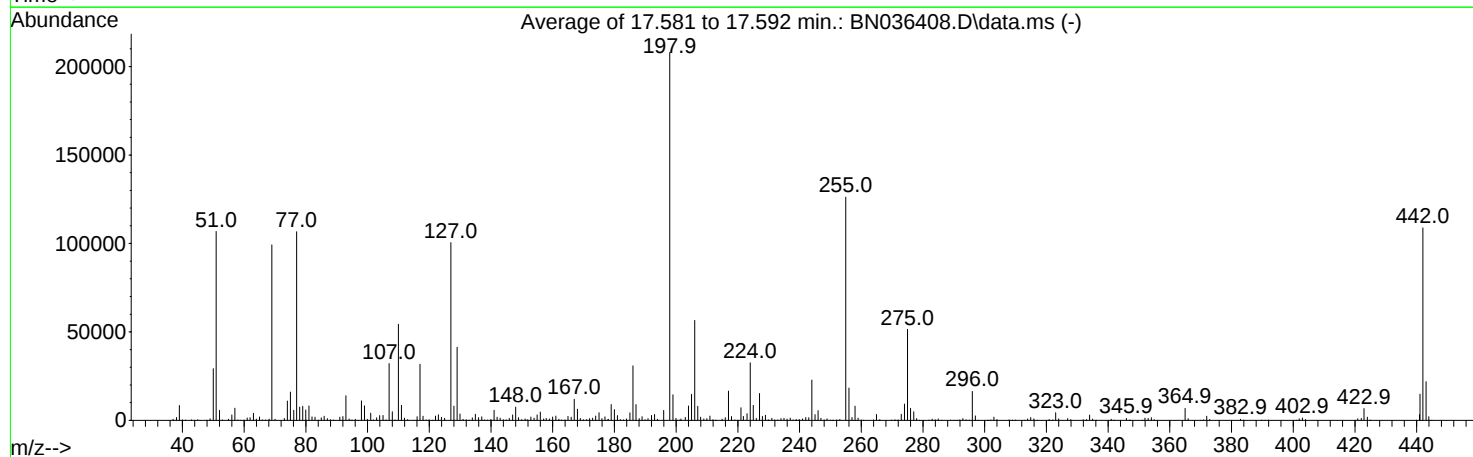


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021025\
Data File : BN036408.D
Acq On : 10 Feb 2025 11:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 11 01:17:14 2025

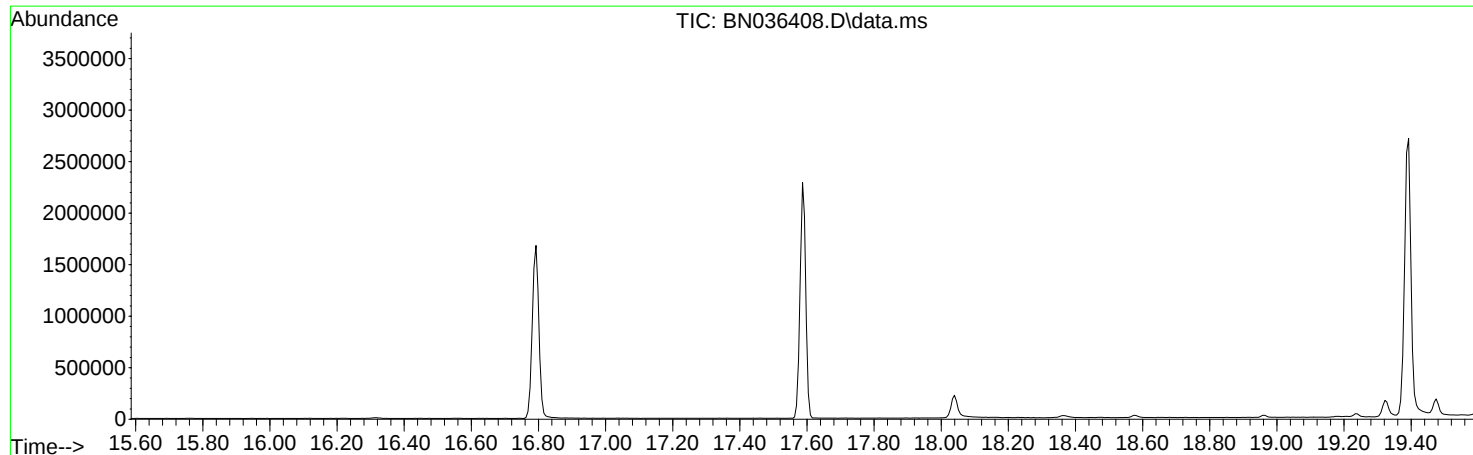

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.4	106809	PASS
68	69	0.00	2	0.7	724	PASS
69	198	0.00	100	47.7	99211	PASS
70	69	0.00	2	0.6	601	PASS
127	198	10	80	48.3	100501	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	207936	PASS
199	198	5	9	7.0	14493	PASS
275	198	10	60	24.7	51437	PASS
365	198	1	100	3.3	6829	PASS
441	198	0.01	100	7.1	14816	PASS
442	442	50	100	100.0	108824	PASS
443	442	15	24	20.1	21911	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/10/2025	BNA_N	<u>BN036408.D</u>
Compound Name	Response	Retention Time
DDT	740190	20.628
DDD	8470	20.239
DDE	0	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8470	748660	1.13

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021025\
Data File : BN036408.D
Acq On : 10 Feb 2025 11:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 11 01:55:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

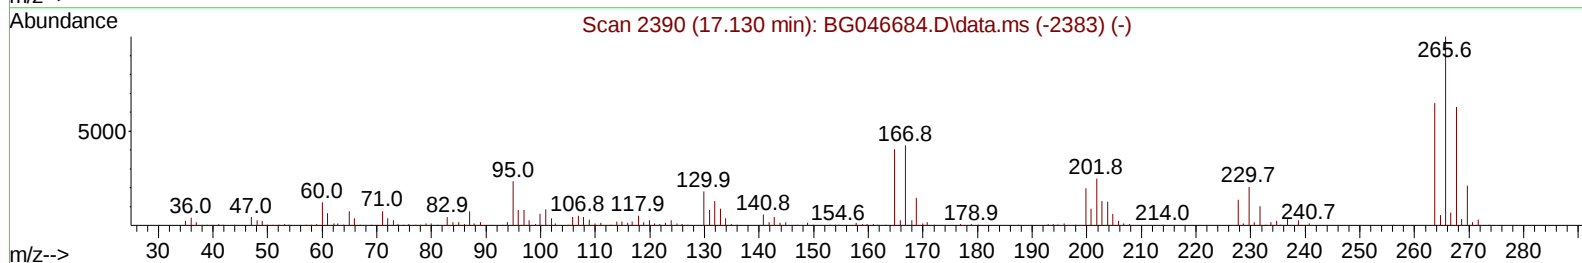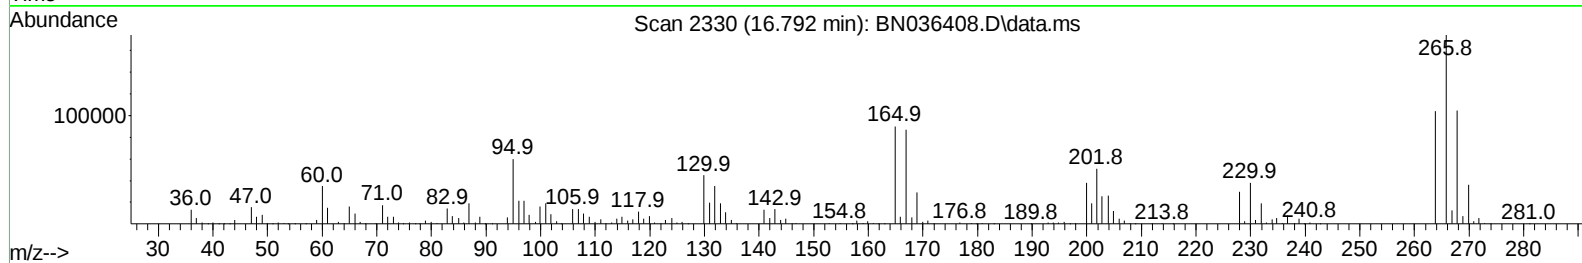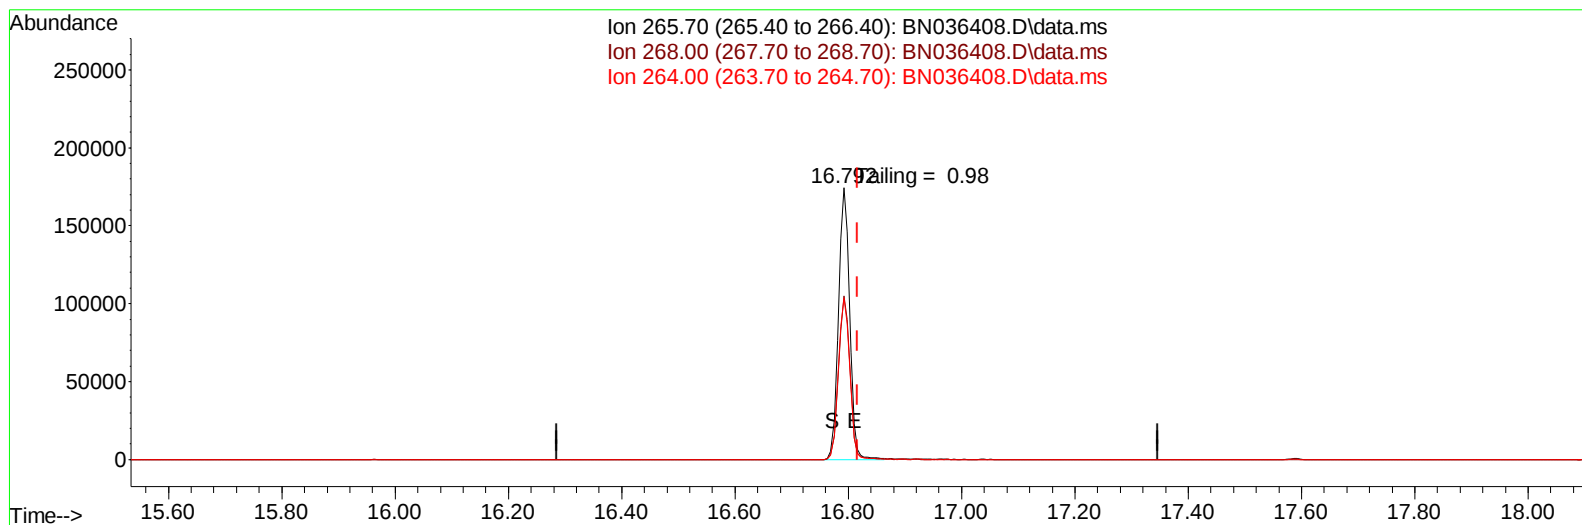

TIC: BN036408.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.024) 22697.76 ng




response 239758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.20
264.00	61.60	59.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021025\
Data File : BN036408.D
Acq On : 10 Feb 2025 11:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 11 01:55:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

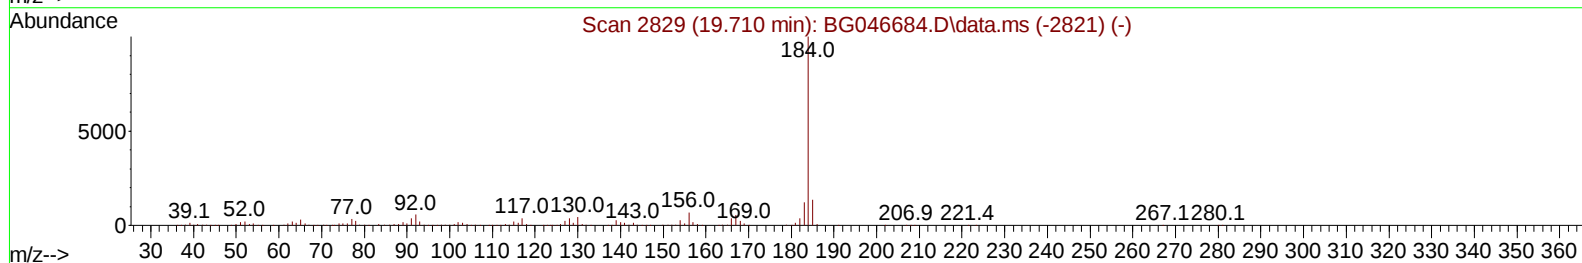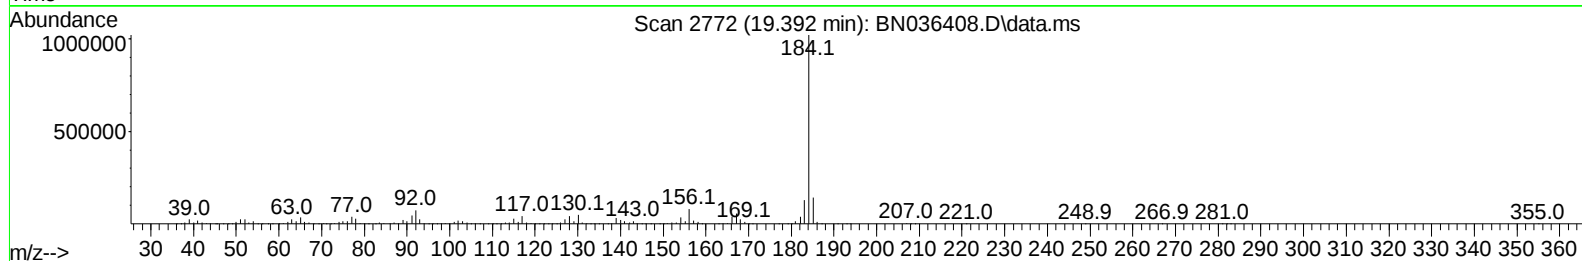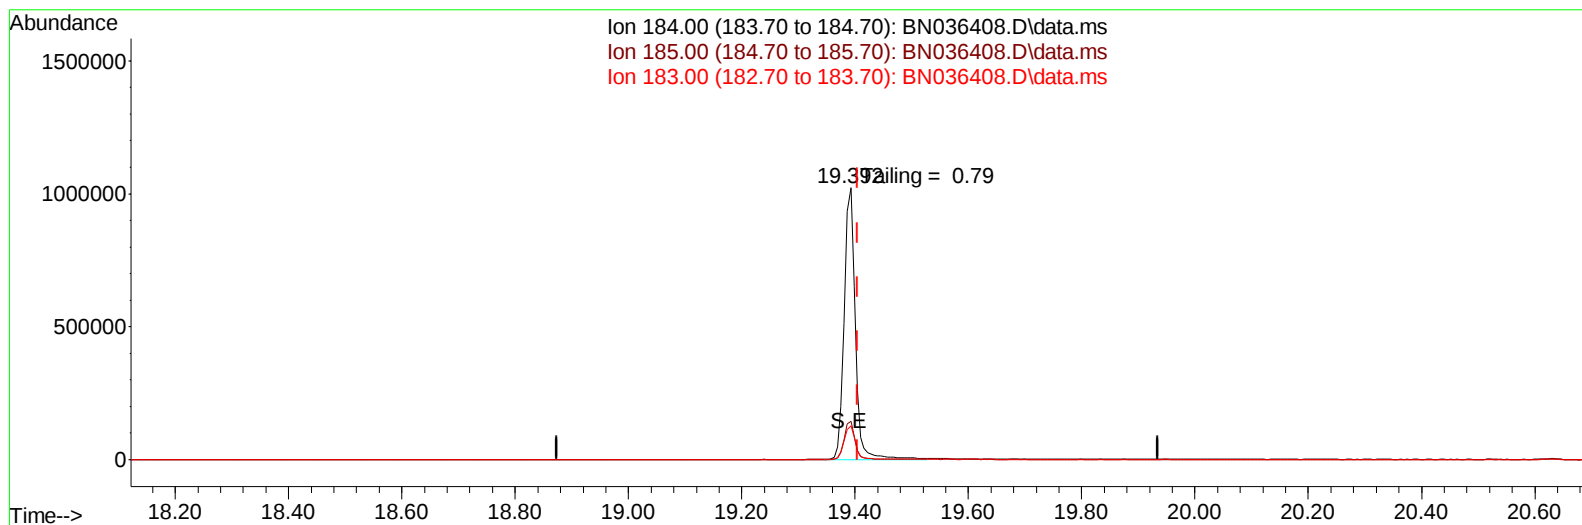

TIC: BN036408.D\data.ms

(77) Benzidine

19.392min (-0.012) 0.00 ng

response 1390167

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	12.43
0.00	0.00	0.00