


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022425\
Data File : BN036491.D
Acq On : 24 Feb 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 11 01:17:14 2025

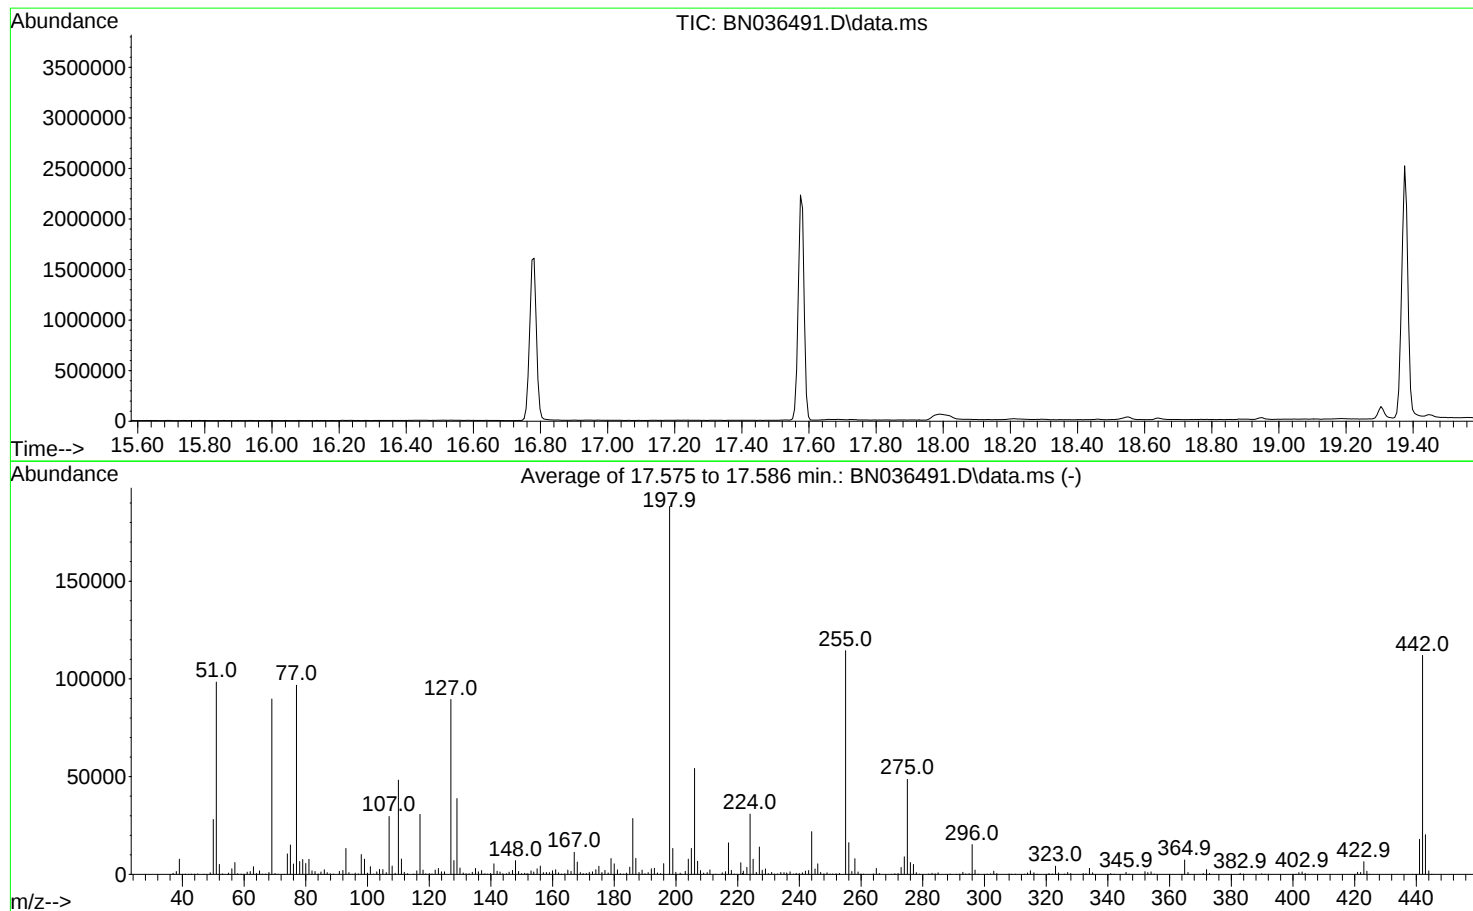

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	98424	PASS
68	69	0.00	2	1.1	1016	PASS
69	198	0.00	100	47.7	89756	PASS
70	69	0.00	2	0.6	506	PASS
127	198	10	80	47.5	89491	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	188205	PASS
199	198	5	9	7.1	13293	PASS
275	198	10	60	25.9	48656	PASS
365	198	1	100	3.9	7382	PASS
441	198	0.01	100	9.5	17970	PASS
442	442	50	100	100.0	112037	PASS
443	442	15	24	18.1	20334	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/24/2025	BNA_N	<u>BN036491.D</u>
Compound Name	Response	Retention Time
DDT	694675	20.616
DDD	7944	20.228
DDE	235	19.663
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8179	702854	1.16

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022425\
Data File : BN036491.D
Acq On : 24 Feb 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 24 12:45:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

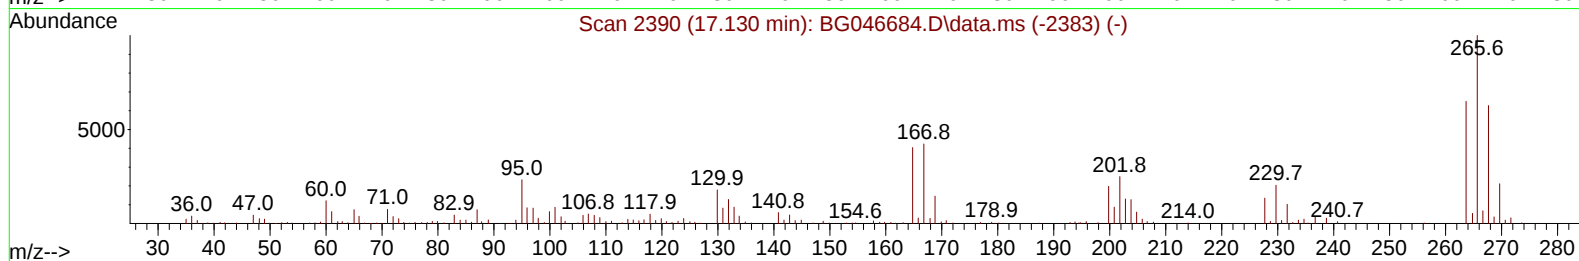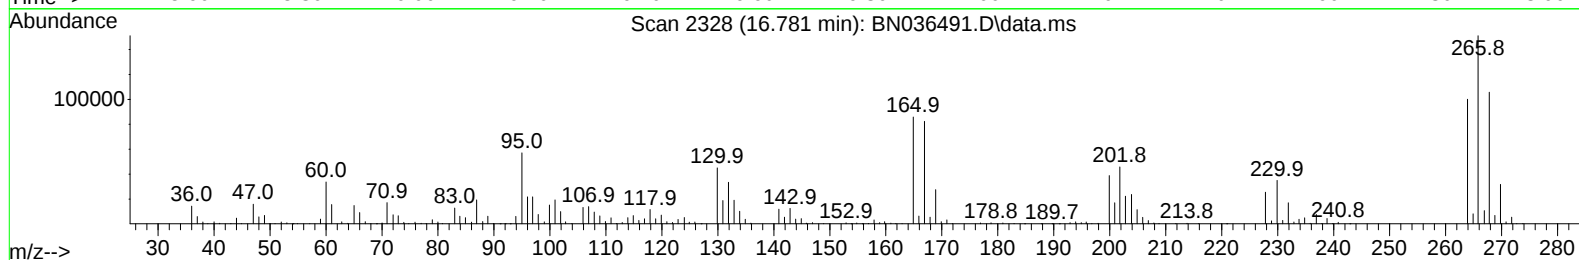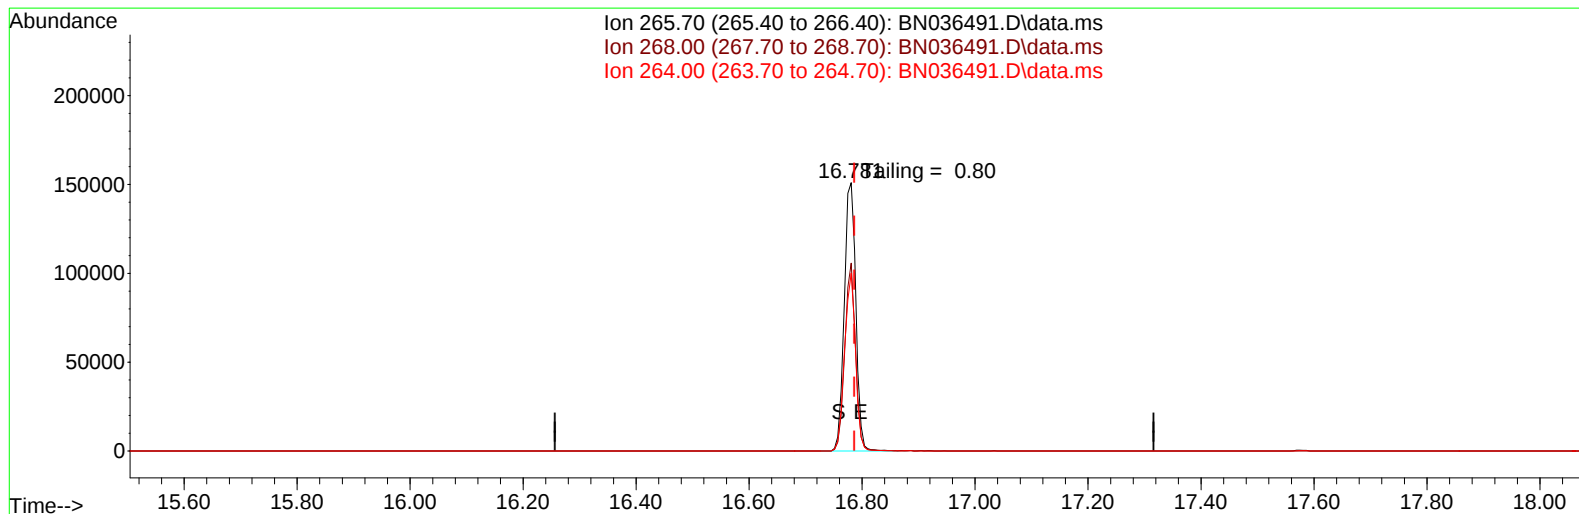

TIC: BN036491.D\data.ms

(70) Pentachlorophenol (C)

16.781min (-0.005) 19002.28 ng




response 213398

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.99
264.00	61.60	66.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022425\
Data File : BN036491.D
Acq On : 24 Feb 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 24 12:45:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

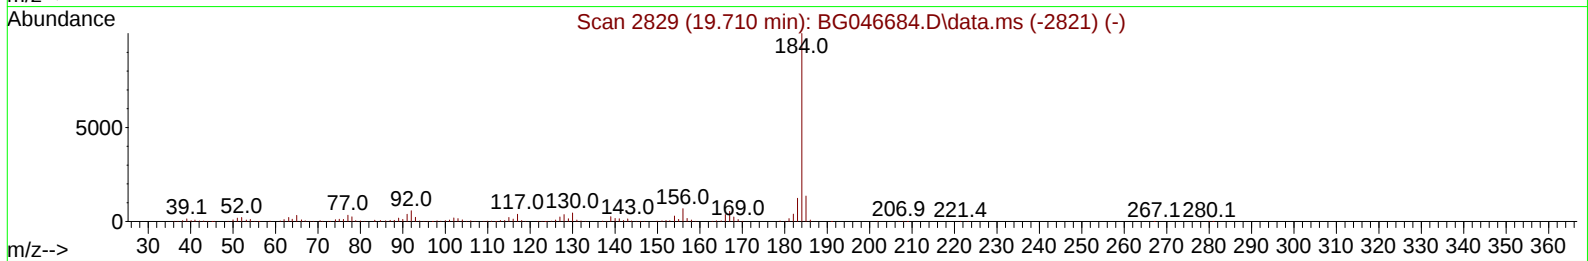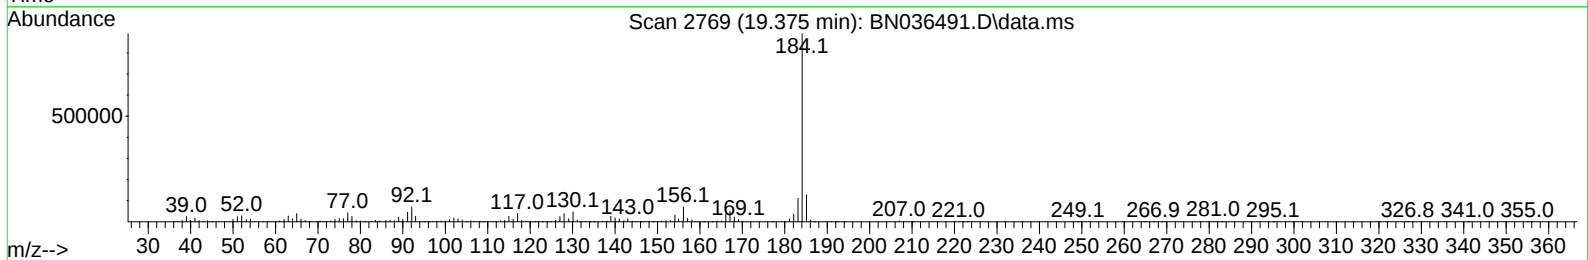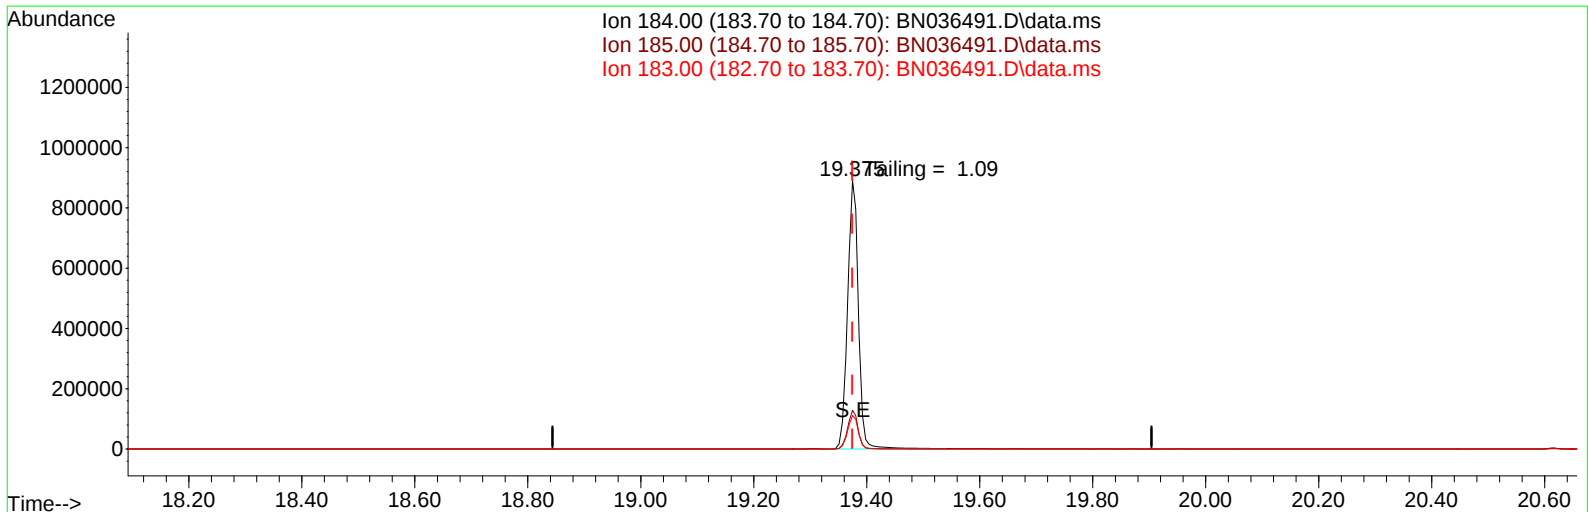

TIC: BN036491.D\data.ms

(77) Benzidine

19.375min (+ 0.001) 0.00 ng

response 1188729

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.43
183.00	13.20	12.54
0.00	0.00	0.00