



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022525\
Data File : VX045028.D
Acq On : 25 Feb 2025 09:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
Title : SW846 8260
Last Update : Tue Feb 11 03:41:08 2025

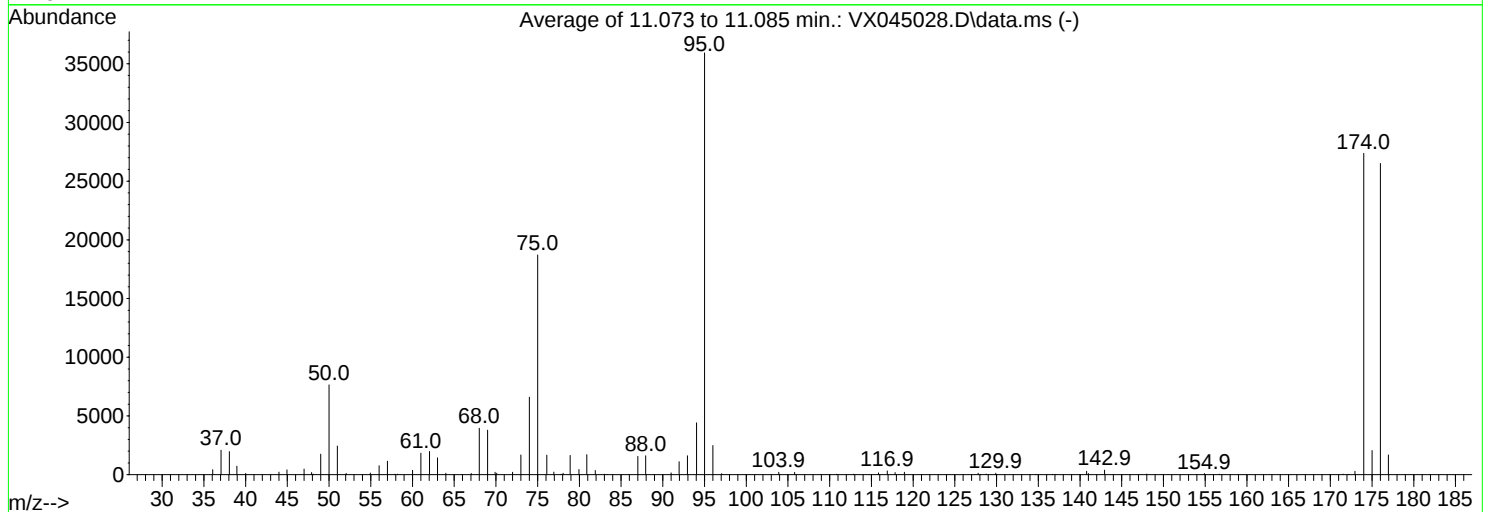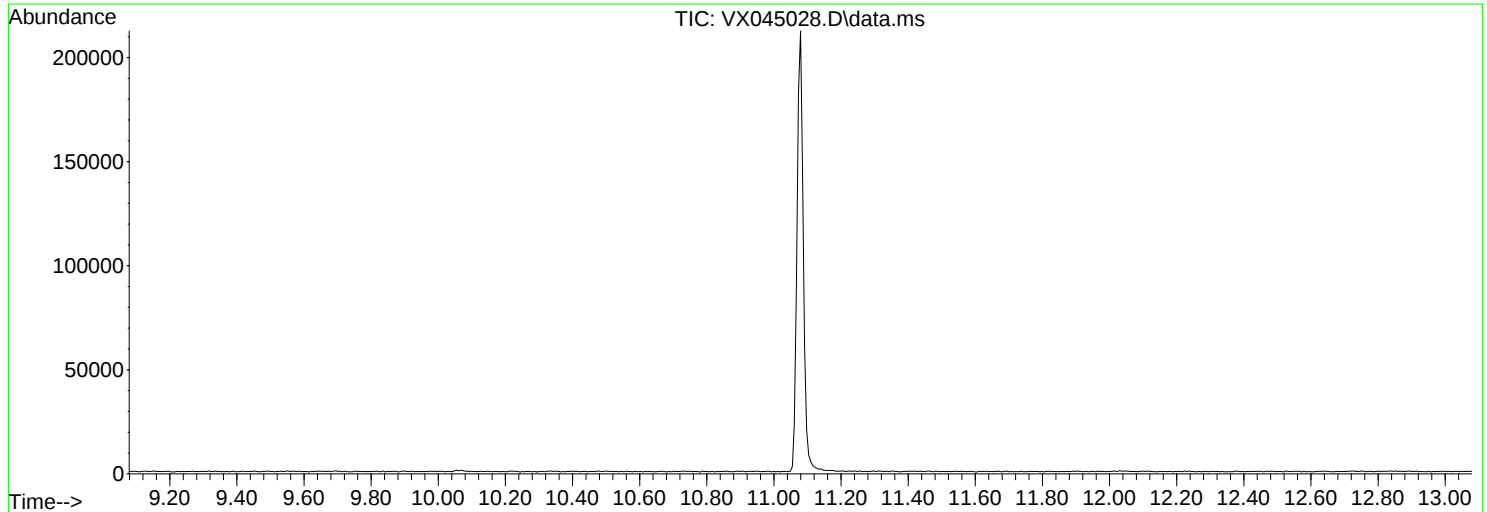

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	7648	PASS
75	95	30	60	52.1	18718	PASS
95	95	100	100	100.0	35928	PASS
96	95	5	9	6.9	2482	PASS
173	174	0.00	2	1.0	281	PASS
174	95	50	100	76.2	27363	PASS
175	174	5	9	7.5	2061	PASS
176	174	95	101	96.9	26515	PASS
177	176	5	9	6.3	1671	PASS