
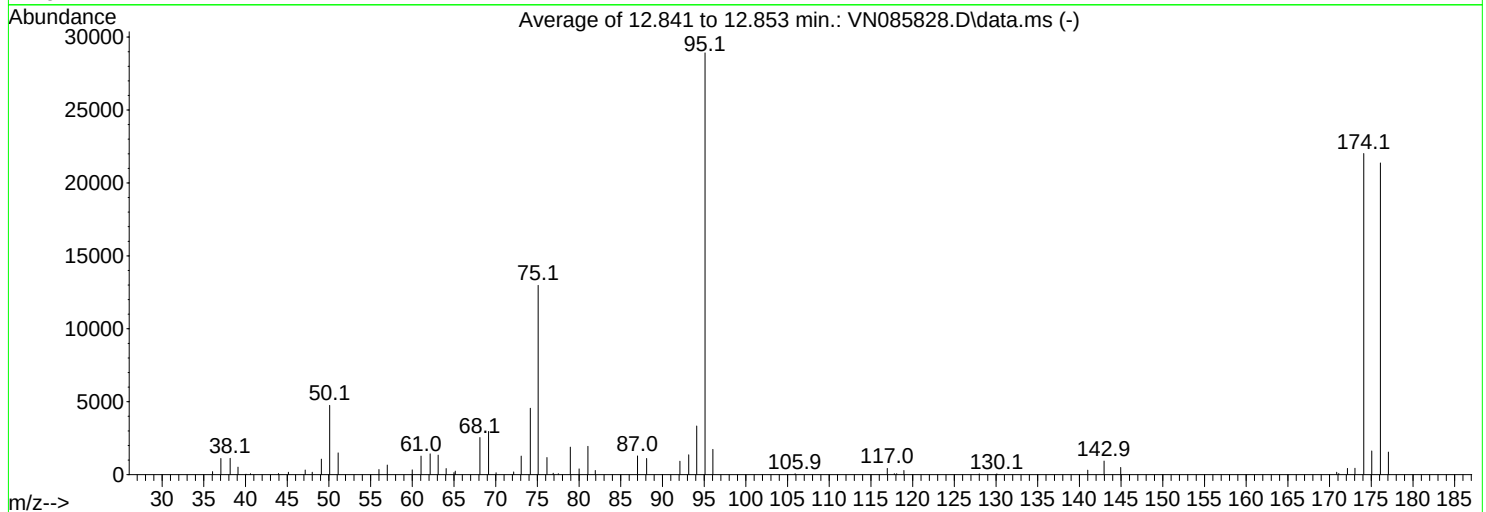


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022425\
Data File : VN085828.D
Acq On : 24 Feb 2025 10:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

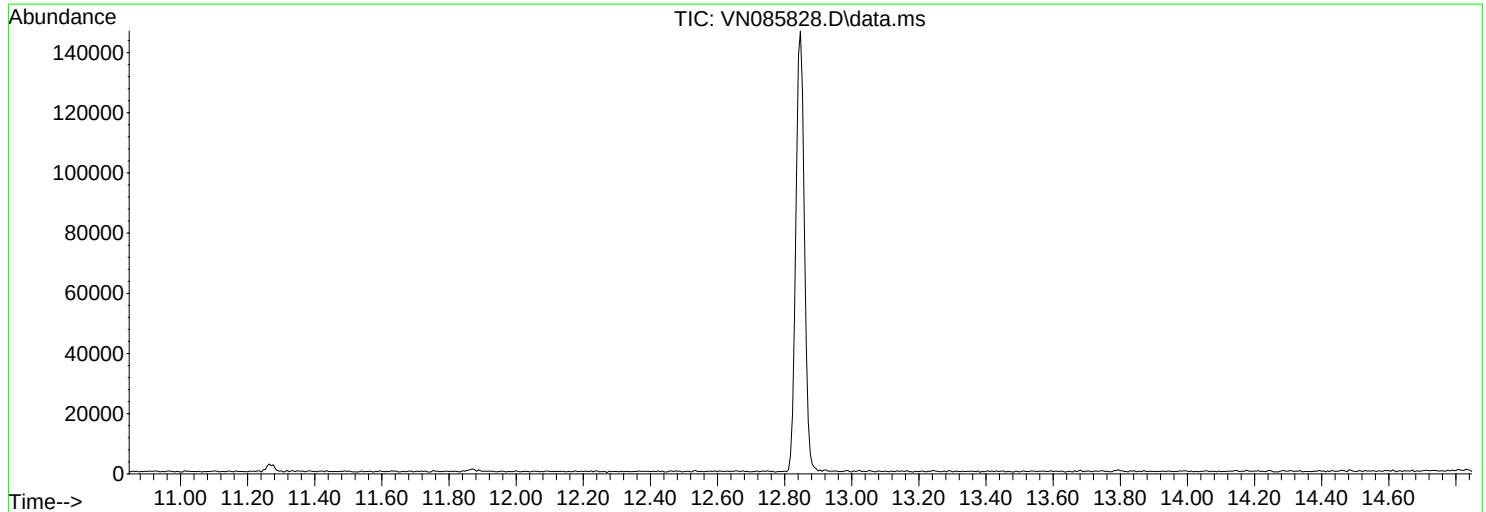

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.4	4752	PASS
75	95	30	60	44.9	12981	PASS
95	95	100	100	100.0	28920	PASS
96	95	5	9	6.0	1735	PASS
173	174	0.00	2	2.0	435	PASS
174	95	50	100	76.1	22019	PASS
175	174	5	9	7.4	1623	PASS
176	174	95	101	97.1	21376	PASS
177	176	5	9	7.2	1547	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	213	50.10	4752	68.10	2541	80.00	391
37.05	1113	51.10	1494	69.15	2959	81.05	193
38.15	1123	56.00	352	70.05	131	81.95	28
39.10	516	57.00	660	72.15	192	87.00	128
40.05	37	60.00	334	73.05	1273	88.10	1113
40.60	70	61.05	1273	74.15	4554	92.10	923
43.95	77	62.15	1425	75.10	12981	93.15	1365
45.15	168	63.10	1344	76.15	1172	94.10	3331
47.15	317	64.05	415	76.90	97	95.10	28920
48.00	169	65.00	146	77.50	65	96.05	1735
49.10	1059	65.15	244	78.95	1892	105.90	64

Average of 12.841 to 12.853 min.: VN085828.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.95	433	172.15	424				
117.80	70	173.05	435				
118.10	66	174.10	22019				
118.95	287	175.05	1623				
128.00	55	176.10	21376				
130.10	57	177.05	1547				
141.00	304						
142.95	938						
144.95	493						
170.85	165						
171.10	77						

Instrument :

MSVOA_N

ClientSampleId :

BFB