

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022525\
 Data File : PP070039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2025 13:28
 Operator : YP\AJ
 Sample : Q1415-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B-163-SB02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/26/2025
 Supervised By :Ankita Jodhani 02/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 03:52:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.528	3.830	35035987	23515727	23.873	24.597
2) SA Decachlor...	10.258	8.889	20467570	19007003	17.969m	17.532

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022525\
Data File : PP070039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2025 13:28
Operator : YP\AJ
Sample : Q1415-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
B-163-SB02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/26/2025
Supervised By :Ankita Jodhani 02/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 03:52:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

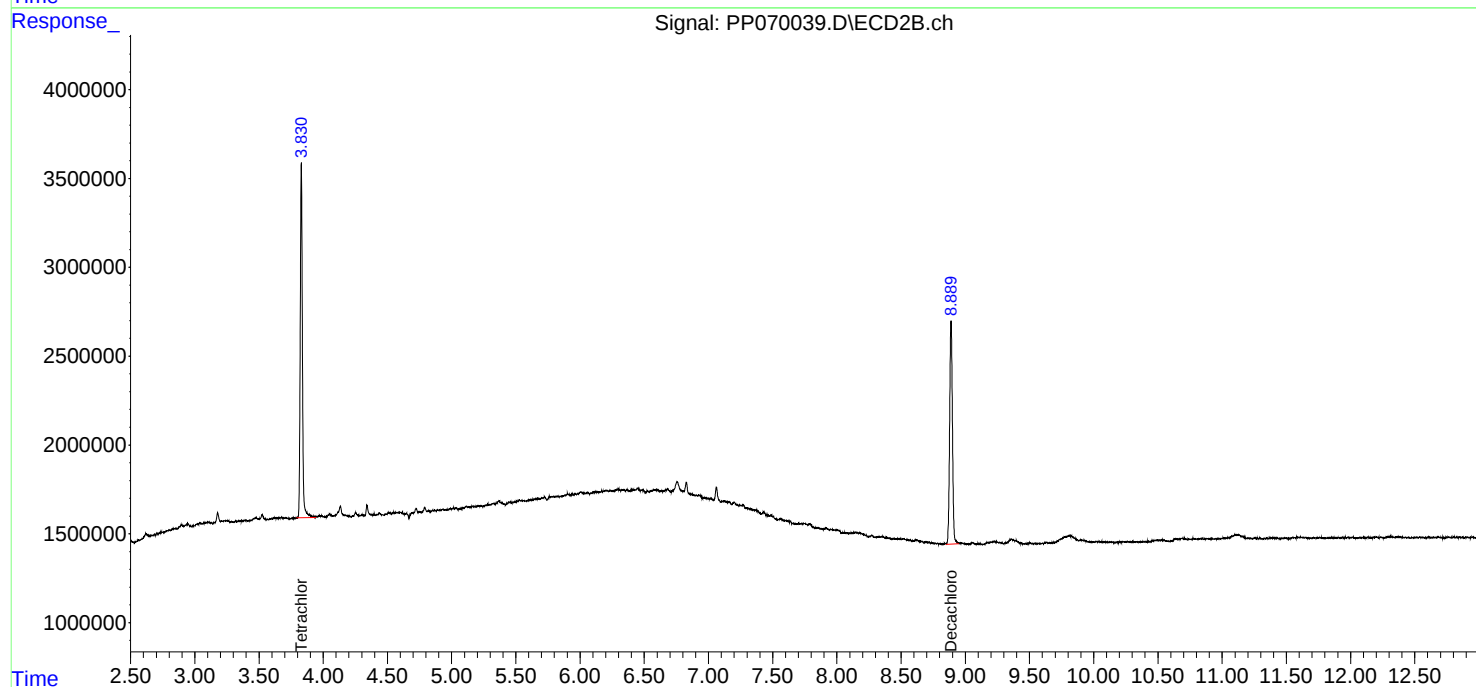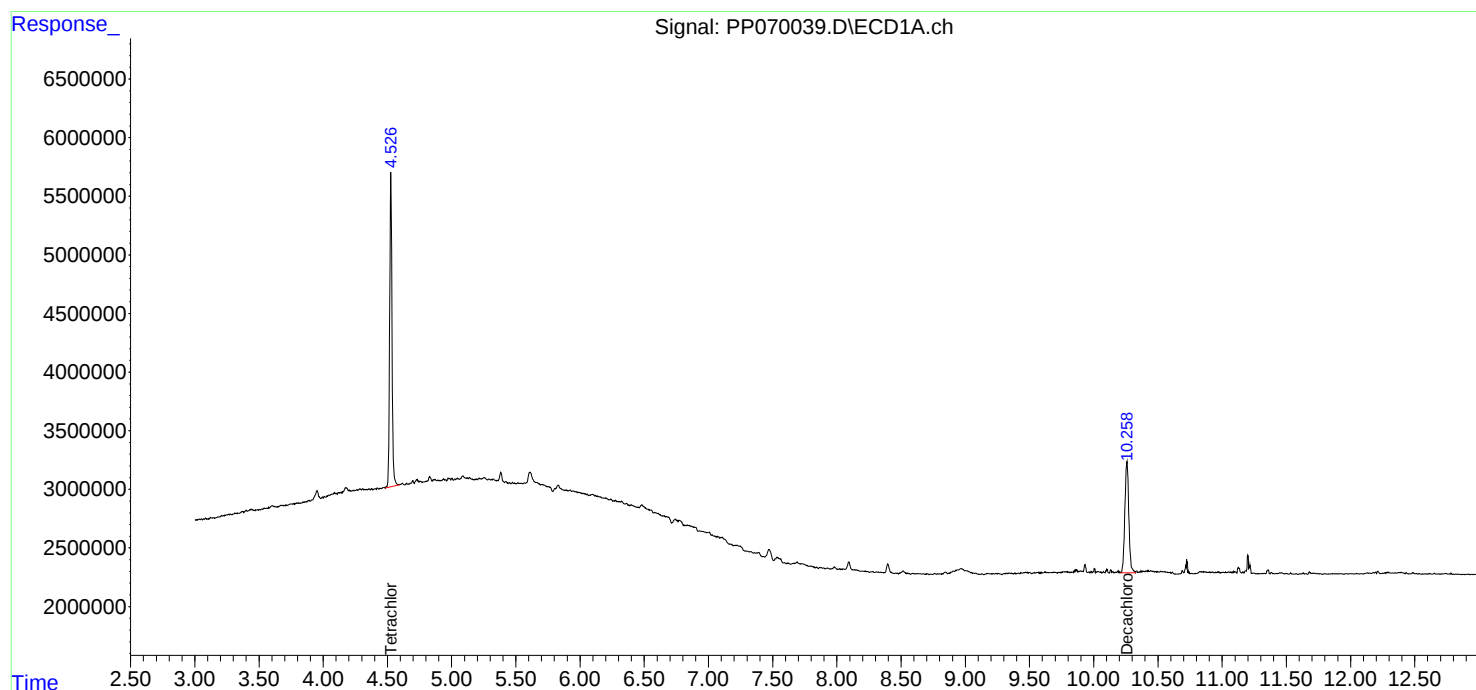

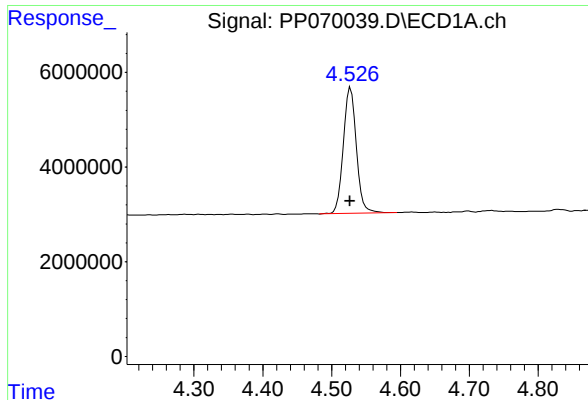


#1 Tetrachloro-m-xylene

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 35035987
Conc: 23.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-163-SB02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/26/2025
Supervised By :Ankita Jodhani 02/26/2025

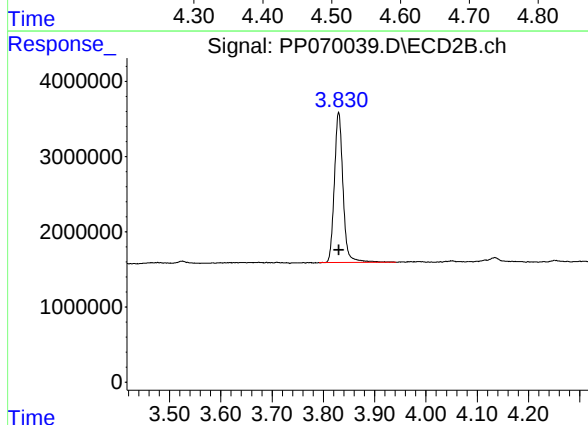


#1 Tetrachloro-m-xylene

R.T.: 3.830 min
Delta R.T.: 0.000 min
Response: 23515727
Conc: 24.60 ng/ml

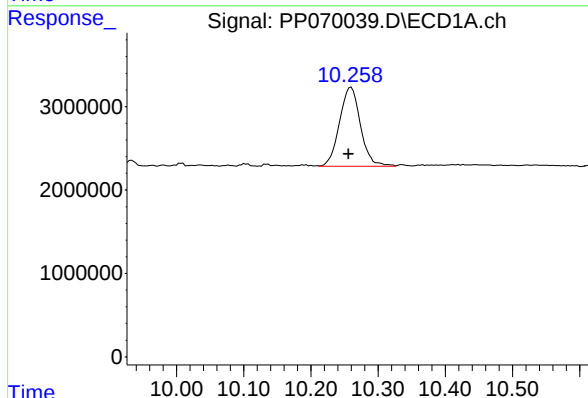

#2 Decachlorobiphenyl

R.T.: 10.258 min
Delta R.T.: 0.002 min
Response: 20467570
Conc: 17.97 ng/ml m

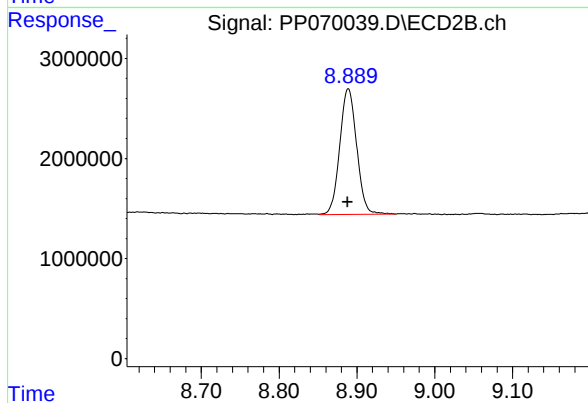

#2 Decachlorobiphenyl

R.T.: 8.889 min
Delta R.T.: 0.001 min
Response: 19007003
Conc: 17.53 ng/ml