

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141780.D
Acq On : 26 Feb 2025 13:55
Operator : RC/JU
Sample : PB166875BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166875BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	559	565	590	rBV	1659137	2438000	73.46%	13.449%
2	6.428	731	737	766	rBV	1646884	2406444	72.51%	13.275%
3	6.781	792	797	811	rVB	353647	450721	13.58%	2.486%
4	7.345	887	893	924	rBV	1137657	1618662	48.78%	8.929%
5	8.063	1009	1015	1040	rBV	410466	607975	18.32%	3.354%
6	9.133	1191	1197	1227	rBV	2227208	3096525	93.31%	17.082%
7	9.816	1307	1313	1327	rBV	484181	705275	21.25%	3.891%
8	10.604	1442	1447	1475	rBV	1242034	1794300	54.07%	9.898%
9	11.298	1560	1565	1588	rBV	471487	715714	21.57%	3.948%
10	12.886	1829	1835	1848	rBV	2460799	3318618	100.00%	18.307%
11	13.939	2009	2014	2031	rBV	343084	539706	16.26%	2.977%
12	15.386	2254	2260	2279	rBV	228373	435941	13.14%	2.405%




Sum of corrected areas: 18127881

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141780.D
Acq On : 26 Feb 2025 13:55
Operator : RC/JU
Sample : PB166875BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

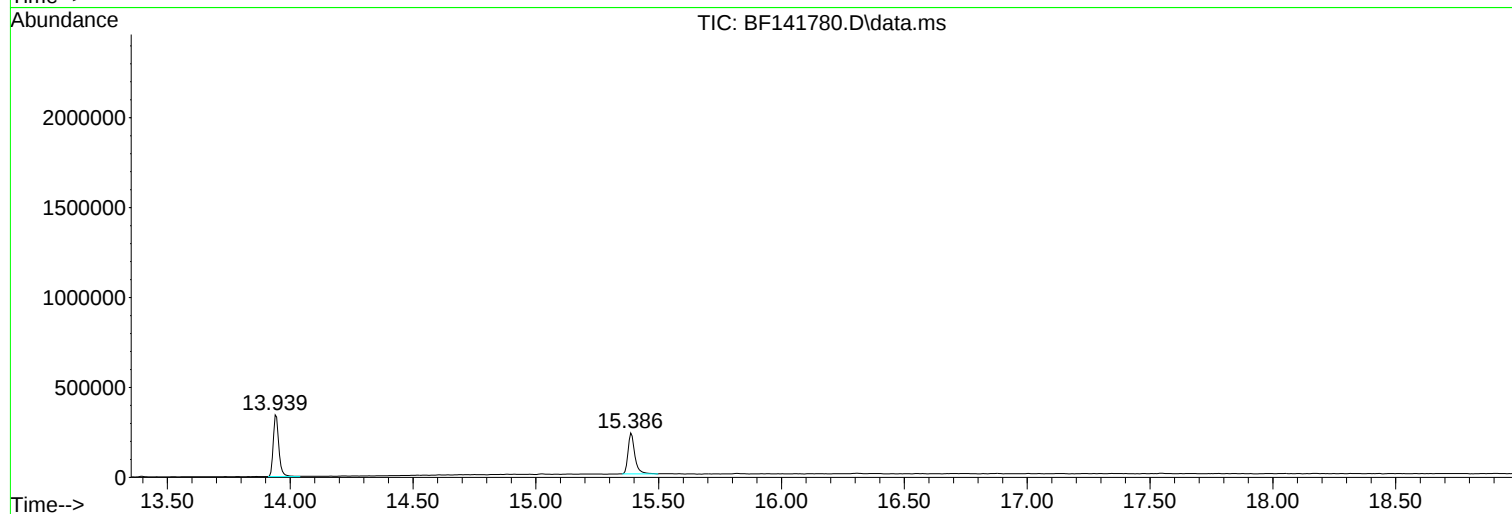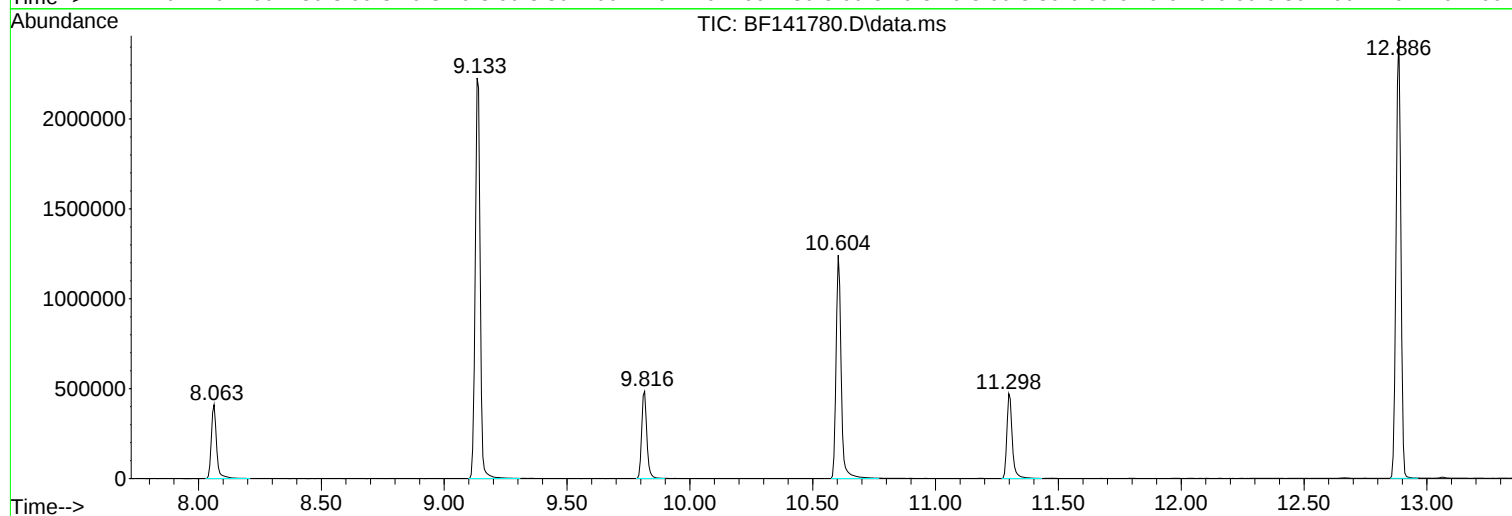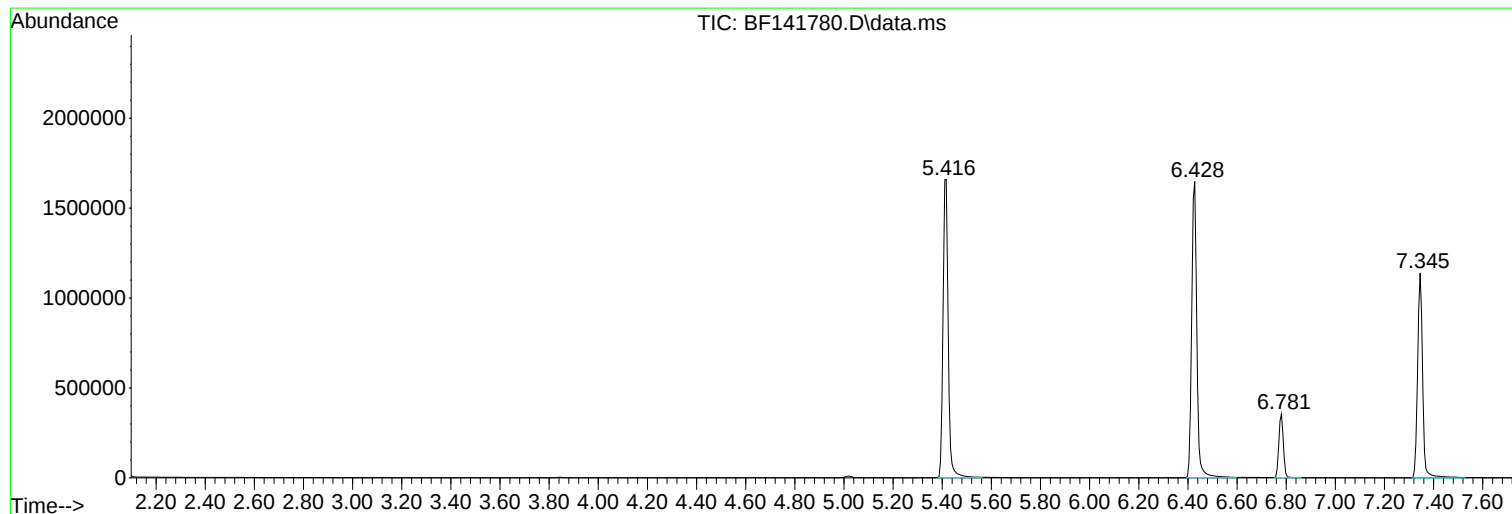

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141780.D
Acq On : 26 Feb 2025 13:55
Operator : RC/JU
Sample : PB166875BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141780.D
Acq On : 26 Feb 2025 13:55
Operator : RC/JU
Sample : PB166875BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------