
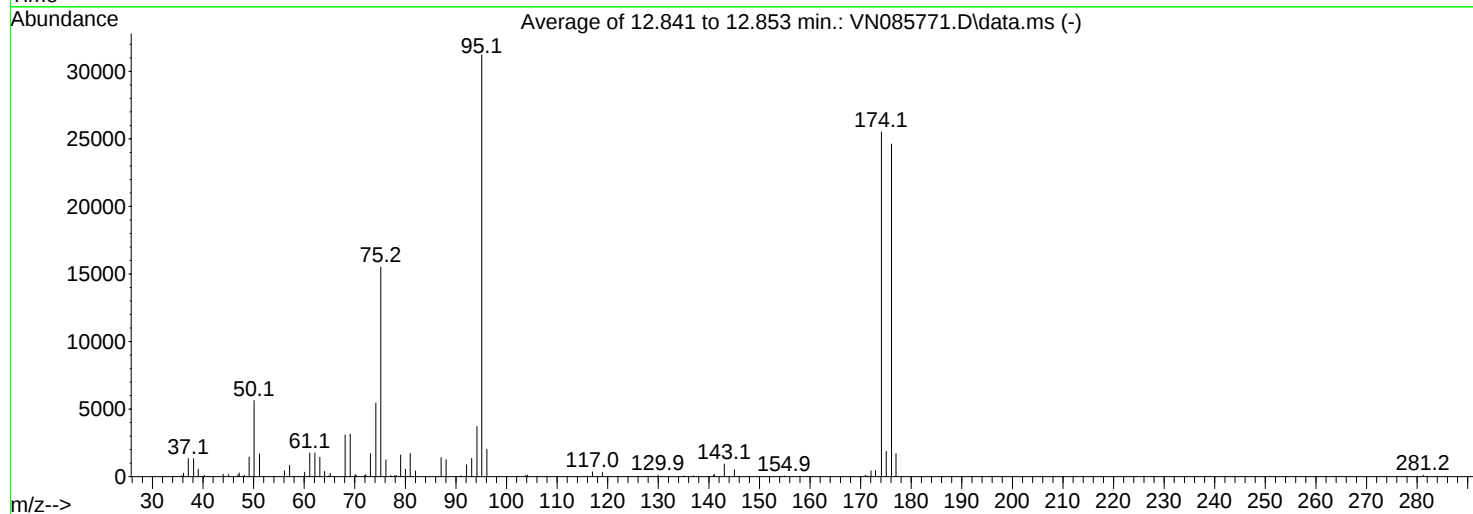


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021825\  
Data File : VN085771.D  
Acq On : 18 Feb 2025 10:35  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021825W.M  
Title : SW846 8260  
Last Update : Wed Feb 19 03:43:32 2025

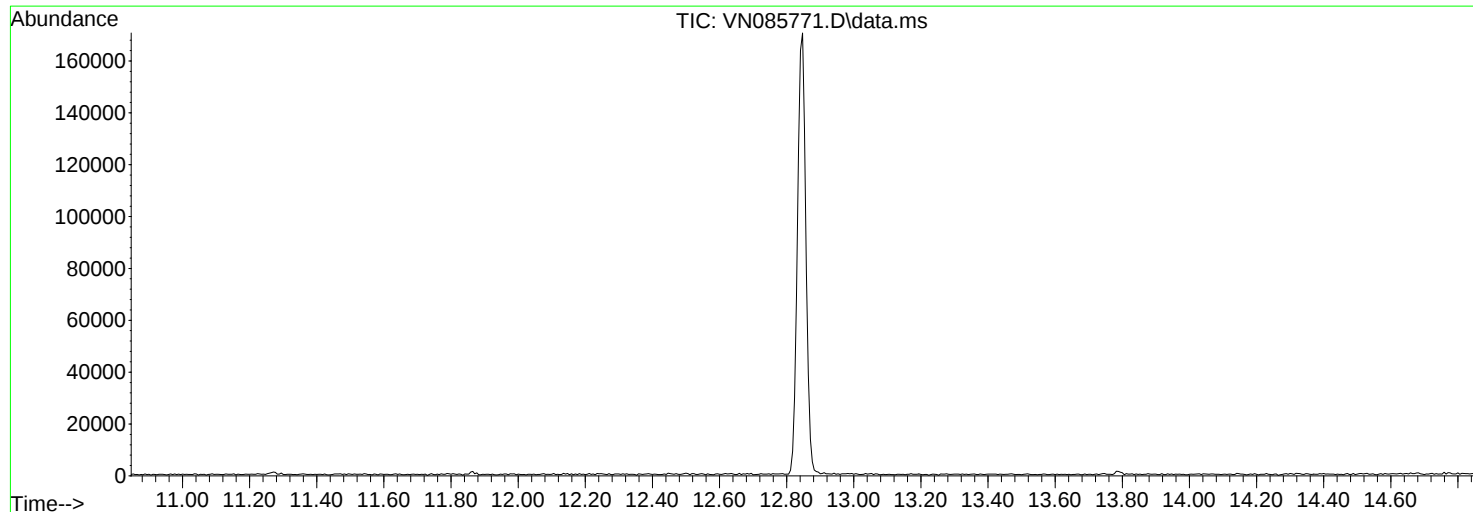

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.1         | 5643       | PASS                |
| 75             | 95              | 30              | 60              | 49.7         | 15509      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 31224      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 2024       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.8          | 452        | PASS                |
| 174            | 95              | 50              | 100             | 81.7         | 25509      | PASS                |
| 175            | 174             | 5               | 9               | 7.4          | 1882       | PASS                |
| 176            | 174             | 95              | 101             | 96.5         | 24621      | PASS                |
| 177            | 176             | 5               | 9               | 6.9          | 1699       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.80 | 65     | 48.15 | 124    | 64.90 | 70     | 76.15 | 124    |
| 36.15 | 261    | 49.10 | 1454   | 65.15 | 255    | 77.10 | 80     |
| 37.10 | 1338   | 50.10 | 5643   | 68.10 | 3096   | 77.90 | 80     |
| 38.15 | 1335   | 51.15 | 1680   | 69.10 | 3155   | 78.20 | 80     |
| 39.05 | 560    | 56.10 | 443    | 70.05 | 161    | 79.05 | 1595   |
| 40.00 | 21     | 57.10 | 824    | 70.30 | 106    | 80.00 | 557    |
| 40.30 | 99     | 60.10 | 333    | 71.90 | 80     | 80.95 | 1716   |
| 44.00 | 176    | 61.10 | 1754   | 72.15 | 148    | 82.00 | 419    |
| 45.05 | 157    | 62.10 | 1754   | 73.10 | 1710   | 87.05 | 1414   |
| 46.90 | 145    | 63.10 | 1428   | 74.15 | 5444   | 88.05 | 1255   |
| 47.15 | 276    | 64.05 | 377    | 75.15 | 15509  | 91.00 | 59     |

Average of 12.841 to 12.853 min.: VN085771.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z | abund. |
|--------|--------|--------|--------|--------|--------|-----|--------|
| 92.10  | 882    | 135.10 | 54     | 174.10 | 25509  |     |        |
| 93.10  | 1346   | 136.90 | 57     | 175.05 | 1882   |     |        |
| 94.15  | 3713   | 140.90 | 114    | 176.10 | 24621  |     |        |
| 95.10  | 31224  | 141.05 | 164    | 177.00 | 1699   |     |        |
| 96.10  | 2024   | 143.05 | 938    | 281.20 | 112    |     |        |
| 103.80 | 81     | 145.05 | 510    |        |        |     |        |
| 104.10 | 121    | 154.90 | 54     |        |        |     |        |
| 116.00 | 52     | 170.90 | 116    |        |        |     |        |
| 117.00 | 351    | 171.30 | 58     |        |        |     |        |
| 118.95 | 331    | 172.05 | 440    |        |        |     |        |
| 129.95 | 112    | 172.95 | 452    |        |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB