
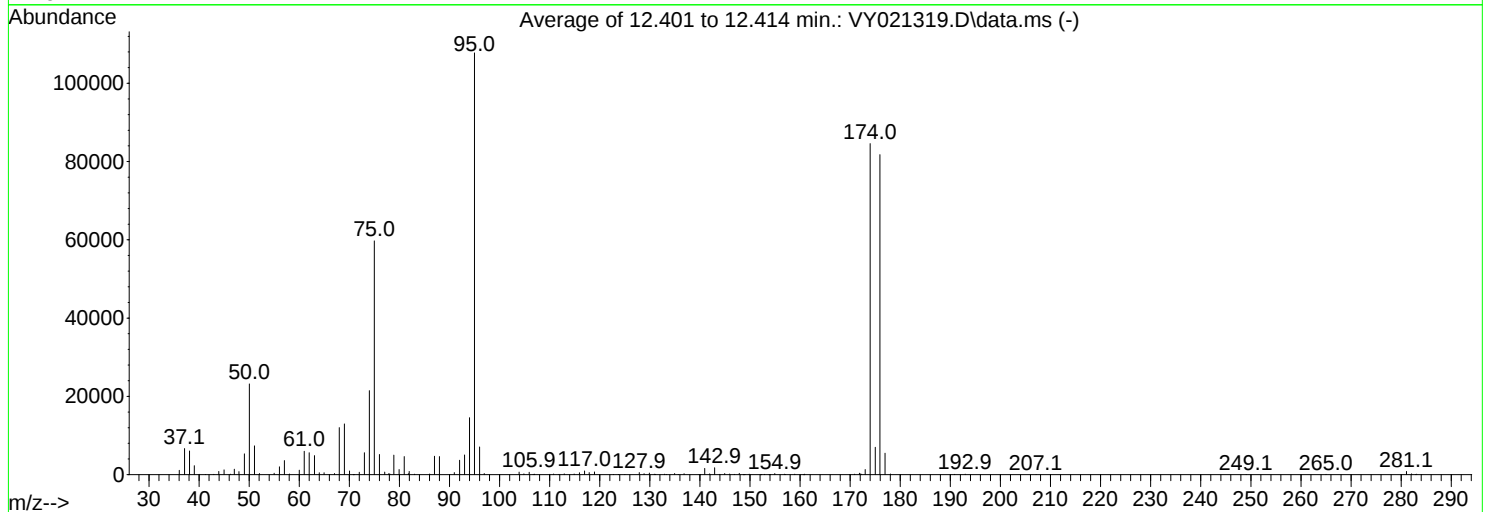


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022625\
Data File : VY021319.D
Acq On : 26 Feb 2025 09:12
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
Title : SW846 8260
Last Update : Wed Feb 26 02:09:13 2025

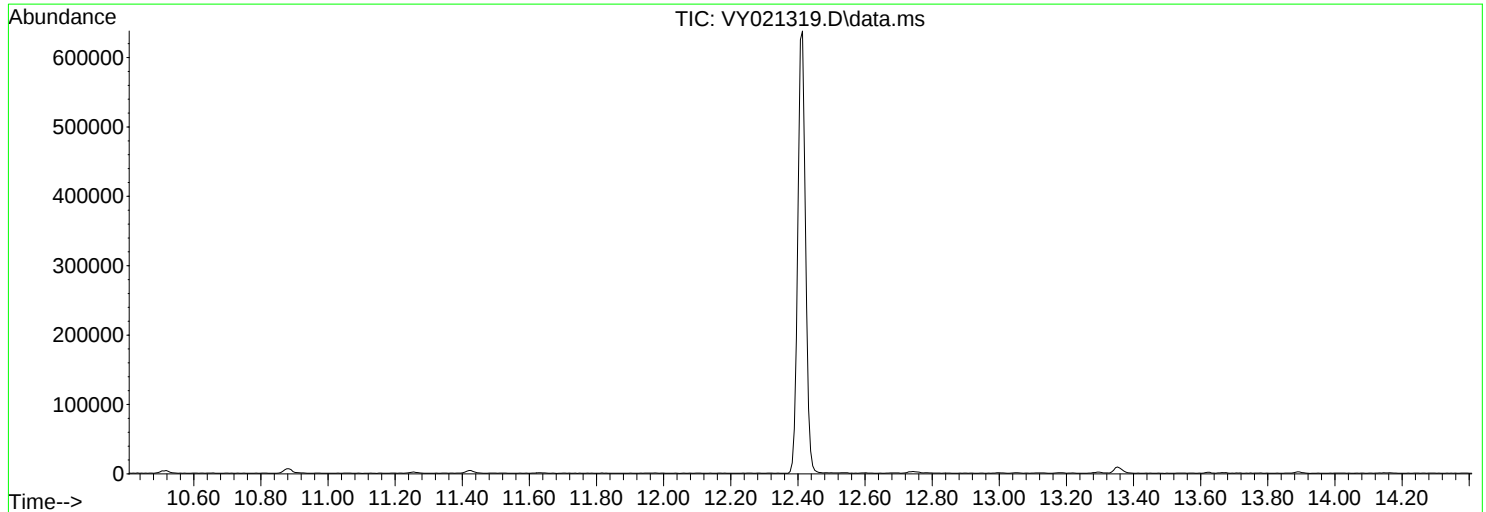

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	23171	PASS
75	95	30	60	55.4	59717	PASS
95	95	100	100	100.0	107776	PASS
96	95	5	9	6.6	7086	PASS
173	174	0.00	2	1.5	1306	PASS
174	95	50	100	78.5	84589	PASS
175	174	5	9	8.3	7013	PASS
176	174	95	101	96.7	81784	PASS
177	176	5	9	6.7	5470	PASS