

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022725\
 Data File : VY021347.D
 Acq On : 27 Feb 2025 10:42
 Operator : SY/MD
 Sample : VY0227SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0227SBL01

Quant Time: Feb 28 00:40:00 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 26 02:09:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	140233	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	264026	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	255103	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	107368	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	94225	59.230	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.460%
35) Dibromofluoromethane	7.634	113	90944	52.539	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.080%
50) Toluene-d8	10.109	98	322284	48.176	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.360%
62) 4-Bromofluorobenzene	12.407	95	111519	49.533	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	99.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022725\
Data File : VY021347.D
Acq On : 27 Feb 2025 10:42
Operator : SY/MD
Sample : VY0227SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0227SBL01

Quant Time: Feb 28 00:40:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 26 02:09:13 2025
Response via : Initial Calibration




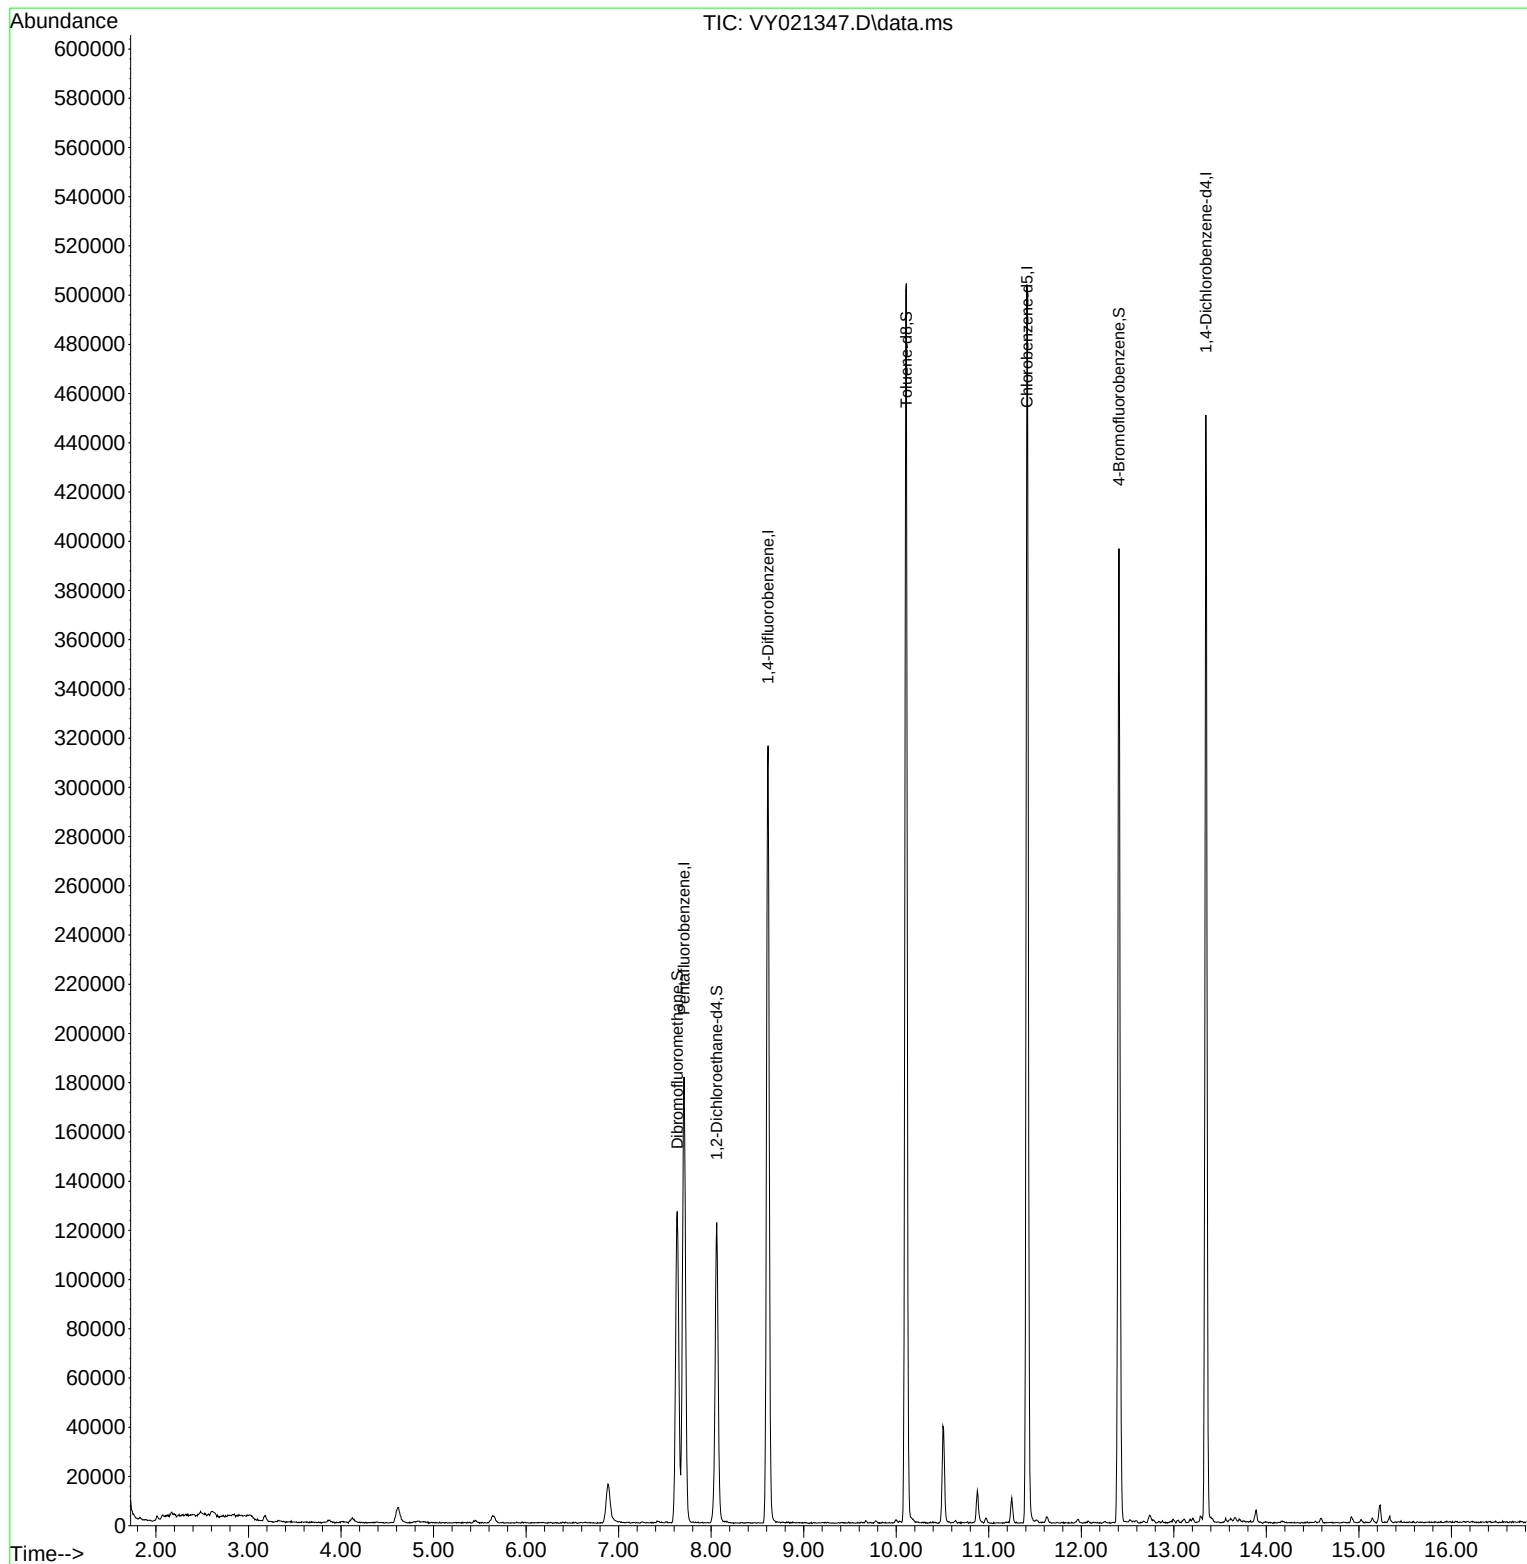


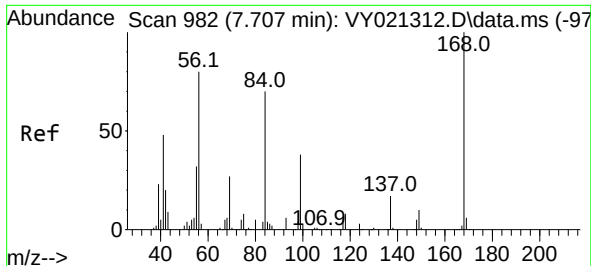

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY021347.D
Acq: 27 Feb 2025 10:42




Instrument :
MSVOA_Y
ClientSampleId :
VY0227SBL01


Tgt Ion:168 Resp: 140233
Ion Ratio Lower Upper
168 100
99 57.6 47.1 70.7

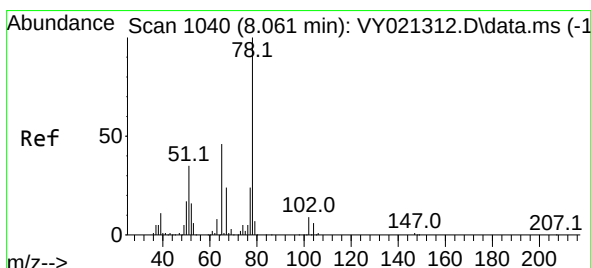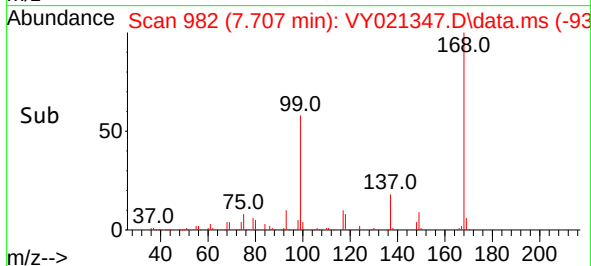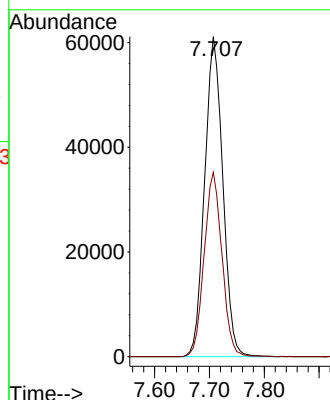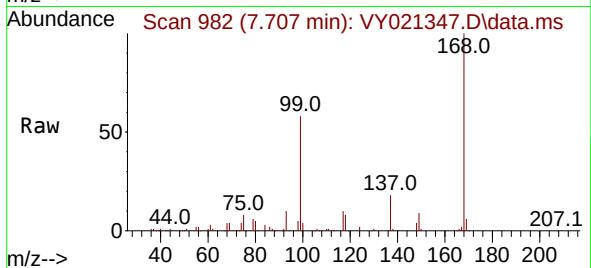

#33
1,2-Dichloroethane-d4
Concen: 59.230 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY021347.D
Acq: 27 Feb 2025 10:42

Tgt Ion: 65 Resp: 94225
Ion Ratio Lower Upper
65 100
67 50.4 0.0 103.6


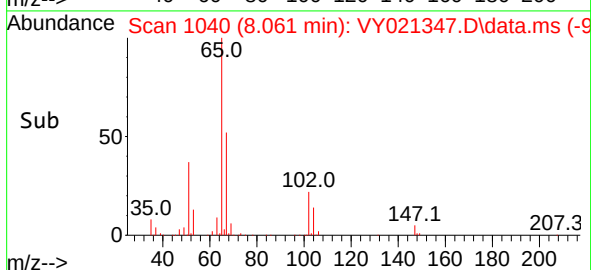
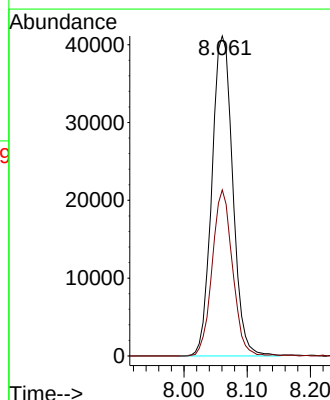
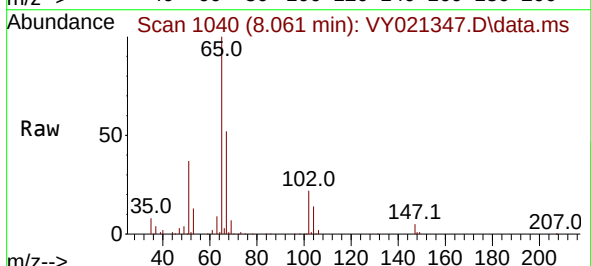


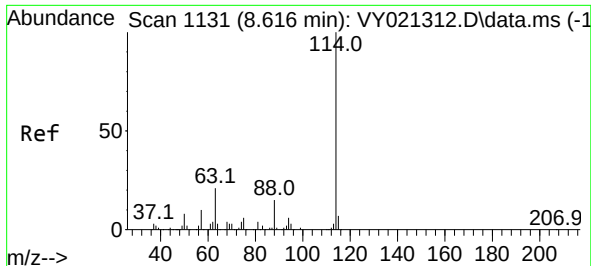

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY021347.D
Acq: 27 Feb 2025 10:42




Instrument :
MSVOA_Y
ClientSampleId :
VY0227SBL01


Tgt Ion:114 Resp: 264026
Ion Ratio Lower Upper
114 100
63 20.1 0.0 42.2
88 15.7 0.0 29.8

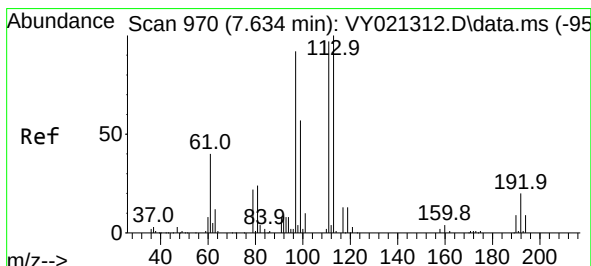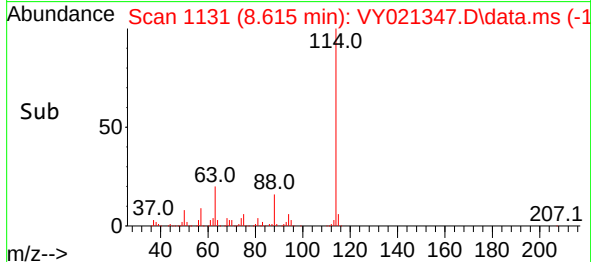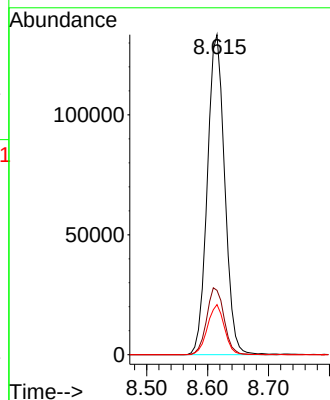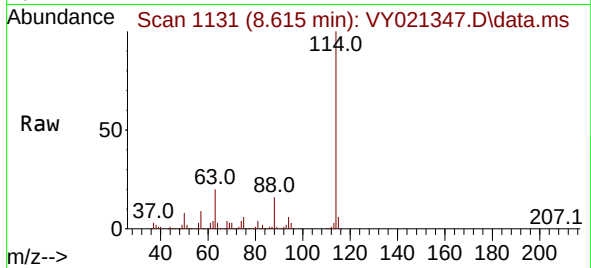

#35
Dibromofluoromethane
Concen: 52.539 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY021347.D
Acq: 27 Feb 2025 10:42

Tgt Ion:113 Resp: 90944
Ion Ratio Lower Upper
113 100
111 103.0 81.0 121.6
192 20.3 15.8 23.8

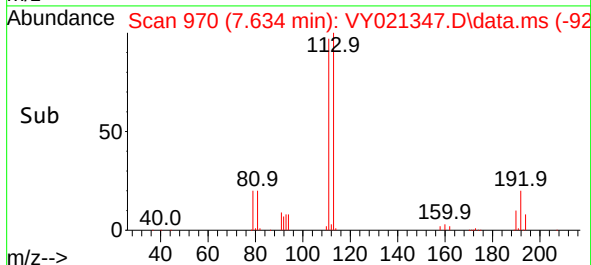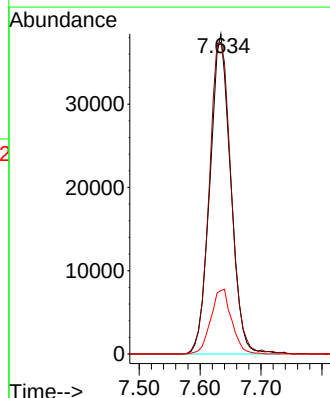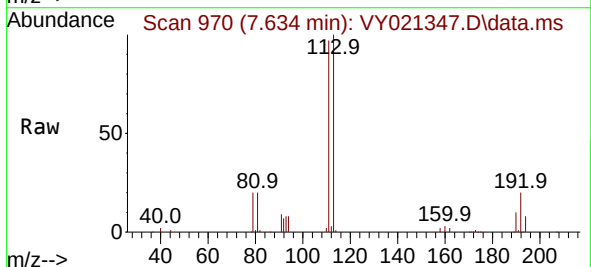

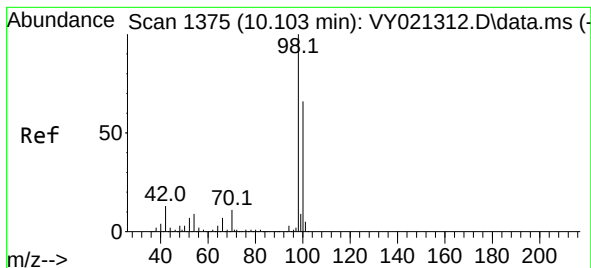

#50

Toluene-d8

Concen: 48.176 ug/l

RT: 10.109 min Scan# 1375

Delta R.T. 0.006 min

Lab File: VY021347.D

Acq: 27 Feb 2025 10:42

Instrument :

MSVOA_Y

ClientSampleId :





VY0227SBL01

Tgt Ion: 98 Resp: 322284

Ion Ratio Lower Upper

98 100

100 65.0 52.4 78.6

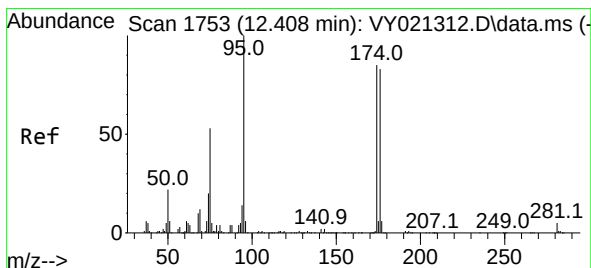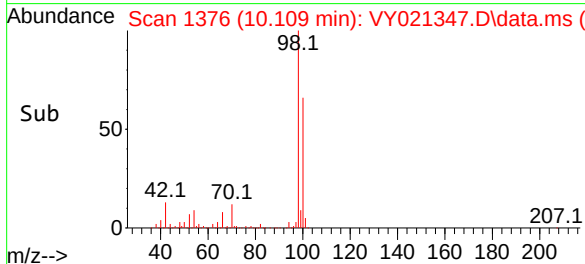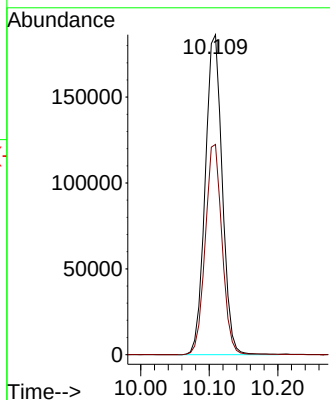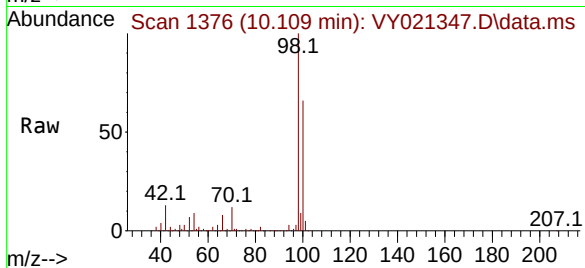

#62

4-Bromofluorobenzene

Concen: 49.533 ug/l

RT: 12.407 min Scan# 1753

Delta R.T. -0.000 min

Lab File: VY021347.D

Acq: 27 Feb 2025 10:42




Tgt Ion: 95 Resp: 111519


Ion Ratio Lower Upper

95 100

174 83.8 0.0 168.0

176 81.7 0.0 162.6


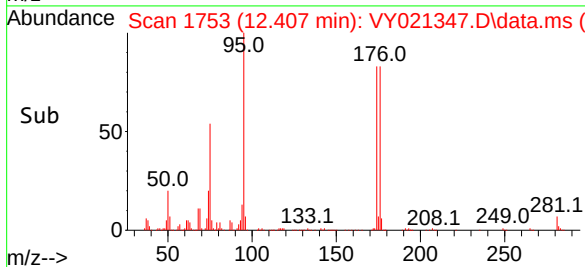
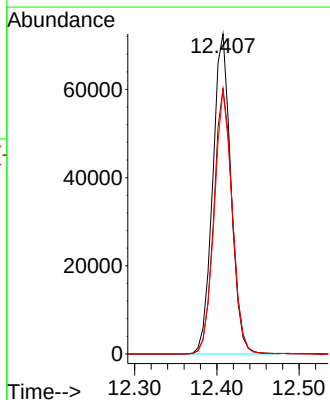
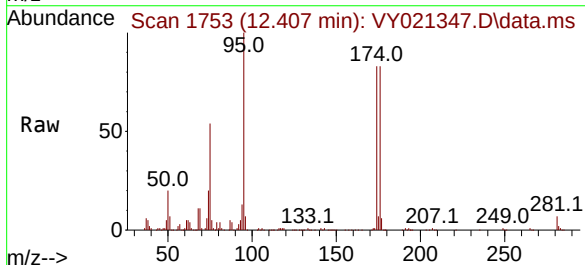


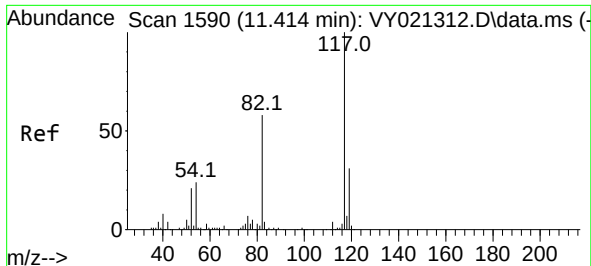

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VY021347.D
Acq: 27 Feb 2025 10:42

Instrument :
MSVOA_Y
ClientSampleId :
VY0227SBL01

Tgt Ion:117 Resp: 255103
Ion Ratio Lower Upper
117 100
82 56.3 46.2 69.4
119 32.3 24.9 37.3

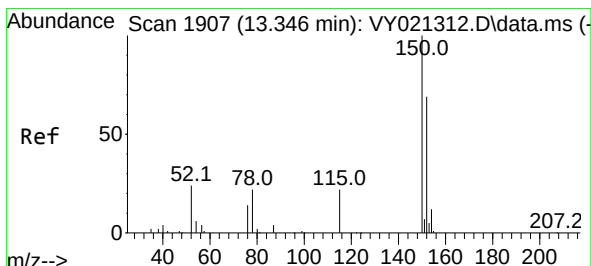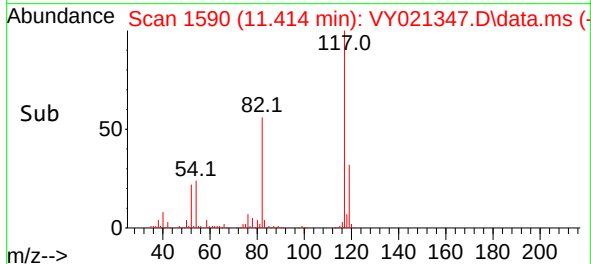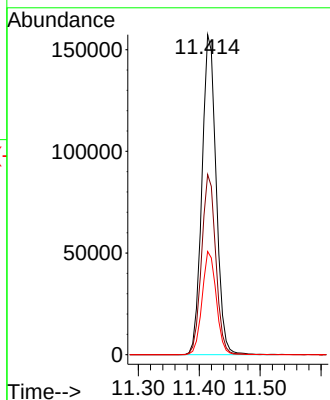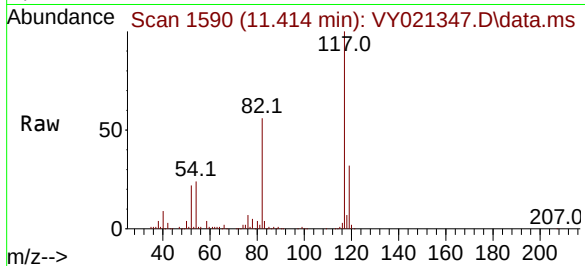

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VY021347.D
Acq: 27 Feb 2025 10:42

Tgt Ion:152 Resp: 107368
Ion Ratio Lower Upper
152 100
115 58.5 29.3 88.0
150 157.4 0.0 347.4

