

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL121624

Review By	SAM	Review On	12/18/2024 8:48:10 AM
Supervise By		Supervise On	
SubDirectory	VL121624	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL121624AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2556		
Initial Calibration Stds	AP2560,AP2561,AP2562		
CCC	AP2560,MDL,AP2561,AP2562		
Internal Standard/PEM	AP2556		
ICV/I.BLK	AP2558		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL041750.D	16 Dec 2024 12:02	SY/MD	Ok
2	VSTDICC0.5	VL041751.D	16 Dec 2024 12:59	SY/MD	Not Ok
3	VSTDICCC010	VL041752.D	16 Dec 2024 13:30	SY/MD	Ok,M
4	VSTDICC002	VL041753.D	16 Dec 2024 14:03	SY/MD	Ok,M
5	VSTDICC001	VL041754.D	16 Dec 2024 14:34	SY/MD	Ok,M
6	VSTDICC0.5	VL041755.D	16 Dec 2024 15:05	SY/MD	Ok,M
7	VSTDICC0.1	VL041756.D	16 Dec 2024 15:37	SY/MD	Ok,M
8	VSTDICC0.03	VL041757.D	16 Dec 2024 16:08	SY/MD	Ok,M
9	VSTDICC015	VL041758.D	16 Dec 2024 16:41	SY/MD	Ok,M
10	VSTDICV010	VL041759.D	16 Dec 2024 18:59	SY/MD	Ok,M
11	VL1216ABL01	VL041760.D	16 Dec 2024 20:20	SY/MD	Ok
12	VL1216ABL02	VL041761.D	16 Dec 2024 20:51	SY/MD	Ok
13	VL1216ABL03	VL041762.D	16 Dec 2024 21:21	SY/MD	Ok
14	MDL 0.4	VL041763.D	16 Dec 2024 21:52	SY/MD	Ok,M
15	MDL 0.4	VL041764.D	16 Dec 2024 22:23	SY/MD	Ok,M
16	MDL 0.4	VL041765.D	16 Dec 2024 22:54	SY/MD	Ok,M
17	MDL 0.03	VL041766.D	16 Dec 2024 23:24	SY/MD	Ok,M
18	MDL 0.03	VL041767.D	16 Dec 2024 23:55	SY/MD	Ok,M
19	VL1216ABS01	VL041768.D	17 Dec 2024 00:57	SY/MD	Ok,M
20	VSTDCCC010	VL041769.D	17 Dec 2024 07:59	SY/MD	Ok,M

M : Manual Integration

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL121824

Review By	MMDadoda	Review On	12/19/2024 2:45:49 PM
Supervise By		Supervise On	
SubDirectory	VL121824	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL121624AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2556		
Initial Calibration Stds	AP2560,AP2561,AP2562		
CCC	AP2560,MDL,AP2561,AP2562		
Internal Standard/PEM	AP2556		
ICV/I.BLK	AP2558		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL041787.D	18 Dec 2024 08:06	SY/MD	Ok
2	VSTDCCC010	VL041788.D	18 Dec 2024 10:29	SY/MD	Ok,M
3	VL1218ABL01	VL041789.D	18 Dec 2024 11:57	SY/MD	Ok
4	VL1218ABL02	VL041790.D	18 Dec 2024 12:28	SY/MD	Ok
5	MDL 0.4	VL041791.D	18 Dec 2024 12:59	SY/MD	Ok,M
6	MDL 0.4	VL041792.D	18 Dec 2024 13:30	SY/MD	Ok,M
7	MDL 0.03	VL041793.D	18 Dec 2024 14:32	SY/MD	Ok,M
8	MDL 0.03	VL041794.D	18 Dec 2024 15:03	SY/MD	Ok,M
9	VL1218ABS01	VL041795.D	18 Dec 2024 16:06	SY/MD	Ok,M
10	QC121724 CAN 10158	VL041796.D	18 Dec 2024 16:37	SY/MD	Ok
11	P5293-01	VL041797.D	18 Dec 2024 17:10	SY/MD	Ok,M
12	P5293-01DUP	VL041798.D	18 Dec 2024 17:43	SY/MD	Ok,M
13	P5293-02	VL041799.D	18 Dec 2024 18:17	SY/MD	Ok,M
14	P5293-03	VL041800.D	18 Dec 2024 18:50	SY/MD	Dilution
15	P5296-01	VL041801.D	18 Dec 2024 19:24	SY/MD	Ok,M
16	P5294-01	VL041802.D	18 Dec 2024 19:58	SY/MD	Ok,M
17	P5294-02	VL041803.D	18 Dec 2024 20:32	SY/MD	Ok,M
18	P5294-03	VL041804.D	18 Dec 2024 21:03	SY/MD	Not Ok
19	P5292-01	VL041805.D	18 Dec 2024 21:35	SY/MD	Not Ok
20	P5292-02	VL041806.D	18 Dec 2024 22:06	SY/MD	Not Ok
21	P5295-01	VL041807.D	18 Dec 2024 22:37	SY/MD	Dilution

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL121824

Review By	MMDadoda	Review On	12/19/2024 2:45:49 PM
Supervise By		Supervise On	
SubDirectory	VL121824	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL121624AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2556		
Initial Calibration Stds	AP2560,AP2561,AP2562		
CCC	AP2560,MDL,AP2561,AP2562		
Internal Standard/PEM	AP2556		
ICV/I.BLK	AP2558		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	P5295-02DL	VL041808.D	18 Dec 2024 23:08	SY/MD	Ok,M
23	VIBLK	VL041809.D	18 Dec 2024 23:40	SY/MD	Ok
24	P5293-03DL	VL041810.D	19 Dec 2024 00:11	SY/MD	Ok,M
25	P5294-03	VL041811.D	19 Dec 2024 00:44	SY/MD	Ok,M
26	P5292-01	VL041812.D	19 Dec 2024 01:18	SY/MD	Ok,M
27	P5292-02	VL041813.D	19 Dec 2024 01:55	SY/MD	Ok,M
28	P5295-01DL	VL041814.D	19 Dec 2024 02:26	SY/MD	Ok,M
29	P5295-02	VL041815.D	19 Dec 2024 02:59	SY/MD	Dilution
30	VSTDCCC010	VL041816.D	19 Dec 2024 03:31	SY/MD	Ok

M : Manual Integration

Process Report

Order ID : q1419



Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
02/24/2025	B2502026	Q1419-02	-3.9	10492	6 L	10528		C2412002	VL041796.D Seq :vl121824 TUNE : VL041787.D ICAL : VL041757.D CCAL : VL041788.D MB : VL041790.D
02/24/2025	B2502026	Q1419-01	-4.7	10267	6 L	10550		C2412002	VL041796.D Seq :vl121824 TUNE : VL041787.D ICAL : VL041757.D CCAL : VL041788.D MB : VL041790.D

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
Data File : VL041750.D
Acq On : 16 Dec 2024 12:02
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Dec 19 07:32:09 2024

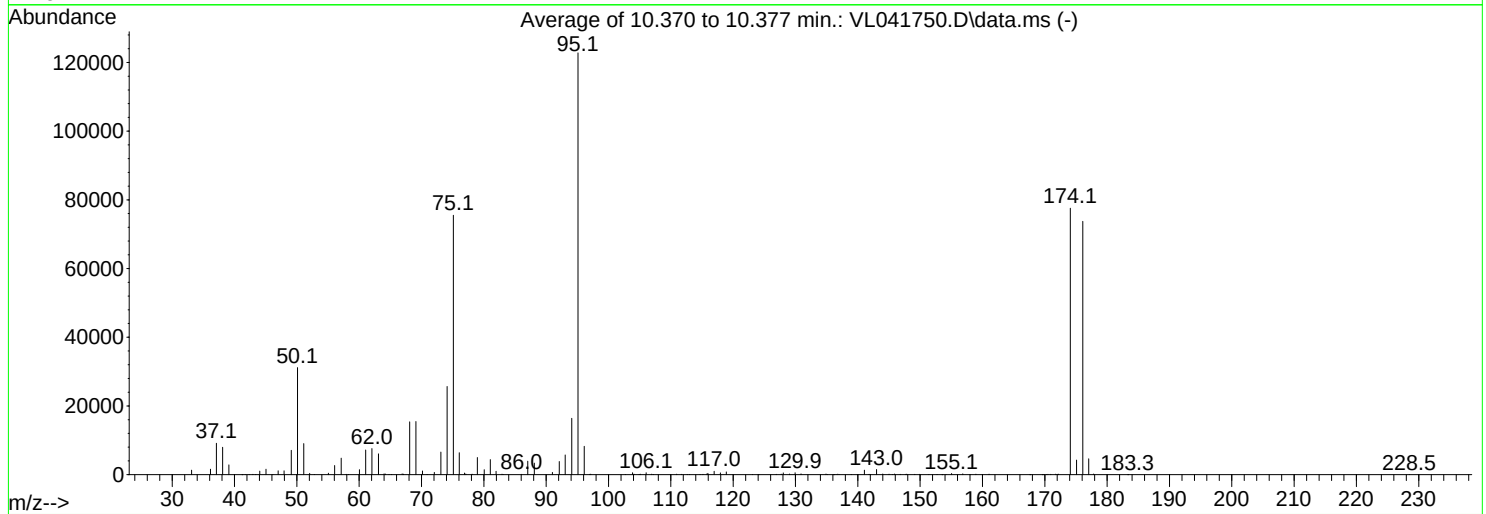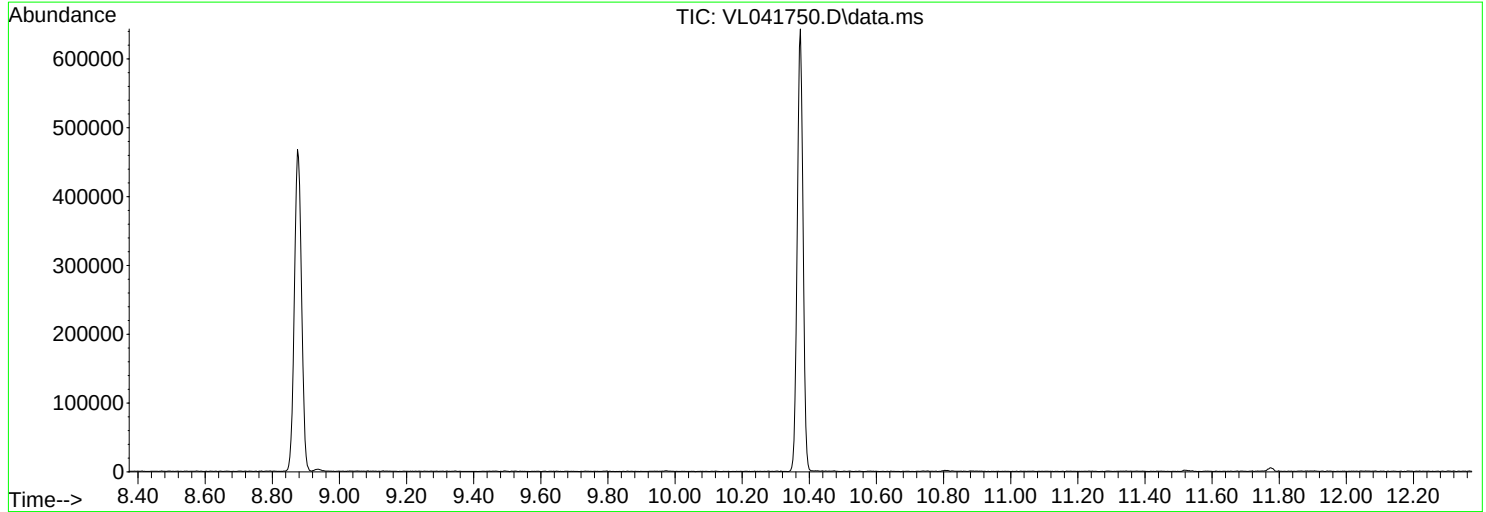

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3162

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	25.4	31157	PASS
75	95	30	66	61.5	75504	PASS
95	95	100	100	100.0	122797	PASS
96	95	5	9	6.7	8239	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.2	77565	PASS
175	174	4	9	5.5	4234	PASS
176	174	93	101	95.0	73717	PASS
177	176	5	9	6.3	4630	PASS

Average of 10.370 to 10.377 min.: VL041750.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1322	44.05	1016	56.05	2649	65.20	61
36.15	1587	45.05	1575	57.10	4784	66.90	24
37.10	9134	46.15	66	57.90	94	67.10	12
38.10	7991	47.00	1132	58.30	32	68.10	1535
39.10	2839	47.95	1114	60.05	1454	69.10	15463
40.00	41	49.10	7069	61.05	7192	70.15	1071
41.20	26	50.10	31157	62.05	7600	70.90	28
41.70	49	51.10	9016	63.10	6081	72.05	651
42.35	60	52.05	392	64.00	224	73.10	6573
42.95	115	52.80	56	64.20	202	74.10	25661
43.40	59	55.05	422	64.80	43	75.10	75504

Average of 10.370 to 10.377 min.: VL041750.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	6364	87.05	3899	103.85	544	113.00	66
76.90	489	88.10	3363	104.10	151	114.70	31
77.10	175	91.00	654	104.90	42	115.15	90
78.10	122	92.10	3845	105.10	151	115.80	221
78.95	4994	93.05	5724	106.05	566	115.95	358
80.05	1429	94.10	16382	106.95	120	116.95	974
81.05	4383	95.10	122797	107.20	40	117.95	511
81.95	969	96.10	8239	109.95	51	118.90	777
82.90	123	97.00	110	110.95	130	123.10	50
83.10	33	97.15	142	111.70	88	124.00	17
86.05	99	102.70	65	112.65	61	126.90	78

Average of 10.370 to 10.377 min.: VL041750.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.70	134	138.95	48	147.70	72	158.95	148
128.05	509	140.00	35	147.85	142	161.05	144
129.05	205	141.05	1317	149.15	97	167.60	18
129.95	553	141.80	73	149.90	118	169.60	17
130.90	245	142.00	67	151.40	43	169.90	39
134.90	170	143.00	1489	152.70	31	170.30	41
135.10	61	144.00	186	153.50	25	170.50	88
136.10	17	145.00	136	154.15	44	170.95	118
136.50	51	145.60	39	155.05	332	171.75	129
136.80	153	145.90	181	156.85	228	172.00	95
137.00	50	146.80	77	158.00	44	172.20	138

Average of 10.370 to 10.377 min.: VL041750.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.10	77565						
175.10	4234						
176.10	73717						
177.05	4630						
177.85	181						
183.30	17						
228.50	47						

Instrument :

MSVOA_L

ClientSampleId :

BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041752.D
 Acq On : 16 Dec 2024 13:30
 Operator : SY/MD
 Sample : VSTDICCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICCC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:11:54 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	68599	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.956	114	183786	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.879	117	163333	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.374 95 138451 10.172 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 101.700%

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	1.496	85	115385	9.453 ppbv	100
3) Chlorodifluoromethane	1.473	51	107429	9.603 ppbv	100
4) Chloromethane	1.531	50	43215	9.049 ppbv	100
5) Vinyl Chloride	1.580	62	42849	8.905 ppbv	100
6) Bromomethane	1.667	94	20252	8.919 ppbv	100
7) Chloroethane	1.703	64	17403	9.311 ppbv	100
8) Dichlorotetrafluoroethane	1.554	85	100191	9.171 ppbv	100
9) Propene	1.483	41	43440	8.959 ppbv	100
10) Heptane	4.979	43	116969	9.391 ppbv	100
11) Trichlorofluoromethane	1.875	101	122831	9.474 ppbv	100
12) 1,1,2-Trichlorotrifluo...	2.137	101	91977	9.327 ppbv	100
13) Ethanol	1.719	45	2484	6.161 ppbv	100
14) Bromoethene	1.781	108	32528	9.770 ppbv	100
15) Acetone	1.832	43	100229	7.509 ppbv	100
16) 1,3-Butadiene	1.606	39	46989	8.940 ppbv	100
17) tert-Butyl alcohol	2.036	59	125757	9.497 ppbv	100
18) 1,1-Dichloroethene	2.033	96	38775	9.379 ppbv	100
19) Isopropyl Alcohol	1.884	45	59026	7.370 ppbv	100
20) Methylene Chloride	2.059	84	32734	8.601 ppbv	100
21) Allyl Chloride	2.095	41	69406	9.588 ppbv	100
22) trans-1,2-Dichloroethene	2.337	96	43898	9.276 ppbv	100
23) Vinyl Acetate	2.457	43	54227	9.350 ppbv	100
24) 1,1-Dichloroethane	2.405	63	89912	9.386 ppbv	100
25) Ethyl Acetate	2.833	43	235305	9.432 ppbv	100
26) Hexane	2.823	57	89385	9.486 ppbv	100
27) Carbon Disulfide	2.150	76	92329	10.873 ppbv	100
28) Methyl tert-Butyl Ether	2.438	73	75330	9.854 ppbv	100
29) Chloroform	2.846	83	135099	9.408 ppbv	100
30) Cyclohexane	3.855	84	75156	9.374 ppbv	100
31) cis-1,2-Dichloroethene	2.719	61	91276	9.374 ppbv	100
32) 1,1,1-Trichloroethane	3.363	97	139102	9.733 ppbv	100
34) 2-Butanone	2.554	43	135331	9.153 ppbv	100
35) Carbon Tetrachloride	3.758	117	138952	10.650 ppbv	100
36) Benzene	3.655	78	179134	9.423 ppbv	100
37) 1,2-Dichloroethane	3.215	62	111770	9.449 ppbv	100
38) Trichloroethene	4.545	130	71297	8.907 ppbv	100
39) 1,2-Dichloropropane	4.309	63	64789	9.423 ppbv	100
40) 1,4-Dioxane	4.580	88	30658	9.128 ppbv #	100
41) Tetrahydrofuran	3.049	42	78480	9.474 ppbv	100
42) Bromodichloromethane	4.483	83	142819	10.494 ppbv	100
43) Methyl Methacrylate	4.878	69	72578	10.020 ppbv	100
44) 2,2,4-Trimethylpentane	4.639	57	307748	9.479 ppbv	100
45) t-1,3-Dichloropropene	6.412	75	77752	10.378 ppbv	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041752.D
 Acq On : 16 Dec 2024 13:30
 Operator : SY/MD
 Sample : VSTDICCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICCC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:11:54 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	97992	10.303	ppbv	100
47) 1,1,2-Trichloroethane	6.577	97	67550	9.406	ppbv	100
48) Dibromochloromethane	7.383	129	108899	11.105	ppbv	100
49) Bromoform	9.481	173	91587	11.410	ppbv	100
50) 4-Methyl-2-Pentanone	5.749	43	194838	9.678	ppbv	100
51) 2-Hexanone	7.432	43	157473	9.650	ppbv	100
52) Tetrachloroethene	8.222	164	62989	8.901	ppbv	100
53) Toluene	6.930	91	206354	9.574	ppbv	100
54) 1,2-Dibromoethane	7.649	107	94016	9.501	ppbv	100
56) 1,1,1,2-Tetrachloroethane	8.924	131	86831	10.027	ppbv	100
57) Chlorobenzene	8.921	112	155349	9.295	ppbv	100
58) Ethyl Benzene	9.354	91	289734	9.853	ppbv	100
59) m/p-Xylene	9.549	91	462802m	19.568	ppbv	
60) o-Xylene	9.963	91	232101	9.789	ppbv	100
61) Styrene	9.869	104	110041	10.733	ppbv	100
62) Isopropylbenzene	10.539	105	348684	9.788	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.963	83	137363	9.255	ppbv	100
64) n-propylbenzene	10.989	120	87360	9.700	ppbv	100
65) tert-Butylbenzene	11.529	119	309036	9.615	ppbv	100
66) Benzyl Chloride	11.614	91	31039	10.954	ppbv	100
67) sec-Butylbenzene	11.769	105	430810	9.687	ppbv	100
69) p-Isopropyltoluene	11.924	119	363072	9.906	ppbv	100
70) n-Butylbenzene	12.280	91	358993	10.137	ppbv	100
71) 2-Chlorotoluene	10.902	91	264002	9.708	ppbv	100
72) 4-Ethyltoluene	11.125	105	282698	10.120	ppbv	100
73) 1,3,5-Trimethylbenzene	11.203	105	239261	10.304	ppbv	100
74) 1,2,4-Trimethylbenzene	11.536	105	255780	10.244	ppbv	100
75) 1,3-Dichlorobenzene	11.607	146	151752	9.532	ppbv	100
76) 1,4-Dichlorobenzene	11.672	146	152099	9.671	ppbv	100
77) 1,2-Dichlorobenzene	11.947	146	141338	9.227	ppbv	100
78) Hexachloro-1,3-Butadiene	13.882	225	95751	8.431	ppbv	100
79) Naphthalene	13.514	128	205511	11.812	ppbv	100
80) Naphthalene,2-methyl-	14.459	142	106311	19.755	ppbv	100
81) 1,2,4-Trichlorobenzene	13.439	180	101461	10.672	ppbv	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041753.D
 Acq On : 16 Dec 2024 14:03
 Operator : SY/MD
 Sample : VSTDICC002
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC002

Quant Time: Dec 19 06:12:42 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/20/2024
 Supervised By : Mahesh Dadoda 12/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	67443	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	182992	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.882	117	163971	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.377 95 138312 10.122 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 101.200%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	24819	2.068	ppbv	98
3) Chlorodifluoromethane	1.476	51	22299	2.027	ppbv	96
4) Chloromethane	1.531	50	9926	2.114	ppbv	99
5) Vinyl Chloride	1.580	62	9300	1.966	ppbv	99
6) Bromomethane	1.667	94	4625	2.072	ppbv	99
7) Chloroethane	1.706	64	4003	2.178	ppbv #	85
8) Dichlorotetrafluoroethane	1.554	85	21791	2.029	ppbv	100
9) Propene	1.483	41	10115	2.122	ppbv	97
10) Heptane	4.978	43	25297	2.066	ppbv	100
11) Trichlorofluoromethane	1.878	101	26208	2.056	ppbv	96
12) 1,1,2-Trichlorotrifluo...	2.140	101	19770	2.039	ppbv	99
13) Ethanol	1.722	45	792	1.998	ppbv #	49
14) Bromoethene	1.784	108	6527	1.994	ppbv #	90
15) Acetone	1.835	43	27613	2.104	ppbv	99
16) 1,3-Butadiene	1.609	39	10478	2.028	ppbv	96
17) tert-Butyl alcohol	2.043	59	26646	2.047	ppbv	99
18) 1,1-Dichloroethene	2.033	96	8389	2.064	ppbv	92
19) Isopropyl Alcohol	1.887	45	14937	1.897	ppbv	93
20) Methylene Chloride	2.062	84	7586	2.027	ppbv	94
21) Allyl Chloride	2.094	41	14731	2.070	ppbv	99
22) trans-1,2-Dichloroethene	2.340	96	9407	2.022	ppbv	94
23) Vinyl Acetate	2.463	43	17652	3.096	ppbv #	95
24) 1,1-Dichloroethane	2.408	63	19070	2.025	ppbv	99
25) Ethyl Acetate	2.836	43	50510	2.059	ppbv	99
26) Hexane	2.826	57	19200	2.073	ppbv	98
27) Carbon Disulfide	2.153	76	16214	1.942	ppbv #	34
28) Methyl tert-Butyl Ether	2.441	73	15039	2.001	ppbv	98
29) Chloroform	2.849	83	28843	2.043	ppbv	98
30) Cyclohexane	3.858	84	16384	2.079	ppbv	99
31) cis-1,2-Dichloroethene	2.719	61	19688	2.057	ppbv	96
32) 1,1,1-Trichloroethane	3.370	97	28341	2.017	ppbv	98
34) 2-Butanone	2.557	43	31483	2.138	ppbv	99
35) Carbon Tetrachloride	3.765	117	27727	2.134	ppbv	98
36) Benzene	3.658	78	38759	2.048	ppbv	94
37) 1,2-Dichloroethane	3.221	62	23800	2.021	ppbv	98
38) Trichloroethene	4.548	130	15660	1.965	ppbv	94
39) 1,2-Dichloropropane	4.315	63	14197	2.074	ppbv	94
40) 1,4-Dioxane	4.603	88	6826m	2.041	ppbv	
41) Tetrahydrofuran	3.059	42	16665	2.021	ppbv	96
42) Bromodichloromethane	4.489	83	26716	1.972	ppbv	98
43) Methyl Methacrylate	4.884	69	14849	2.059	ppbv	100
44) 2,2,4-Trimethylpentane	4.642	57	67432	2.086	ppbv	100
45) t-1,3-Dichloropropene	6.415	75	14885	1.995	ppbv	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041753.D
 Acq On : 16 Dec 2024 14:03
 Operator : SY/MD
 Sample : VSTDICC002
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC002

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:12:42 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LFri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.606	75	19105m	2.017	ppbv	
47) 1,1,2-Trichloroethane	6.584	97	14858	2.078	ppbv	89
48) Dibromochloromethane	7.390	129	19764	2.024	ppbv	98
49) Bromoform	9.484	173	16200	2.027	ppbv	98
50) 4-Methyl-2-Pentanone	5.758	43	42045	2.098	ppbv	97
51) 2-Hexanone	7.441	43	34878	2.147	ppbv #	98
52) Tetrachloroethene	8.225	164	13612	1.932	ppbv	93
53) Toluene	6.933	91	44470	2.072	ppbv	99
54) 1,2-Dibromoethane	7.655	107	19820	2.012	ppbv	91
56) 1,1,1,2-Tetrachloroethane	8.924	131	18613	2.141	ppbv	98
57) Chlorobenzene	8.920	112	35685	2.127	ppbv	99
58) Ethyl Benzene	9.354	91	63316	2.145	ppbv	97
59) m/p-Xylene	9.535	91	99821m	4.204	ppbv	
60) o-Xylene	9.966	91	51152	2.149	ppbv	99
61) Styrene	9.872	104	20842	2.025	ppbv	96
62) Isopropylbenzene	10.539	105	75206	2.103	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.966	83	29751	1.997	ppbv	100
64) n-propylbenzene	10.992	120	19146	2.117	ppbv	99
65) tert-Butylbenzene	11.532	119	68879	2.135	ppbv	98
66) Benzyl Chloride	11.617	91	5400	1.898	ppbv	99
67) sec-Butylbenzene	11.769	105	95968	2.149	ppbv	100
69) p-Isopropyltoluene	11.927	119	79236	2.153	ppbv	100
70) n-Butylbenzene	12.283	91	75430	2.122	ppbv	99
71) 2-Chlorotoluene	10.901	91	57724	2.114	ppbv	99
72) 4-Ethyltoluene	11.125	105	58841	2.098	ppbv	99
73) 1,3,5-Trimethylbenzene	11.206	105	48645	2.087	ppbv	97
74) 1,2,4-Trimethylbenzene	11.539	105	53084	2.118	ppbv	96
75) 1,3-Dichlorobenzene	11.610	146	32609	2.040	ppbv	98
76) 1,4-Dichlorobenzene	11.675	146	32527	2.060	ppbv	98
77) 1,2-Dichlorobenzene	11.950	146	32223	2.095	ppbv	100
78) Hexachloro-1,3-Butadiene	13.882	225	25358	2.224	ppbv	98
79) Naphthalene	13.513	128	37855	2.167	ppbv	100
80) Naphthalene,2-methyl-	14.462	142	4482	0.830	ppbv	94
81) 1,2,4-Trichlorobenzene	13.442	180	19425	2.035	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041754.D
 Acq On : 16 Dec 2024 14:34
 Operator : SY/MD
 Sample : VSTDICC001
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC001

Quant Time: Dec 19 06:13:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Thu Dec 19 06:09:59 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/20/2024
 Supervised By : Mahesh Dadoda 12/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	65928	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.955	114	178926	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	162267	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.374	95	132857	9.825	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.300%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.496	85	12706	1.083	ppbv	98
3) Chlorodifluoromethane	1.473	51	11187	1.041	ppbv	98
4) Chloromethane	1.531	50	4805	1.047	ppbv	99
5) Vinyl Chloride	1.580	62	4580	0.990	ppbv	98
6) Bromomethane	1.667	94	2394	1.097	ppbv	99
7) Chloroethane	1.703	64	1763	0.981	ppbv	95
8) Dichlorotetrafluoroethane	1.554	85	10938	1.042	ppbv	99
9) Propene	1.483	41	4840	1.039	ppbv	94
10) Heptane	4.972	43	12004	1.003	ppbv	93
11) Trichlorofluoromethane	1.874	101	12625	1.013	ppbv	94
12) 1,1,2-Trichlorotrifluo...	2.136	101	9915	1.046	ppbv	98
13) Ethanol	1.719	45	525m	1.355	ppbv	
14) Bromoethene	1.780	108	3148	0.984	ppbv #	86
15) Acetone	1.832	43	15060	1.174	ppbv	99
16) 1,3-Butadiene	1.609	39	5137	1.017	ppbv	95
17) tert-Butyl alcohol	2.039	59	13341	1.048	ppbv	96
18) 1,1-Dichloroethene	2.033	96	4139	1.042	ppbv	96
19) Isopropyl Alcohol	1.884	45	8703	1.131	ppbv	100
20) Methylene Chloride	2.059	84	3868	1.057	ppbv	92
21) Allyl Chloride	2.094	41	7425	1.067	ppbv	98
22) trans-1,2-Dichloroethene	2.337	96	4599	1.011	ppbv	96
23) Vinyl Acetate	2.460	43	5345	0.959	ppbv #	95
24) 1,1-Dichloroethane	2.408	63	9621	1.045	ppbv	98
25) Ethyl Acetate	2.836	43	25141	1.049	ppbv	99
26) Hexane	2.826	57	9250	1.021	ppbv	93
27) Carbon Disulfide	2.149	76	8152	0.999	ppbv #	19
28) Methyl tert-Butyl Ether	2.441	73	8539	1.162	ppbv	94
29) Chloroform	2.845	83	14384	1.042	ppbv	96
30) Cyclohexane	3.852	84	7824	1.015	ppbv	94
31) cis-1,2-Dichloroethene	2.719	61	10013	1.070	ppbv	96
32) 1,1,1-Trichloroethane	3.363	97	14415	1.049	ppbv	98
34) 2-Butanone	2.557	43	14673	1.019	ppbv	99
35) Carbon Tetrachloride	3.761	117	12808m	1.008	ppbv	
36) Benzene	3.651	78	19331	1.044	ppbv	97
37) 1,2-Dichloroethane	3.214	62	11490	0.998	ppbv #	94
38) Trichloroethene	4.551	130	7824m	1.004	ppbv	
39) 1,2-Dichloropropane	4.311	63	7068	1.056	ppbv	86
40) 1,4-Dioxane	4.596	88	3241	0.991	ppbv #	40
41) Tetrahydrofuran	3.062	42	8727	1.082	ppbv	97
42) Bromodichloromethane	4.489	83	13154	0.993	ppbv	100
43) Methyl Methacrylate	4.875	69	7044m	0.999	ppbv	
44) 2,2,4-Trimethylpentane	4.638	57	32361	1.024	ppbv	97
45) t-1,3-Dichloropropene	6.412	75	7027	0.963	ppbv	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041754.D
 Acq On : 16 Dec 2024 14:34
 Operator : SY/MD
 Sample : VSTDICC001
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:13:31 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LFri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	8815m	0.952	ppbv	
47) 1,1,2-Trichloroethane	6.587	97	7189m	1.028	ppbv	
48) Dibromochloromethane	7.383	129	8817	0.924	ppbv	97
49) Bromoform	9.480	173	7073	0.905	ppbv	96
50) 4-Methyl-2-Pentanone	5.761	43	20212	1.031	ppbv	100
51) 2-Hexanone	7.441	43	16514	1.040	ppbv #	99
52) Tetrachloroethene	8.225	164	7067m	1.026	ppbv	
53) Toluene	6.930	91	21594	1.029	ppbv	100
54) 1,2-Dibromoethane	7.648	107	9758	1.013	ppbv	96
56) 1,1,1,2-Tetrachloroethane	8.924	131	8643	1.005	ppbv	93
57) Chlorobenzene	8.920	112	17500	1.054	ppbv	97
58) Ethyl Benzene	9.351	91	29762	1.019	ppbv	98
59) m/p-Xylene	9.529	91	47599m	2.026	ppbv	
60) o-Xylene	9.963	91	24210	1.028	ppbv	98
61) Styrene	9.869	104	9707	0.953	ppbv	100
62) Isopropylbenzene	10.539	105	36251	1.024	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.963	83	14752	1.001	ppbv	98
64) n-propylbenzene	10.985	120	9432	1.054	ppbv	91
65) tert-Butylbenzene	11.529	119	32887	1.030	ppbv	100
66) Benzyl Chloride	11.610	91	2518	0.894	ppbv	97
67) sec-Butylbenzene	11.765	105	45015	1.019	ppbv	98
69) p-Isopropyltoluene	11.924	119	36298	0.997	ppbv	98
70) n-Butylbenzene	12.280	91	35432	1.007	ppbv	98
71) 2-Chlorotoluene	10.901	91	27561	1.020	ppbv	97
72) 4-Ethyltoluene	11.125	105	26921	0.970	ppbv	98
73) 1,3,5-Trimethylbenzene	11.202	105	22360	0.969	ppbv	95
74) 1,2,4-Trimethylbenzene	11.536	105	24654	0.994	ppbv	98
75) 1,3-Dichlorobenzene	11.604	146	16476	1.042	ppbv	100
76) 1,4-Dichlorobenzene	11.668	146	15774	1.010	ppbv	98
77) 1,2-Dichlorobenzene	11.947	146	15866	1.043	ppbv	97
78) Hexachloro-1,3-Butadiene	13.882	225	12266	1.087	ppbv	97
79) Naphthalene	13.513	128	16971	0.982	ppbv	96
80) Naphthalene,2-methyl-	14.458	142	1504	0.281	ppbv #	90
81) 1,2,4-Trichlorobenzene	13.439	180	8973	0.950	ppbv	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
Data File : VL041754.D
Acq On : 16 Dec 2024 14:34
Operator : SY/MD
Sample : VSTDICC001
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:13:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug
QLast Update : Thu Dec 19 06:09:59 2024
Response via : Initial Calibration

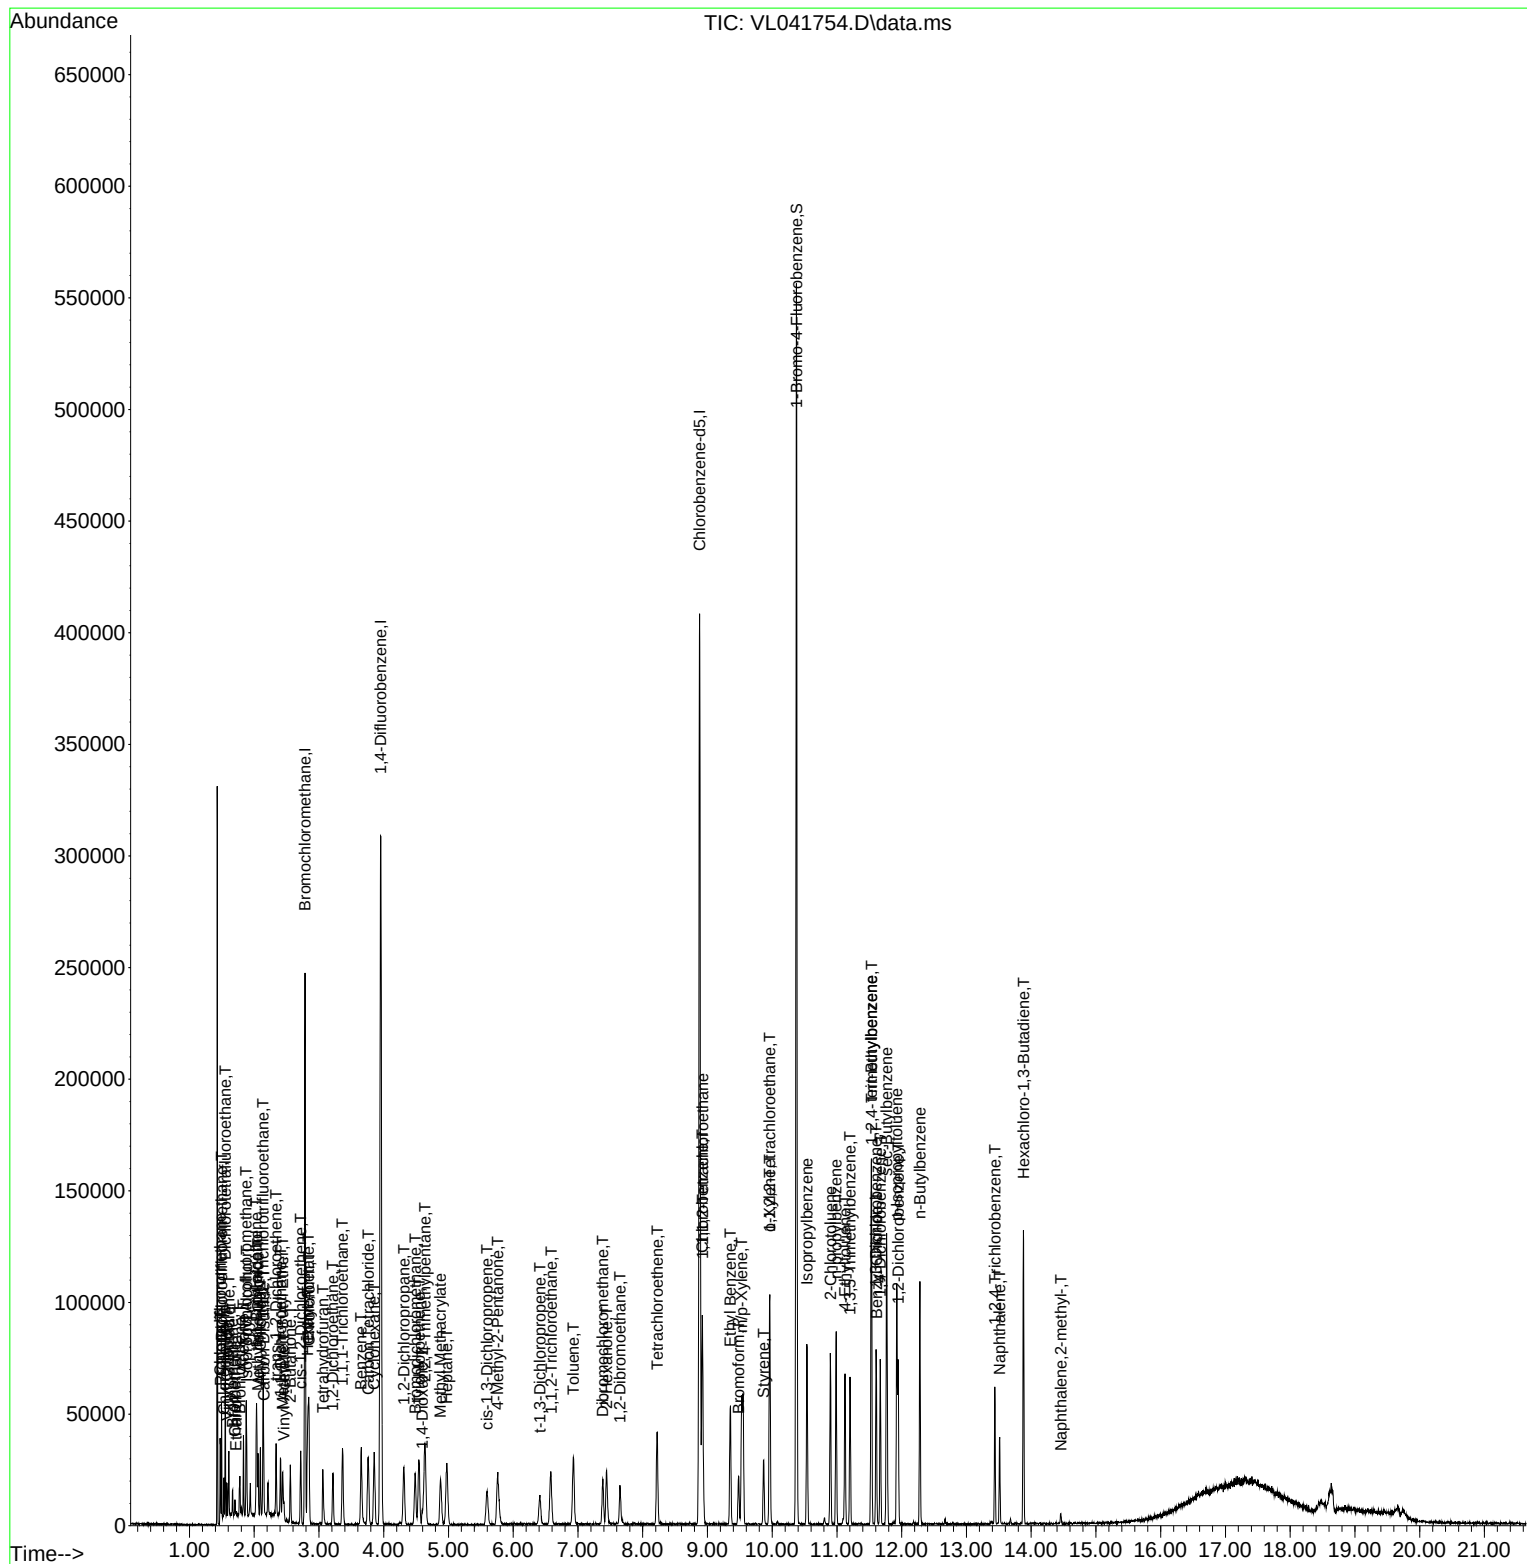

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041755.D
 Acq On : 16 Dec 2024 15:05
 Operator : SY/MD
 Sample : VSTDICC0.5
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.5

Quant Time: Dec 19 06:14:17 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/20/2024
 Supervised By : Mahesh Dadoda 12/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	66562	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.959	114	178453	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.882	117	158571	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.377 95 132273 10.010 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.100%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.496	85	6277	0.530	ppbv	94
3) Chlorodifluoromethane	1.476	51	5587	0.515	ppbv	95
4) Chloromethane	1.531	50	2452	0.529	ppbv	90
5) Vinyl Chloride	1.580	62	2269	0.486	ppbv	97
6) Bromomethane	1.667	94	1143	0.519	ppbv #	78
7) Chloroethane	1.703	64	939	0.518	ppbv	88
8) Dichlorotetrafluoroethane	1.554	85	5699	0.538	ppbv	97
9) Propene	1.483	41	2622	0.557	ppbv #	82
10) Heptane	4.978	43	6491m	0.537	ppbv	
11) Trichlorofluoromethane	1.878	101	6594	0.524	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.140	101	4962	0.519	ppbv	96
13) Ethanol	1.719	45	269m	0.688	ppbv	
14) Bromoethene	1.781	108	1694	0.524	ppbv #	93
15) Acetone	1.836	43	8233	0.636	ppbv	97
16) 1,3-Butadiene	1.609	39	2966	0.582	ppbv	88
17) tert-Butyl alcohol	2.043	59	6654	0.518	ppbv #	91
18) 1,1-Dichloroethene	2.033	96	2022	0.504	ppbv	96
19) Isopropyl Alcohol	1.884	45	5687	0.732	ppbv #	39
20) Methylene Chloride	2.062	84	2174	0.589	ppbv #	91
21) Allyl Chloride	2.098	41	3354	0.478	ppbv	86
22) trans-1,2-Dichloroethene	2.341	96	2494	0.543	ppbv	83
23) Vinyl Acetate	2.464	43	2599	0.462	ppbv #	98
24) 1,1-Dichloroethane	2.409	63	4854	0.522	ppbv #	97
25) Ethyl Acetate	2.839	43	12040	0.497	ppbv #	97
26) Hexane	2.829	57	4735	0.518	ppbv	96
27) Carbon Disulfide	2.153	76	3409	0.414	ppbv #	37
28) Methyl tert-Butyl Ether	2.441	73	3438	0.464	ppbv	99
29) Chloroform	2.849	83	7172	0.515	ppbv	98
30) Cyclohexane	3.859	84	4051	0.521	ppbv	96
31) cis-1,2-Dichloroethene	2.723	61	4758	0.504	ppbv	91
32) 1,1,1-Trichloroethane	3.367	97	7182	0.518	ppbv	99
34) 2-Butanone	2.557	43	7756	0.540	ppbv	94
35) Carbon Tetrachloride	3.765	117	5655	0.446	ppbv	90
36) Benzene	3.658	78	9629	0.522	ppbv	97
37) 1,2-Dichloroethane	3.218	62	6154	0.536	ppbv	99
38) Trichloroethene	4.551	130	3637m	0.468	ppbv	
39) 1,2-Dichloropropane	4.318	63	3410m	0.511	ppbv	
40) 1,4-Dioxane	4.606	88	1892m	0.580	ppbv	
41) Tetrahydrofuran	3.066	42	4061	0.505	ppbv	99
42) Bromodichloromethane	4.490	83	5926m	0.448	ppbv	
43) Methyl Methacrylate	4.881	69	3322	0.472	ppbv	99
44) 2,2,4-Trimethylpentane	4.645	57	16294m	0.517	ppbv	
45) t-1,3-Dichloropropene	6.422	75	3406m	0.468	ppbv	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041755.D
 Acq On : 16 Dec 2024 15:05
 Operator : SY/MD
 Sample : VSTDICC0.5
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.5

Quant Time: Dec 19 06:14:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Thu Dec 19 06:09:59 2024
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 12/20/2024
 Supervised By : Mahesh Dadoda 12/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.597	75	4462m	0.483	ppbv	
47) 1,1,2-Trichloroethane	6.587	97	3636m	0.521	ppbv	
48) Dibromochloromethane	7.387	129	3865	0.406	ppbv	99
49) Bromoform	9.484	173	2928m	0.376	ppbv	
50) 4-Methyl-2-Pentanone	5.765	43	9479m	0.485	ppbv	
51) 2-Hexanone	7.451	43	7412	0.468	ppbv #	99
52) Tetrachloroethene	8.225	164	3091	0.450	ppbv #	78
53) Toluene	6.933	91	10554	0.504	ppbv	99
54) 1,2-Dibromoethane	7.658	107	4819m	0.502	ppbv	
56) 1,1,1,2-Tetrachloroethane	8.930	131	3858m	0.459	ppbv	
57) Chlorobenzene	8.927	112	8346m	0.514	ppbv	
58) Ethyl Benzene	9.358	91	13428	0.470	ppbv	97
59) m/p-Xylene	9.552	91	22560m	0.983	ppbv	
60) o-Xylene	9.963	91	10954	0.476	ppbv	98
61) Styrene	9.869	104	4314	0.433	ppbv	94
62) Isopropylbenzene	10.542	105	16953	0.490	ppbv	95
63) 1,1,2,2-Tetrachloroethane	9.966	83	7559	0.525	ppbv	98
64) n-propylbenzene	10.989	120	4126	0.472	ppbv	92
65) tert-Butylbenzene	11.529	119	15569	0.499	ppbv	99
66) Benzyl Chloride	11.620	91	1340m	0.487	ppbv	
67) sec-Butylbenzene	11.769	105	21263	0.492	ppbv	96
69) p-Isopropyltoluene	11.928	119	17041	0.479	ppbv	99
70) n-Butylbenzene	12.284	91	15671	0.456	ppbv	99
71) 2-Chlorotoluene	10.902	91	13000	0.492	ppbv	97
72) 4-Ethyltoluene	11.128	105	13324	0.491	ppbv	98
73) 1,3,5-Trimethylbenzene	11.206	105	10497	0.466	ppbv	91
74) 1,2,4-Trimethylbenzene	11.536	105	11070	0.457	ppbv #	76
75) 1,3-Dichlorobenzene	11.604	146	8107	0.525	ppbv	99
76) 1,4-Dichlorobenzene	11.672	146	7893	0.517	ppbv	97
77) 1,2-Dichlorobenzene	11.950	146	7997	0.538	ppbv	96
78) Hexachloro-1,3-Butadiene	13.882	225	6232	0.565	ppbv	98
79) Naphthalene	13.517	128	7360	0.436	ppbv	99
80) Naphthalene,2-methyl-	14.462	142	748	0.143	ppbv	94
81) 1,2,4-Trichlorobenzene	13.442	180	4248	0.460	ppbv	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041756.D
 Acq On : 16 Dec 2024 15:37
 Operator : SY/MD
 Sample : VSTDICC0.1
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:15:07 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	65926	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	177964	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	158649	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	131540	9.950	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.500%
Target Compounds						
5) Vinyl Chloride	1.580	62	444	0.096	ppbv #	78
32) 1,1,1-Trichloroethane	3.370	97	1393	0.101	ppbv	97
35) Carbon Tetrachloride	3.771	117	1170	0.093	ppbv #	84
38) Trichloroethene	4.548	130	835m	0.108	ppbv	
52) Tetrachloroethene	8.228	164	593m	0.087	ppbv	
54) 1,2-Dibromoethane	7.658	107	1005m	0.105	ppbv	
63) 1,1,2,2-Tetrachloroethane	9.966	83	1485m	0.103	ppbv	
79) Naphthalene	13.523	128	1196	0.071	ppbv #	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
Data File : VL041756.D
Acq On : 16 Dec 2024 15:37
Operator : SY/MD
Sample : VSTDICC0.1
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:15:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug
QLast Update : Thu Dec 19 06:09:59 2024
Response via : Initial Calibration

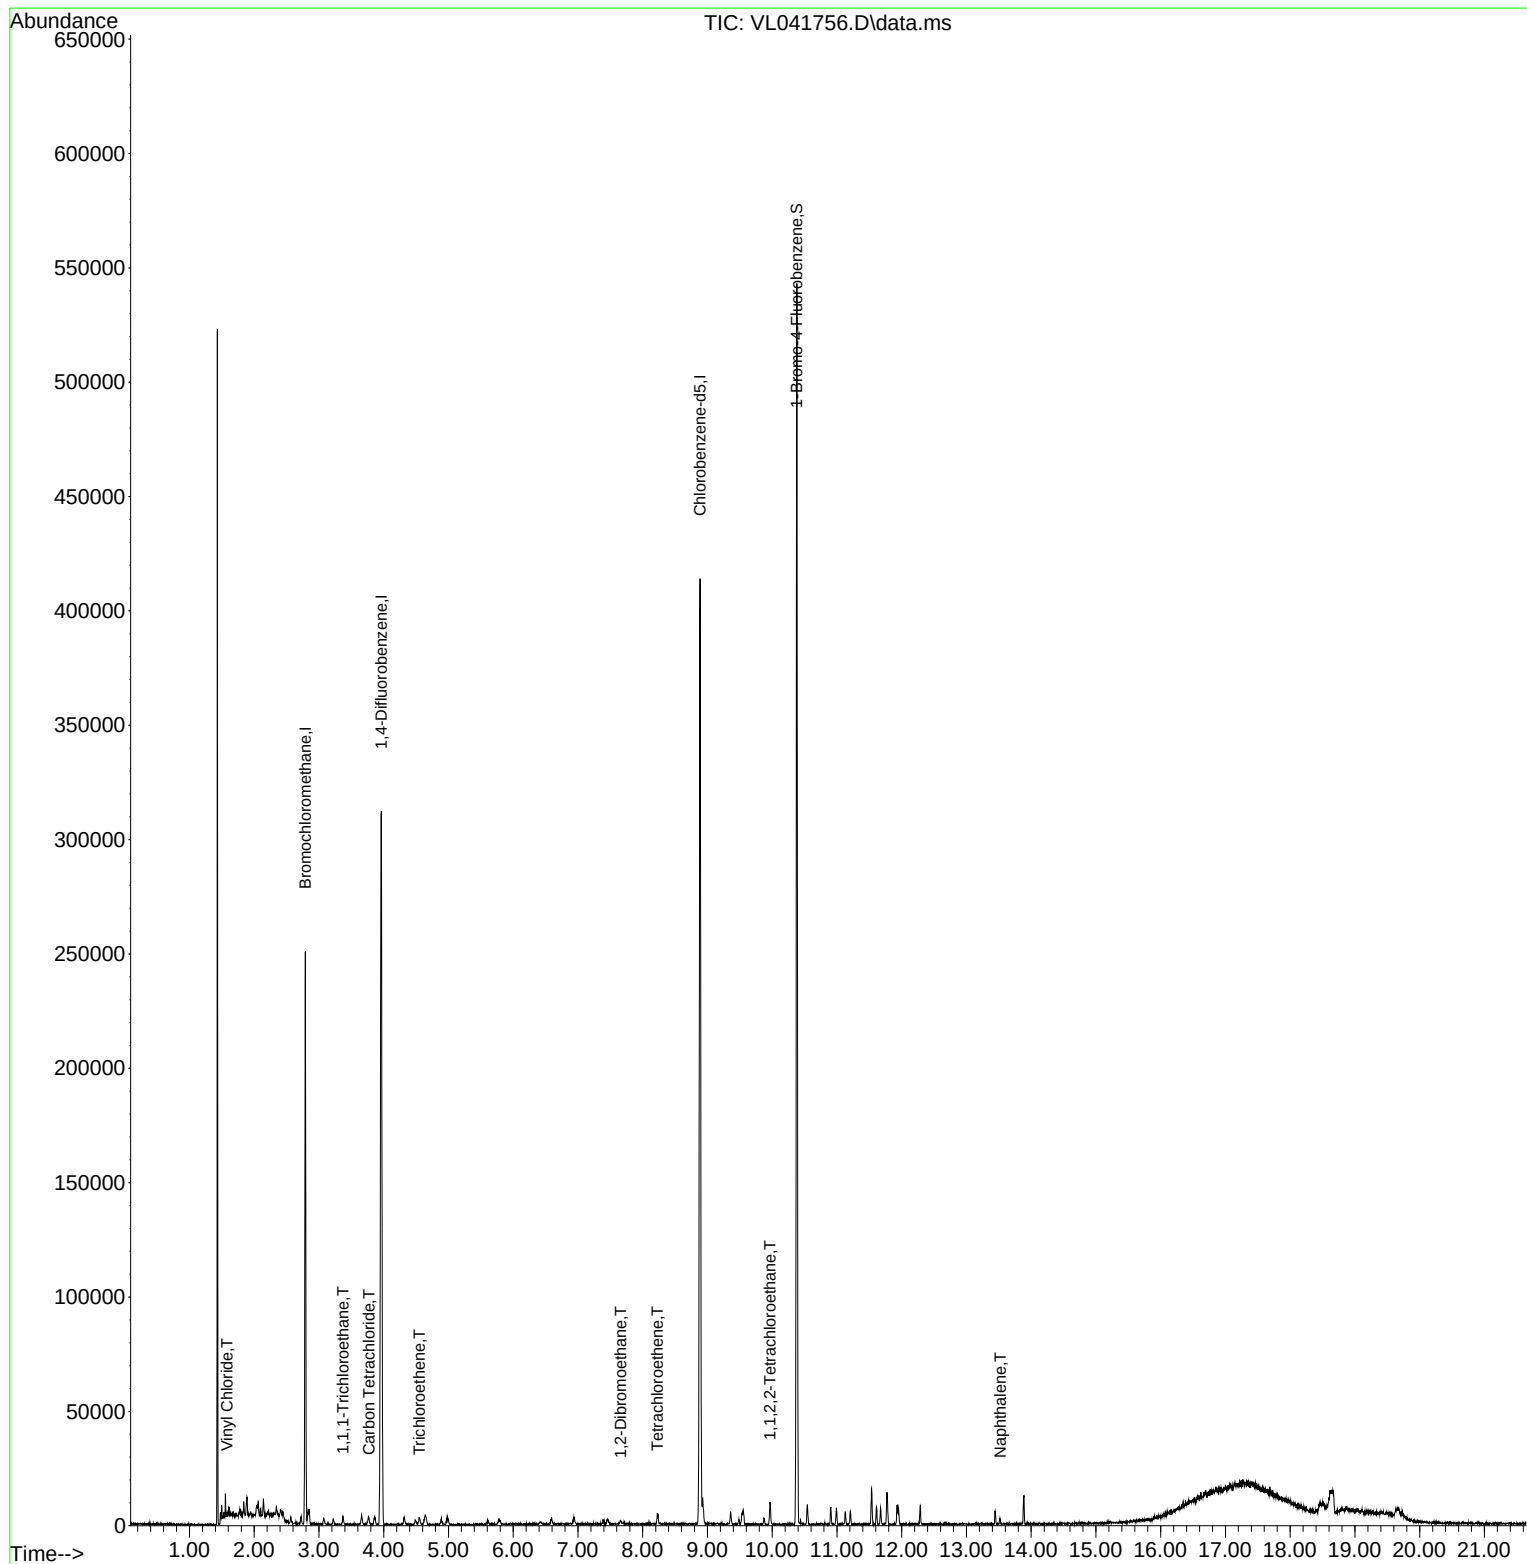

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041757.D
 Acq On : 16 Dec 2024 16:08
 Operator : SY/MD
 Sample : VSTDICC0.03
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.03

Quant Time: Dec 19 06:15:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Thu Dec 19 06:09:59 2024
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 12/20/2024
 Supervised By : Mahesh Dadoda 12/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	64158	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.958	114	174825	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	154998	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.377	95	128167	9.923	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.200%
Target Compounds						
					Qvalue	
5) Vinyl Chloride	1.580	62	175	0.039	ppbv #	84
32) 1,1,1-Trichloroethane	3.369	97	427m	0.032	ppbv	
35) Carbon Tetrachloride	3.768	117	352m	0.028	ppbv	
38) Trichloroethene	4.551	130	289m	0.038	ppbv	
52) Tetrachloroethene	8.234	164	291m	0.043	ppbv	
63) 1,1,2,2-Tetrachloroethane	9.969	83	455	0.032	ppbv #	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
Data File : VL041757.D
Acq On : 16 Dec 2024 16:08
Operator : SY/MD
Sample : VSTDICC0.03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.03

Quant Time: Dec 19 06:15:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug
QLast Update : Thu Dec 19 06:09:59 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 12/20/2024
Supervised By : Mahesh Dadoda 12/20/2024

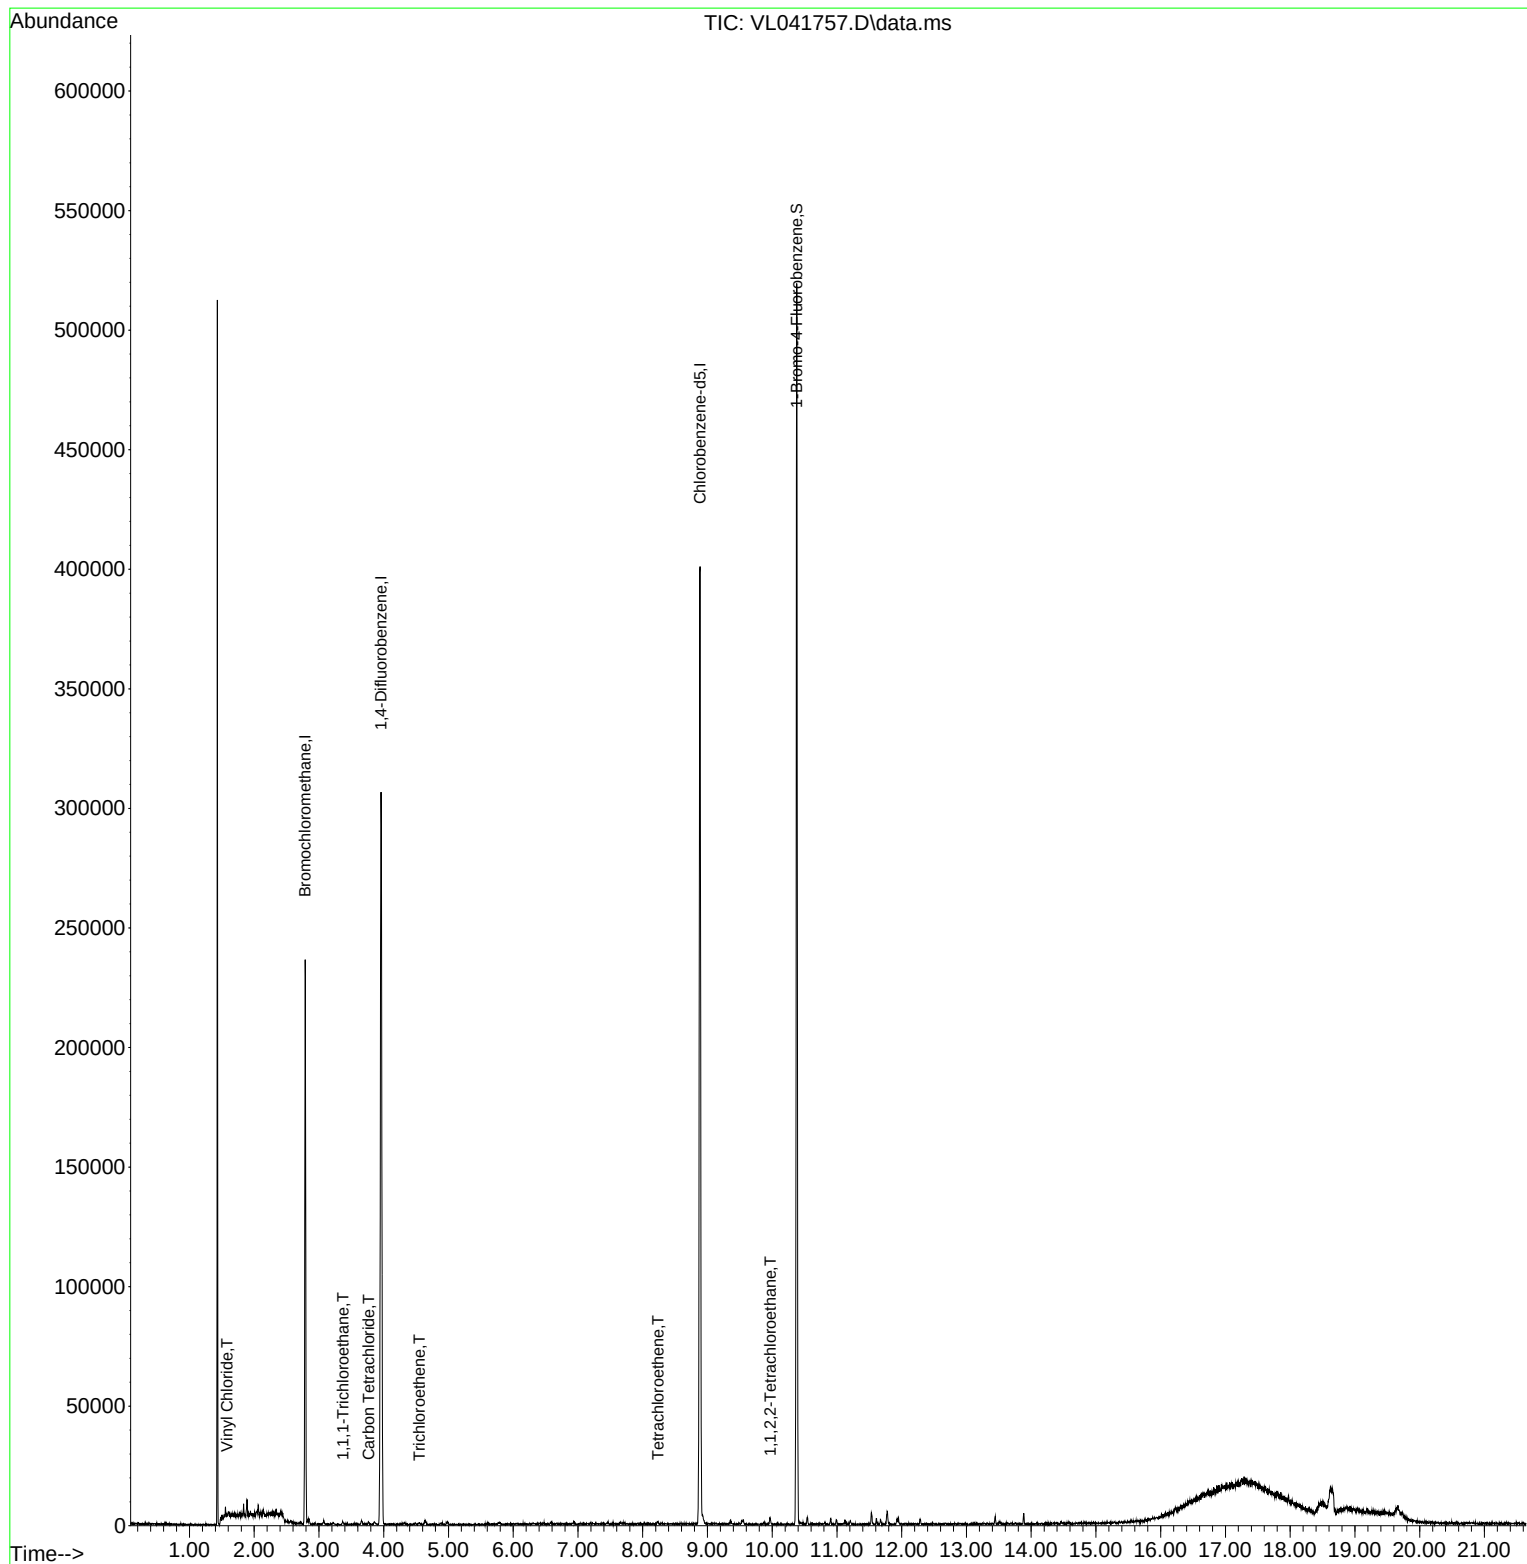

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041758.D
 Acq On : 16 Dec 2024 16:41
 Operator : SY/MD
 Sample : VSTDICC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC015

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 12/20/2024
 Supervised By : Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:16:40 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	65186	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.955	114	176856	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	160457	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.374 95 133687 9.998 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.000%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.496	85	152683	13.163	ppbv	95
3) Chlorodifluoromethane	1.473	51	152455	14.341	ppbv	98
4) Chloromethane	1.531	50	63517	13.996	ppbv	98
5) Vinyl Chloride	1.577	62	62250	13.615	ppbv	99
6) Bromomethane	1.667	94	30345	14.064	ppbv	96
7) Chloroethane	1.703	64	25650	14.442	ppbv	95
8) Dichlorotetrafluoroethane	1.554	85	148190	14.274	ppbv	99
9) Propene	1.483	41	61515	13.351	ppbv	99
10) Heptane	4.978	43	168804	14.263	ppbv	100
11) Trichlorofluoromethane	1.874	101	177984	14.446	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.136	101	135538	14.464	ppbv	98
13) Ethanol	1.719	45	3643	9.509	ppbv	100
14) Bromoethene	1.780	108	47132	14.898	ppbv	99
15) Acetone	1.832	43	142980	11.273	ppbv	100
16) 1,3-Butadiene	1.606	39	68311	13.678	ppbv	98
17) tert-Butyl alcohol	2.036	59	177908	14.140	ppbv	99
18) 1,1-Dichloroethene	2.033	96	57770	14.705	ppbv	99
19) Isopropyl Alcohol	1.884	45	82211	10.802	ppbv	99
20) Methylene Chloride	2.059	84	48356	13.371	ppbv	99
21) Allyl Chloride	2.094	41	101528	14.760	ppbv	99
22) trans-1,2-Dichloroethene	2.337	96	65029	14.461	ppbv	97
23) Vinyl Acetate	2.460	43	80795	14.661	ppbv	98
24) 1,1-Dichloroethane	2.405	63	131030	14.394	ppbv	100
25) Ethyl Acetate	2.832	43	341429	14.402	ppbv	100
26) Hexane	2.823	57	128657	14.369	ppbv	99
27) Carbon Disulfide	2.149	76	134963	16.726	ppbv	99
28) Methyl tert-Butyl Ether	2.438	73	100758	13.871	ppbv	100
29) Chloroform	2.845	83	197713	14.489	ppbv	99
30) Cyclohexane	3.855	84	110448	14.497	ppbv	99
31) cis-1,2-Dichloroethene	2.719	61	132821	14.355	ppbv	99
32) 1,1,1-Trichloroethane	3.366	97	204468	15.055	ppbv	100
34) 2-Butanone	2.554	43	195439	13.736	ppbv	99
35) Carbon Tetrachloride	3.761	117	206252	16.428	ppbv	94
36) Benzene	3.654	78	259630	14.192	ppbv	99
37) 1,2-Dichloroethane	3.214	62	166576	14.633	ppbv	100
38) Trichloroethene	4.548	130	104184	13.525	ppbv	95
39) 1,2-Dichloropropane	4.312	63	93624	14.150	ppbv	97
40) 1,4-Dioxane	4.577	88	44377	13.730	ppbv #	96
41) Tetrahydrofuran	3.052	42	113618	14.254	ppbv	100
42) Bromodichloromethane	4.486	83	211145	16.123	ppbv	96
43) Methyl Methacrylate	4.878	69	107165	15.374	ppbv	100
44) 2,2,4-Trimethylpentane	4.638	57	445947	14.274	ppbv	99
45) t-1,3-Dichloropropene	6.409	75	115159	15.973	ppbv	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041758.D
 Acq On : 16 Dec 2024 16:41
 Operator : SY/MD
 Sample : VSTDICC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC015

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:16:40 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LFri Aug 2

QLast Update : Thu Dec 19 06:09:59 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.600	75	143172	15.643	ppbv	95
47) 1,1,2-Trichloroethane	6.580	97	98426	14.242	ppbv	94
48) Dibromochloromethane	7.386	129	161661	17.131	ppbv	100
49) Bromoform	9.484	173	137786	17.838	ppbv	99
50) 4-Methyl-2-Pentanone	5.749	43	285467	14.735	ppbv	99
51) 2-Hexanone	7.435	43	232363	14.798	ppbv #	100
52) Tetrachloroethene	8.225	164	93120	13.675	ppbv	98
53) Toluene	6.930	91	301428	14.533	ppbv	100
54) 1,2-Dibromoethane	7.652	107	139889	14.690	ppbv	100
56) 1,1,1,2-Tetrachloroethane	8.924	131	128108	15.059	ppbv	99
57) Chlorobenzene	8.924	112	227716	13.869	ppbv	100
58) Ethyl Benzene	9.354	91	425852	14.742	ppbv	99
59) m/p-Xylene	9.552	91	678656m	29.209	ppbv	
60) o-Xylene	9.963	91	337891	14.506	ppbv	100
61) Styrene	9.869	104	165328	16.415	ppbv	100
62) Isopropylbenzene	10.539	105	506570	14.475	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.963	83	201057	13.790	ppbv	100
64) n-propylbenzene	10.989	120	129200	14.602	ppbv	97
65) tert-Butylbenzene	11.532	119	446690	14.148	ppbv	98
66) Benzyl Chloride	11.617	91	45189	16.234	ppbv	99
67) sec-Butylbenzene	11.769	105	624565	14.295	ppbv	99
69) p-Isopropyltoluene	11.927	119	528265	14.671	ppbv	99
70) n-Butylbenzene	12.283	91	525377	15.101	ppbv	100
71) 2-Chlorotoluene	10.901	91	387300	14.498	ppbv	100
72) 4-Ethyltoluene	11.125	105	409822	14.934	ppbv	100
73) 1,3,5-Trimethylbenzene	11.202	105	350895	15.383	ppbv	97
74) 1,2,4-Trimethylbenzene	11.539	105	371476	15.144	ppbv	96
75) 1,3-Dichlorobenzene	11.610	146	219506	14.036	ppbv	99
76) 1,4-Dichlorobenzene	11.672	146	222290	14.388	ppbv	99
77) 1,2-Dichlorobenzene	11.947	146	205737	13.672	ppbv	99
78) Hexachloro-1,3-Butadiene	13.882	225	138481	12.412	ppbv	100
79) Naphthalene	13.513	128	301006	17.611	ppbv	99
80) Naphthalene,2-methyl-	14.458	142	161927	30.630	ppbv	98
81) 1,2,4-Trichlorobenzene	13.442	180	146340	15.669	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
 Data File : VL041758.D
 Acq On : 16 Dec 2024 16:41
 Operator : SY/MD
 Sample : VSTDIC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDIC015

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 06:16:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug
 QLast Update : Thu Dec 19 06:09:59 2024
 Response via : Initial Calibration


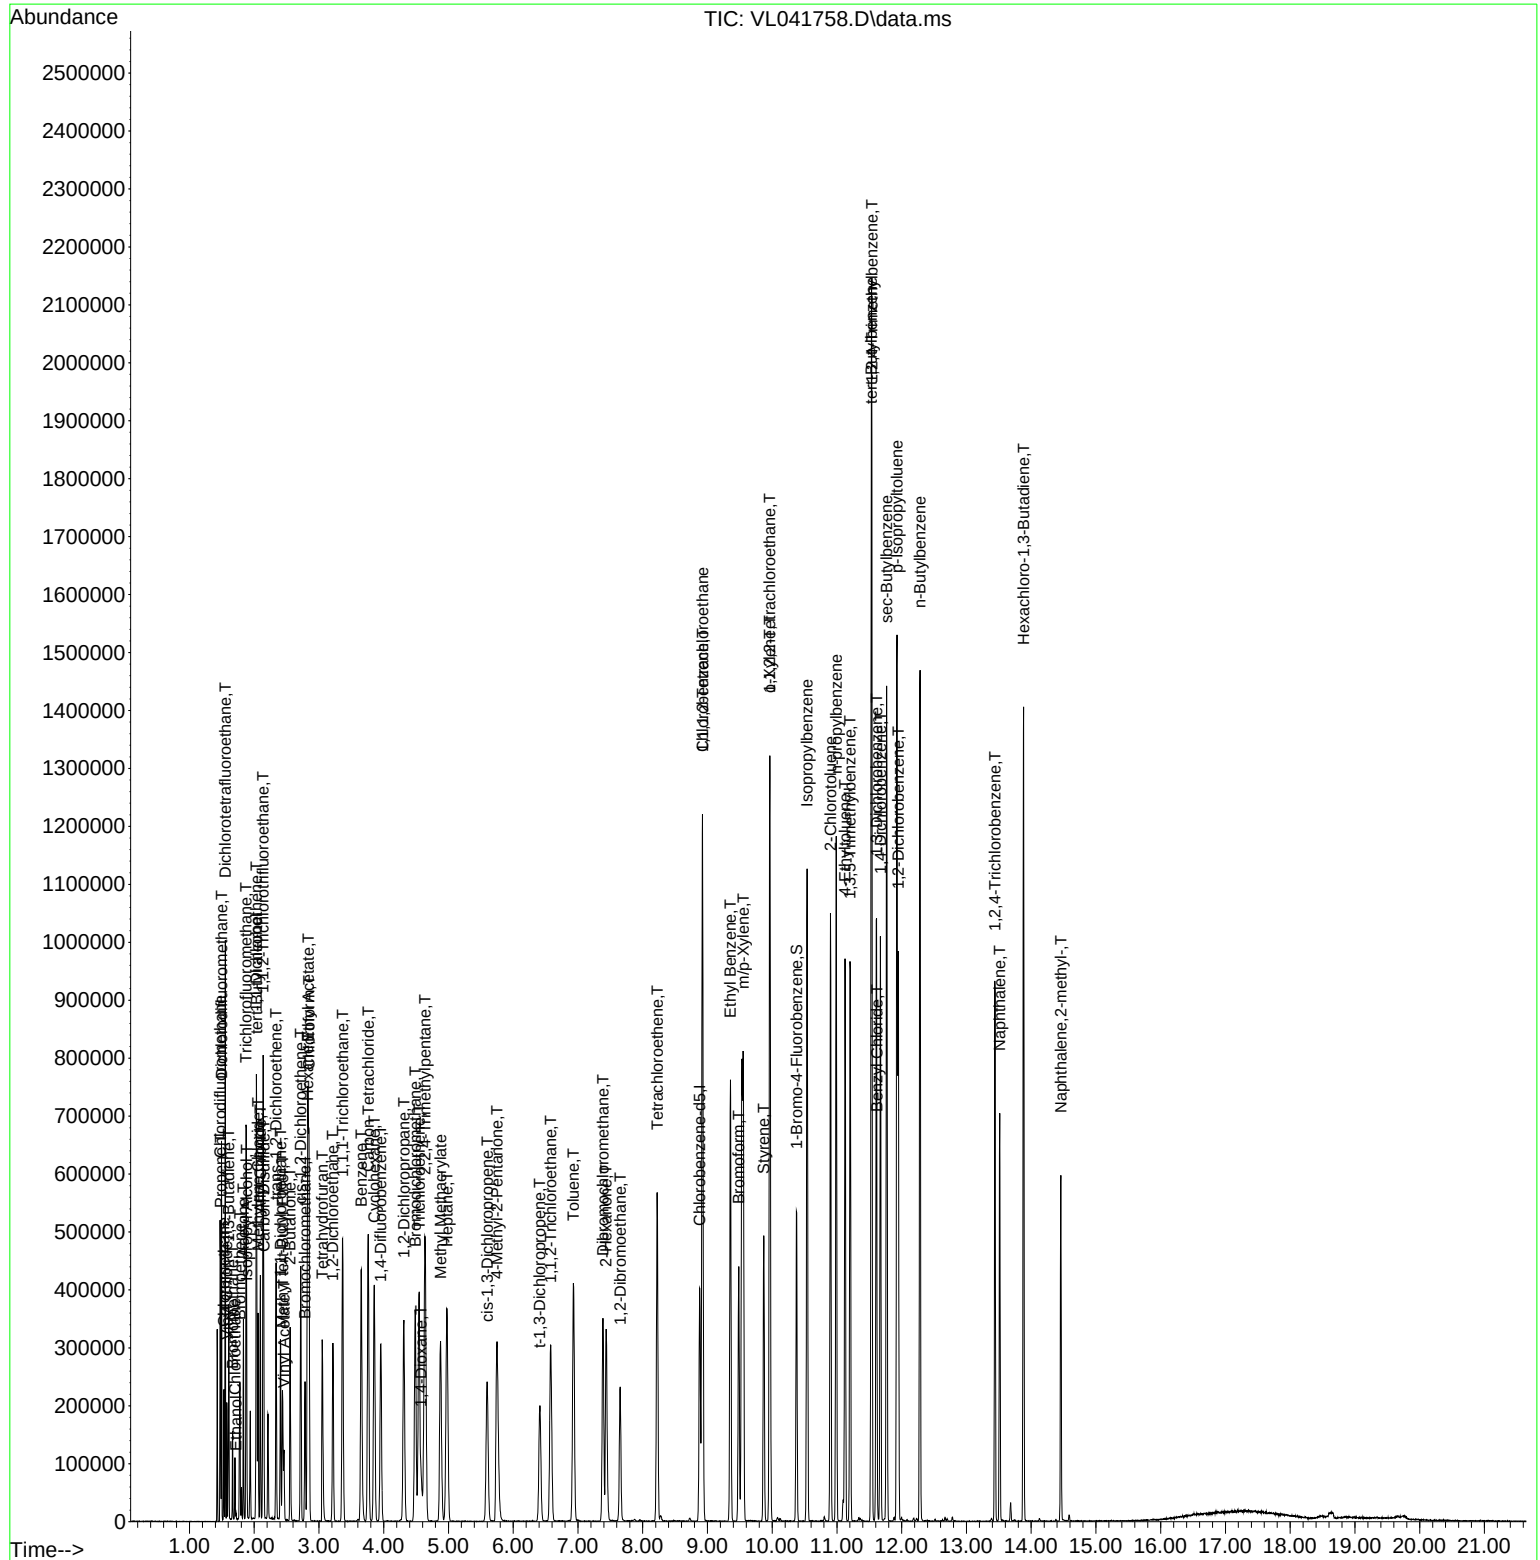


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
Data File : VL041787.D
Acq On : 18 Dec 2024 08:06
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Dec 19 07:32:09 2024

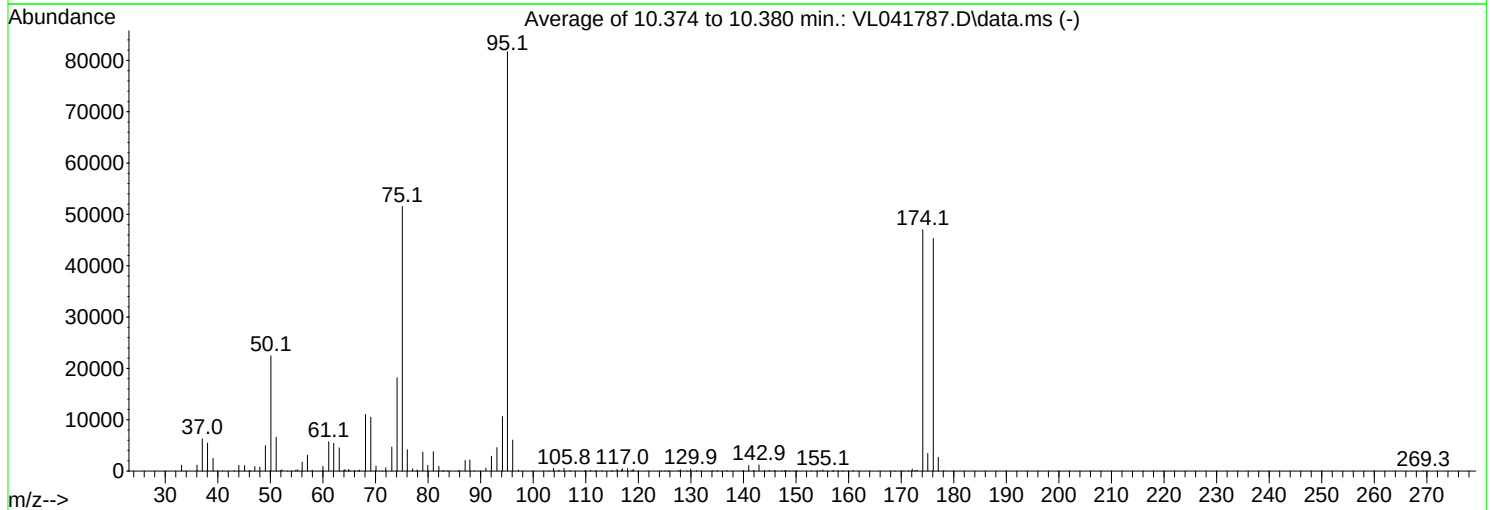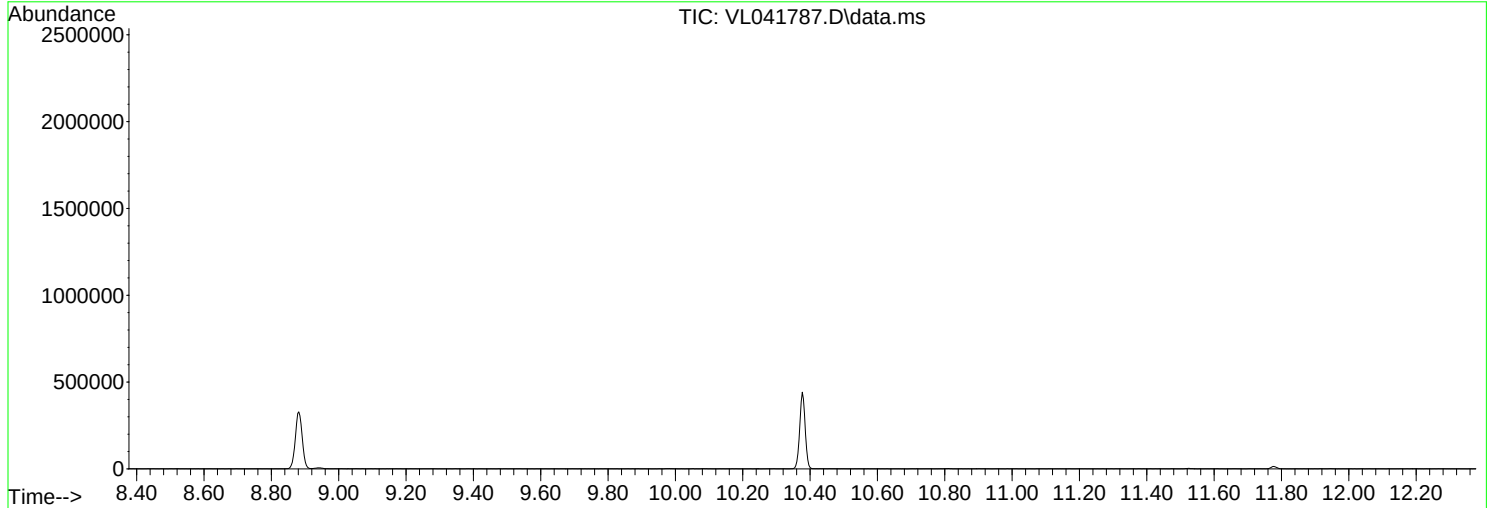

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.5	22445	PASS
75	95	30	66	63.1	51533	PASS
95	95	100	100	100.0	81685	PASS
96	95	5	9	7.4	6040	PASS
173	174	0.00	2	0.4	189	PASS
174	95	50	120	57.6	47024	PASS
175	174	4	9	7.3	3435	PASS
176	174	93	101	96.3	45299	PASS
177	176	5	9	5.9	2683	PASS

Average of 10.374 to 10.380 min.: VL041787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1141	47.05	858	57.05	3102	66.70	47
36.05	1180	48.00	764	57.95	178	66.95	200
37.05	6288	49.05	4965	60.00	923	68.10	11038
38.05	5467	50.10	22445	61.10	5714	69.10	10482
39.10	2494	51.10	6553	62.05	5427	70.10	981
40.90	31	51.90	123	63.10	4527	71.30	41
43.15	73	52.20	256	64.00	189	71.95	649
44.00	1141	53.30	30	64.20	301	73.10	4685
45.10	1066	54.85	179	64.85	304	74.10	18195
45.95	73	55.20	262	65.10	104	75.10	51533
46.20	47	56.05	1736	65.95	70	76.05	4174

Average of 10.374 to 10.380 min.: VL041787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	436	87.95	2170	104.90	187	116.95	484
77.90	224	88.80	41	105.85	548	117.95	466
79.00	3700	91.00	562	107.00	137	118.80	212
79.95	1115	92.05	2894	109.75	61	119.05	329
81.00	3787	93.10	4562	110.90	154	124.40	18
82.05	950	94.15	10629	111.85	82	125.10	79
82.70	32	95.10	81685	113.10	84	125.75	80
83.00	122	96.10	6040	114.80	31	127.70	141
83.75	45	97.20	186	115.10	55	128.00	257
85.80	123	103.00	19	115.95	361	129.30	28
87.05	2079	103.85	509	116.80	188	129.95	400

Average of 10.374 to 10.380 min.: VL041787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
131.05	108	147.30	17	157.15	89	175.05	3435
134.10	38	147.85	124	158.05	61	176.10	45299
135.00	142	148.10	54	158.90	87	177.05	2683
136.85	125	148.70	21	160.85	126	178.10	67
139.90	91	149.60	20	168.80	17	269.30	24
141.00	1101	150.15	64	170.50	21		
141.95	144	152.90	26	171.40	50		
142.95	1185	154.00	17	172.10	387		
143.95	74	154.60	41	172.60	118		
144.90	164	155.10	249	173.00	189		
146.00	151	156.90	28	174.10	47024		

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
 Data File : VL041788.D
 Acq On : 18 Dec 2024 10:29
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Quant Time: Dec 19 07:49:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Thu Dec 19 07:32:09 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/19/2024
 Supervised By : Mahesh Dadoda 12/19/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	76040	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	198370	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.881	117	172190	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.377	95	150705	10.503	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	105.000%

Target Compounds	Qvalue					
2) Dichlorodifluoromethane	1.495	85	112841	8.340	ppbv	96
3) Chlorodifluoromethane	1.473	51	112096	9.040	ppbv	98
4) Chloromethane	1.531	50	48418	9.146	ppbv	99
5) Vinyl Chloride	1.580	62	46631	8.743	ppbv	99
6) Bromomethane	1.667	94	22202	8.821	ppbv	98
7) Chloroethane	1.703	64	19203	9.269	ppbv	99
8) Dichlorotetrafluoroethane	1.554	85	111653	9.220	ppbv	96
9) Propene	1.483	41	41427	7.708	ppbv	96
10) Heptane	4.975	43	111650	8.087	ppbv	96
11) Trichlorofluoromethane	1.874	101	134331	9.347	ppbv	99
12) 1,1,2-Trichlorotrifluoro...	2.136	101	96469	8.825	ppbv	98
13) Ethanol	1.719	45	3276m	7.361	ppbv	
14) Bromoethene	1.780	108	33118	8.974	ppbv	97
15) Acetone	1.832	43	111294	7.522	ppbv	99
16) 1,3-Butadiene	1.606	39	53299	9.149	ppbv	97
17) tert-Butyl alcohol	2.036	59	135516	9.233	ppbv	100
18) 1,1-Dichloroethene	2.033	96	41224	8.996	ppbv	93
19) Isopropyl Alcohol	1.884	45	64831	7.303	ppbv	99
20) Methylene Chloride	2.059	84	35699	8.462	ppbv	96
21) Allyl Chloride	2.094	41	74468	9.281	ppbv	99
22) trans-1,2-Dichloroethene	2.337	96	45331	8.641	ppbv	94
23) Vinyl Acetate	2.460	43	52709	7.673	ppbv #	95
24) 1,1-Dichloroethane	2.405	63	95779	9.020	ppbv	99
25) Ethyl Acetate	2.832	43	238771	8.675	ppbv	100
26) Hexane	2.822	57	87593	8.386	ppbv	95
27) Carbon Disulfide	2.149	76	85318	9.064	ppbv	98
28) Methyl tert-Butyl Ether	2.437	73	67965	8.021	ppbv	97
29) Chloroform	2.845	83	145536	9.143	ppbv	97
30) Cyclohexane	3.855	84	74346	8.366	ppbv	97
31) cis-1,2-Dichloroethene	2.719	61	92460	8.567	ppbv	98
32) 1,1,1-Trichloroethane	3.366	97	144038	8.902	ppbv	99
34) 2-Butanone	2.554	43	139509	8.742	ppbv	99
35) Carbon Tetrachloride	3.761	117	147726	10.490	ppbv	99
36) Benzene	3.654	78	178114	8.680	ppbv	98
37) 1,2-Dichloroethane	3.214	62	121412	9.509	ppbv	100
38) Trichloroethene	4.548	130	70175	8.057	ppbv	98
39) 1,2-Dichloropropane	4.308	63	64154	8.645	ppbv	97
40) 1,4-Dioxane	4.583	88	30262	8.347	ppbv #	96
41) Tetrahydrofuran	3.052	42	74734	8.359	ppbv	98
42) Bromodichloromethane	4.486	83	140832	9.588	ppbv	95
43) Methyl Methacrylate	4.878	69	69545	8.895	ppbv	99
44) 2,2,4-Trimethylpentane	4.635	57	302332	8.627	ppbv	97
45) t-1,3-Dichloropropene	6.412	75	69601	8.607	ppbv	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
 Data File : VL041788.D
 Acq On : 18 Dec 2024 10:29
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Quant Time: Dec 19 07:49:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Thu Dec 19 07:32:09 2024
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 12/19/2024
 Supervised By : Mahesh Dadoda 12/19/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	89328m	8.701	ppbv	
47) 1,1,2-Trichloroethane	6.580	97	67717	8.736	ppbv	93
48) Dibromochloromethane	7.386	129	101875	9.625	ppbv	97
49) Bromoform	9.483	173	83649	9.655	ppbv	99
50) 4-Methyl-2-Pentanone	5.752	43	186865	8.600	ppbv	99
51) 2-Hexanone	7.438	43	149217	8.472	ppbv #	98
52) Tetrachloroethene	8.224	164	59756	7.824	ppbv	93
53) Toluene	6.930	91	195158	8.389	ppbv	99
54) 1,2-Dibromoethane	7.648	107	94138	8.814	ppbv	97
56) 1,1,1,2-Tetrachloroethane	8.924	131	87869	9.626	ppbv	99
57) Chlorobenzene	8.920	112	157039	8.912	ppbv	97
58) Ethyl Benzene	9.354	91	281290	9.074	ppbv	97
59) m/p-Xylene	9.548	91	466737m	18.725	ppbv	
60) o-Xylene	9.963	91	232028	9.283	ppbv	100
61) Styrene	9.869	104	103216	9.550	ppbv	99
62) Isopropylbenzene	10.539	105	352903	9.397	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.963	83	144197	9.216	ppbv	99
64) n-propylbenzene	10.989	120	90043	9.483	ppbv	99
65) tert-Butylbenzene	11.532	119	314940	9.295	ppbv	98
66) Benzyl Chloride	11.616	91	22164	7.426	ppbv	100
67) sec-Butylbenzene	11.769	105	442201	9.431	ppbv	100
69) p-Isopropyltoluene	11.927	119	369746	9.569	ppbv	99
70) n-Butylbenzene	12.283	91	373294	9.999	ppbv	99
71) 2-Chlorotoluene	10.901	91	264866	9.240	ppbv	100
72) 4-Ethyltoluene	11.124	105	285469	9.676	ppbv	99
73) 1,3,5-Trimethylbenzene	11.202	105	242783	9.918	ppbv	97
74) 1,2,4-Trimethylbenzene	11.536	105	263301	10.003	ppbv	90
75) 1,3-Dichlorobenzene	11.607	146	154857	9.227	ppbv	99
76) 1,4-Dichlorobenzene	11.671	146	154115	9.296	ppbv	99
77) 1,2-Dichlorobenzene	11.947	146	145375	9.002	ppbv	99
78) Hexachloro-1,3-Butadiene	13.882	225	93437	7.804	ppbv	100
79) Naphthalene	13.513	128	200311	10.921	ppbv	98
80) Naphthalene,2-methyl-	14.458	142	94903	16.728	ppbv	97
81) 1,2,4-Trichlorobenzene	13.442	180	93675	9.346	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
Data File : VL041788.D
Acq On : 18 Dec 2024 10:29
Operator : SY/MD
Sample : VSTDCCC010
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDCCC010

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 12/19/2024
Supervised By : Mahesh Dadoda 12/19/2024

Quant Time: Dec 19 07:49:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Thu Dec 19 07:32:09 2024
Response via : Initial Calibration

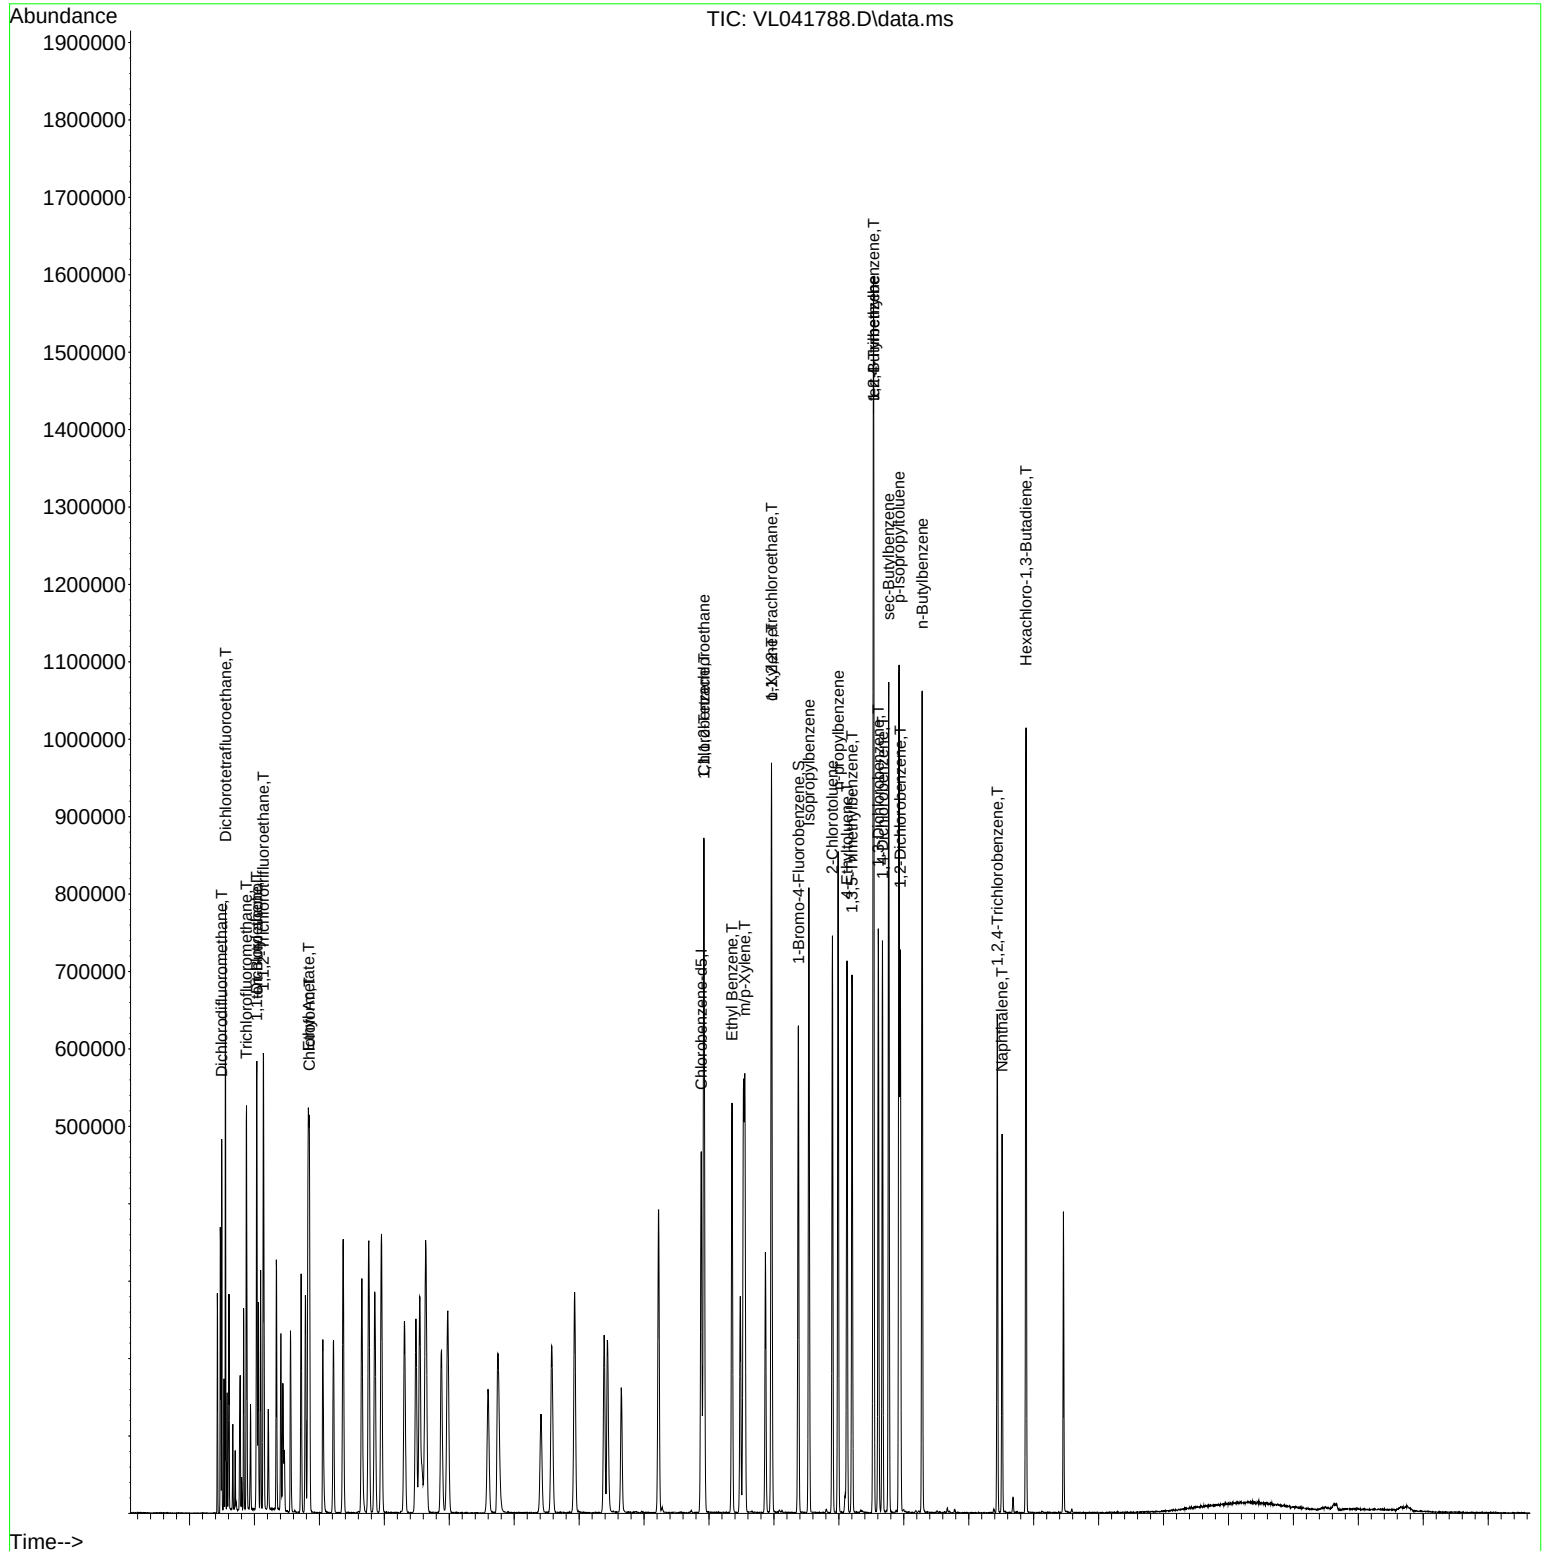

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
 Data File : VL041790.D
 Acq On : 18 Dec 2024 12:28
 Operator : SY/MD
 Sample : VL1218ABL02
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL1218ABL02

Quant Time: Dec 19 07:52:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Thu Dec 19 07:32:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.793	49	70249	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.965	114	175356	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.891	117	151060	10.000	ppbv	0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.383	95	127683	10.143	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.400%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
Data File : VL041790.D
Acq On : 18 Dec 2024 12:28
Operator : SY/MD
Sample : VL1218ABL02
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL1218ABL02

Quant Time: Dec 19 07:52:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Thu Dec 19 07:32:09 2024
Response via : Initial Calibration

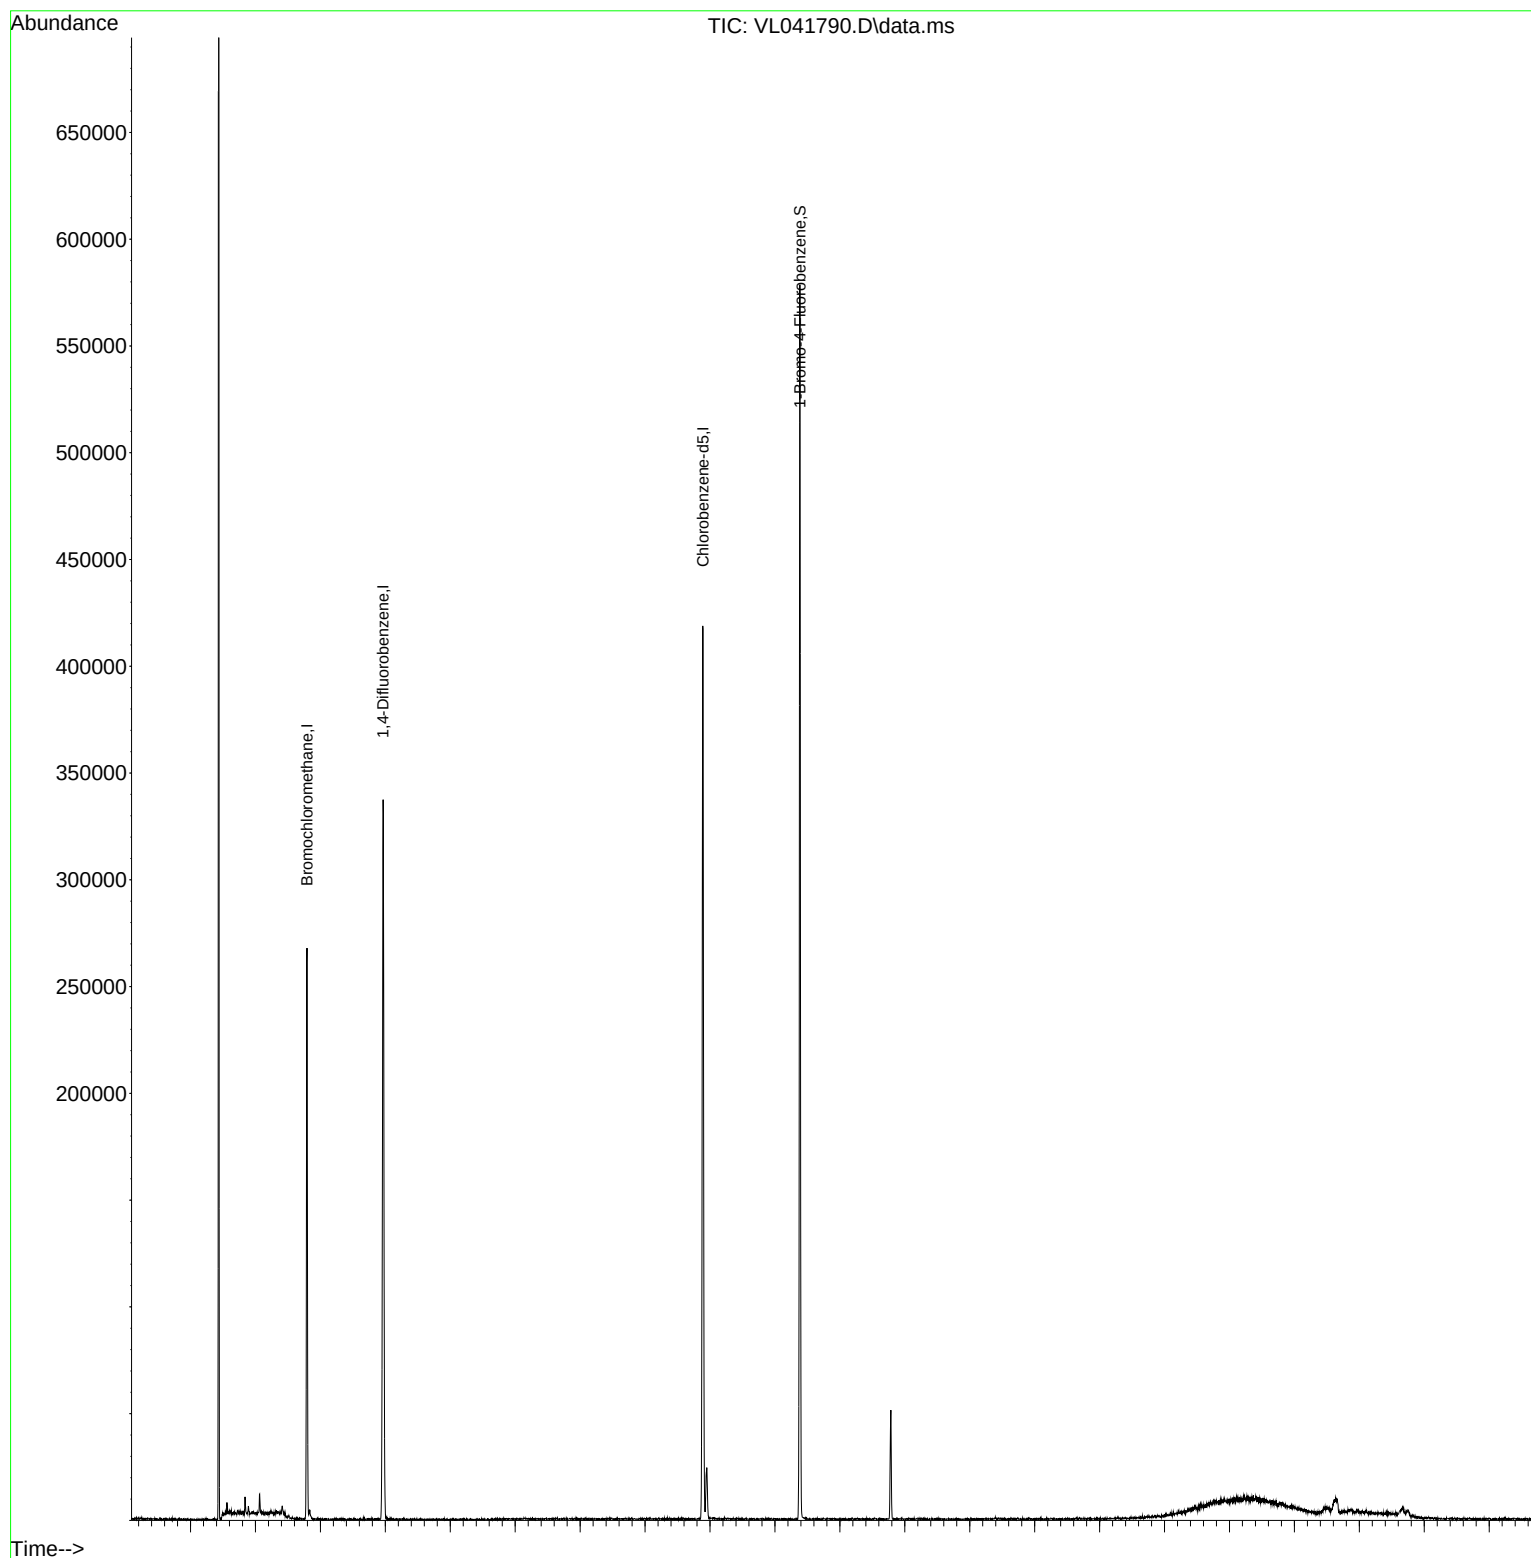

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
 Data File : VL041795.D
 Acq On : 18 Dec 2024 16:06
 Operator : SY/MD
 Sample : VL1218ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL1218ABS01

Quant Time: Dec 19 07:55:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Thu Dec 19 07:32:09 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/19/2024
 Supervised By : Mahesh Dadoda 12/19/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.797	49	72600	10.000	ppbv	0.01
33) 1,4-Difluorobenzene	3.972	114	183255	10.000	ppbv	0.02
55) Chlorobenzene-d5	8.898	117	159496	10.000	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.390	95	143879	10.825	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	108.300%

Target Compounds	Qvalue					
2) Dichlorodifluoromethane	1.502	85	112657	8.721	ppbv	99
3) Chlorodifluoromethane	1.479	51	102210	8.633	ppbv	97
4) Chloromethane	1.538	50	46901	9.279	ppbv	100
5) Vinyl Chloride	1.583	62	44104	8.661	ppbv	98
6) Bromomethane	1.674	94	21119	8.788	ppbv	99
7) Chloroethane	1.709	64	18047	9.123	ppbv	98
8) Dichlorotetrafluoroethane	1.557	85	110410	9.549	ppbv	93
9) Propene	1.486	41	35133	6.846	ppbv	98
10) Heptane	5.001	43	106572	8.085	ppbv	100
11) Trichlorofluoromethane	1.884	101	132171	9.632	ppbv	98
12) 1,1,2-Trichlorotrifluo...	2.146	101	96243	9.222	ppbv	95
13) Ethanol	1.725	45	2865	6.742	ppbv	98
14) Bromoethene	1.787	108	30065	8.533	ppbv	96
15) Acetone	1.842	43	110277	7.807	ppbv	97
16) 1,3-Butadiene	1.612	39	52562	9.450	ppbv	92
17) tert-Butyl alcohol	2.046	59	122872	8.768	ppbv	100
18) 1,1-Dichloroethene	2.039	96	38415	8.780	ppbv	80
19) Isopropyl Alcohol	1.890	45	59665	7.039	ppbv #	37
20) Methylene Chloride	2.068	84	35310	8.766	ppbv	94
21) Allyl Chloride	2.104	41	68525	8.945	ppbv	95
22) trans-1,2-Dichloroethene	2.350	96	42821	8.550	ppbv	98
23) Vinyl Acetate	2.470	43	43463	6.627	ppbv	97
24) 1,1-Dichloroethane	2.418	63	92680	9.142	ppbv	99
25) Ethyl Acetate	2.845	43	223419	8.502	ppbv	99
26) Hexane	2.835	57	81413	8.164	ppbv	93
27) Carbon Disulfide	2.159	76	76433	8.505	ppbv	94
28) Methyl tert-Butyl Ether	2.447	73	64037	7.915	ppbv	99
29) Chloroform	2.858	83	139818	9.200	ppbv	99
30) Cyclohexane	3.871	84	66237	7.806	ppbv	98
31) cis-1,2-Dichloroethene	2.732	61	82779	8.033	ppbv	99
32) 1,1,1-Trichloroethane	3.379	97	136055	8.807	ppbv	98
34) 2-Butanone	2.564	43	125687	8.525	ppbv	100
35) Carbon Tetrachloride	3.777	117	141202	10.854	ppbv	97
36) Benzene	3.667	78	164423	8.674	ppbv	98
37) 1,2-Dichloroethane	3.230	62	113600	9.631	ppbv	99
38) Trichloroethene	4.564	130	63280	7.864	ppbv	93
39) 1,2-Dichloropropane	4.331	63	58553	8.541	ppbv	92
40) 1,4-Dioxane	4.599	88	28884	8.624	ppbv #	92
41) Tetrahydrofuran	3.065	42	67017	8.114	ppbv	99
42) Bromodichloromethane	4.509	83	133513	9.839	ppbv	95
43) Methyl Methacrylate	4.897	69	61014	8.448	ppbv	99
44) 2,2,4-Trimethylpentane	4.658	57	284140	8.777	ppbv	96
45) t-1,3-Dichloropropene	6.438	75	58865	7.879	ppbv	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
 Data File : VL041795.D
 Acq On : 18 Dec 2024 16:06
 Operator : SY/MD
 Sample : VL1218ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL1218ABS01

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 12/19/2024
 Supervised By : Mahesh Dadoda 12/19/2024

Quant Time: Dec 19 07:55:13 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Dec 19 07:32:09 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.625	75	74198	7.824	ppbv	89
47) 1,1,2-Trichloroethane	6.603	97	64954	9.071	ppbv	93
48) Dibromochloromethane	7.406	129	96996	9.920	ppbv	99
49) Bromoform	9.500	173	80840	10.100	ppbv	99
50) 4-Methyl-2-Pentanone	5.774	43	175817	8.759	ppbv	99
51) 2-Hexanone	7.457	43	142403	8.752	ppbv #	96
52) Tetrachloroethene	8.244	164	54531	7.729	ppbv	93
53) Toluene	6.952	91	177625	8.265	ppbv	99
54) 1,2-Dibromoethane	7.671	107	90389	9.161	ppbv	92
56) 1,1,1,2-Tetrachloroethane	8.943	131	86262	10.202	ppbv	100
57) Chlorobenzene	8.937	112	153659	9.415	ppbv	99
58) Ethyl Benzene	9.370	91	267795	9.326	ppbv	98
59) m/p-Xylene	9.564	91	455916m	19.747	ppbv	
60) o-Xylene	9.975	91	229919	9.930	ppbv	100
61) Styrene	9.885	104	95536	9.543	ppbv	100
62) Isopropylbenzene	10.552	105	339599	9.762	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.975	83	142272	9.817	ppbv	100
64) n-propylbenzene	11.002	120	86896	9.880	ppbv	97
65) tert-Butylbenzene	11.542	119	307835	9.808	ppbv	97
66) Benzyl Chloride	11.626	91	21939	7.936	ppbv	97
67) sec-Butylbenzene	11.778	105	441578	10.167	ppbv	99
69) p-Isopropyltoluene	11.937	119	366111	10.229	ppbv	99
70) n-Butylbenzene	12.293	91	366451	10.597	ppbv	98
71) 2-Chlorotoluene	10.914	91	255490	9.622	ppbv	99
72) 4-Ethyltoluene	11.137	105	277025	10.137	ppbv	99
73) 1,3,5-Trimethylbenzene	11.215	105	240648	10.613	ppbv	100
74) 1,2,4-Trimethylbenzene	11.548	105	260378	10.679	ppbv	96
75) 1,3-Dichlorobenzene	11.620	146	152493	9.809	ppbv	98
76) 1,4-Dichlorobenzene	11.684	146	152432	9.926	ppbv	97
77) 1,2-Dichlorobenzene	11.960	146	148412	9.922	ppbv	99
78) Hexachloro-1,3-Butadiene	13.892	225	88582	7.987	ppbv	100
79) Naphthalene	13.523	128	189506	11.154	ppbv	99
80) Naphthalene,2-methyl-	14.468	142	82155	15.634	ppbv	96
81) 1,2,4-Trichlorobenzene	13.452	180	89052	9.592	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
 Data File : VL041796.D
 Acq On : 18 Dec 2024 16:37
 Operator : SY/MD
 Sample : QC121724 CAN 10158
 Misc : 400mL/MSVOA_L
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC121724 CAN 10158

Quant Time: Dec 19 07:56:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Thu Dec 19 07:32:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.793	49	73011	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.968	114	179409	10.000	ppbv	0.01
55) Chlorobenzene-d5	8.891	117	152308	10.000	ppbv	0.01

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.386	95	125911	9.920	ppbv	0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.200%

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
Data File : VL041796.D
Acq On : 18 Dec 2024 16:37
Operator : SY/MD
Sample : QC121724 CAN 10158
Misc : 400mL/MSVOA_L
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC121724 CAN 10158

Quant Time: Dec 19 07:56:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Thu Dec 19 07:32:09 2024
Response via : Initial Calibration

