
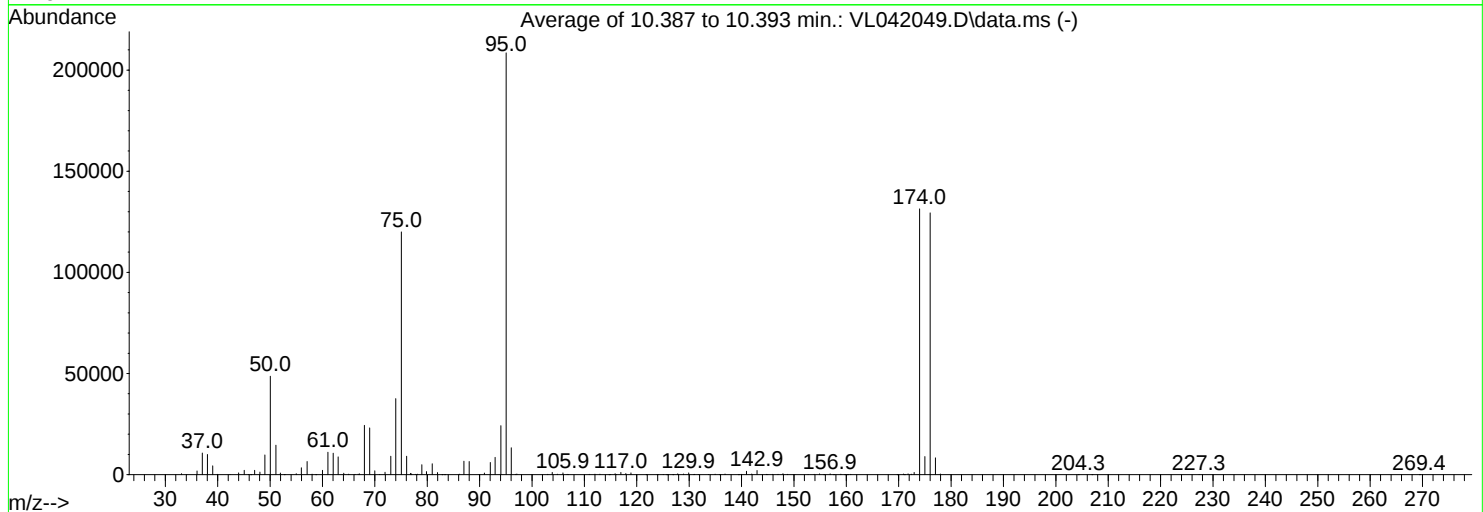


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022625\
Data File : VL042049.D
Acq On : 26 Feb 2025 07:46
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Feb 26 01:08:36 2025

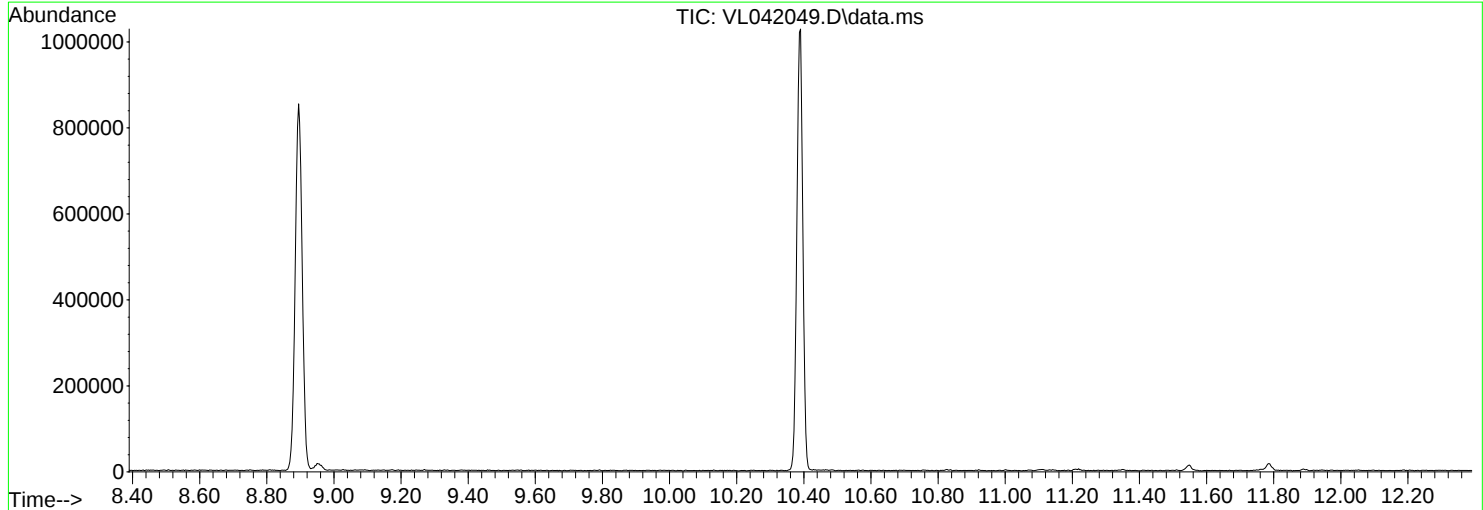

AutoFind: Scans 3182, 3183, 3184; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.3	48688	PASS
75	95	30	66	57.6	120021	PASS
95	95	100	100	100.0	208533	PASS
96	95	5	9	6.4	13271	PASS
173	174	0.00	2	0.8	1077	PASS
174	95	50	120	63.0	131429	PASS
175	174	4	9	6.8	8951	PASS
176	174	93	101	98.5	129411	PASS
177	176	5	9	6.4	8302	PASS

Average of 10.387 to 10.393 min.: VL042049.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	444	46.30	33	58.00	267	68.00	2439
34.10	89	47.05	2153	58.70	32	69.00	2312
36.05	1844	48.05	1303	60.00	2109	70.00	188
37.05	10667	49.00	9754	61.05	11094	70.90	4
38.05	10014	50.05	48688	62.05	10570	71.95	1166
39.05	4341	51.10	14536	63.00	8757	73.05	9099
39.95	189	51.95	802	64.05	705	74.00	37563
42.35	56	52.70	38	65.00	222	75.05	120021
44.00	882	55.00	489	66.20	139	76.05	9120
45.05	2180	55.95	3385	66.80	237	76.80	665
45.90	90	57.05	6526	67.05	420	77.00	419

Average of 10.387 to 10.393 min.: VL042049.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.80	203	88.00	6528	103.85	1108	116.10	59
78.10	234	89.90	62	104.85	242	116.95	1104
78.95	4879	90.90	798	105.90	845	117.90	569
79.85	1525	92.05	6030	106.70	150	118.90	897
80.95	5390	92.95	8533	106.90	52	121.80	44
81.95	1037	94.05	24184	110.90	178	123.90	33
82.80	33	95.05	208533	112.00	270	125.05	99
82.95	48	96.05	13271	112.95	245	125.70	47
83.30	28	96.90	139	114.70	43	125.90	24
86.10	258	97.10	324	115.00	85	126.90	27
87.00	6686	103.00	143	115.85	504	127.80	366

Average of 10.387 to 10.393 min.: VL042049.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.00	203	140.00	207	150.15	121	169.70	19
128.95	297	140.95	1699	152.70	102	170.00	109
129.90	864	141.95	314	153.85	170	170.90	280
130.90	100	142.95	2085	154.90	374	171.10	47
131.05	133	144.75	159	155.70	26	171.80	411
131.75	78	145.00	70	156.90	423	172.40	275
133.70	60	145.95	199	157.55	37	172.95	1077
134.95	225	146.95	149	158.95	230	174.00	131429
135.80	37	147.90	442	159.70	18	175.00	8951
136.85	340	148.80	149	160.20	18	176.00	129411
139.40	37	149.90	73	160.85	143	177.00	8302

Average of 10.387 to 10.393 min.: VL042049.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.95	321						
204.30	18						
206.90	17						
227.35	73						
269.40	18						