

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022725\
Data File : PP070098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2025 17:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:21:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.526	3.832	27590404	18800625	18.799	19.665
2) SA Decachlor...	10.257	8.890	20088421	19985309	17.636	18.435

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022725\
Data File : PP070098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2025 17:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:21:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

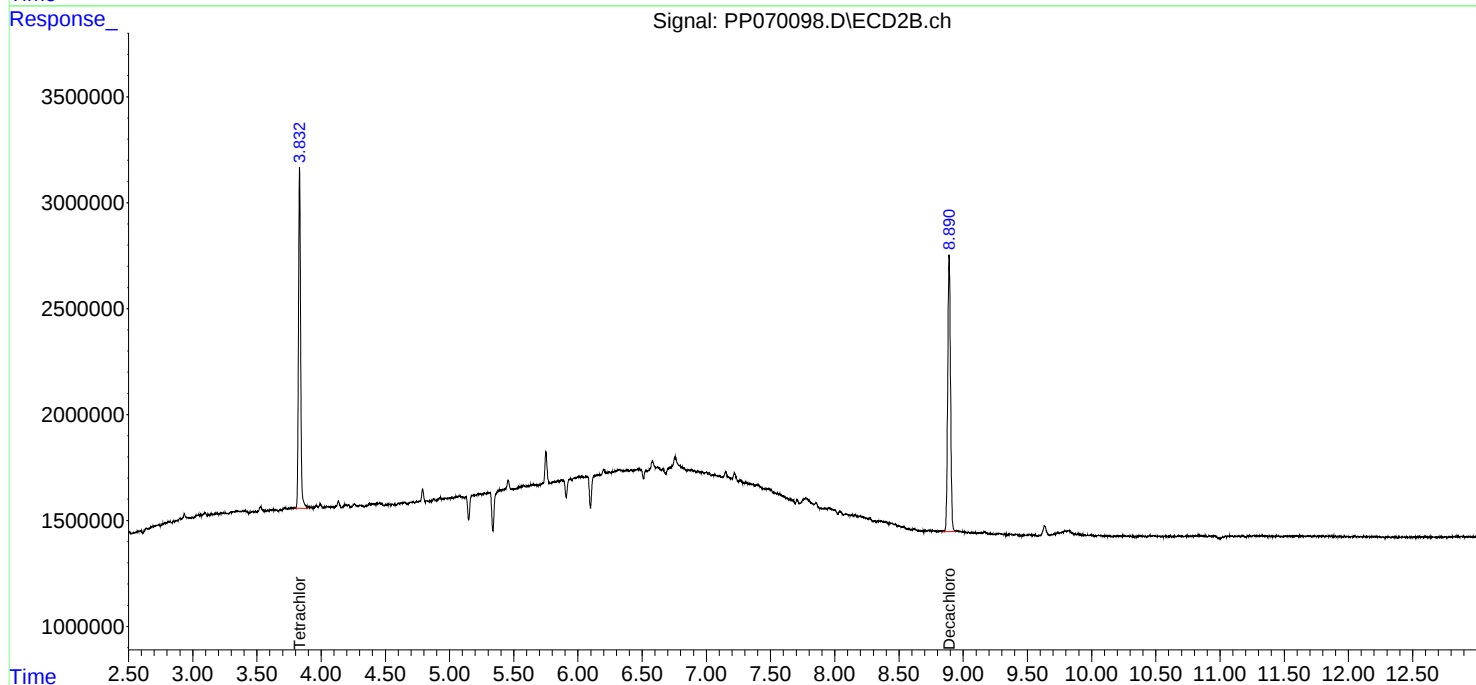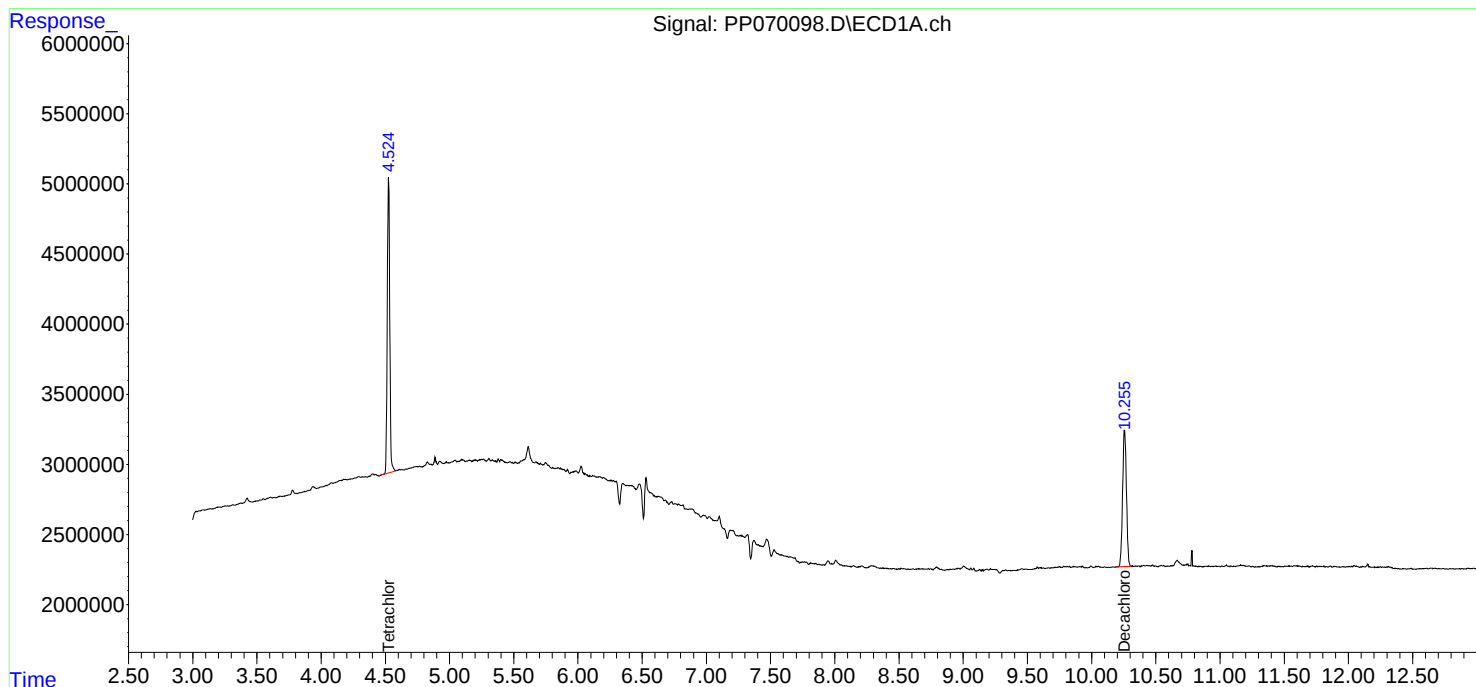


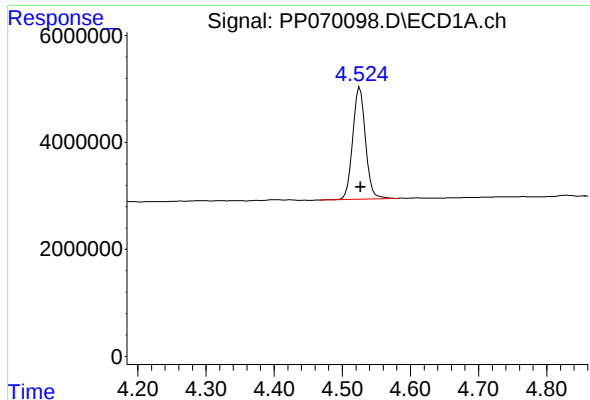

#1 Tetrachloro-m-xylene


R.T.: 4.526 min
Delta R.T.: -0.001 min
Response: 27590404
Conc: 18.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

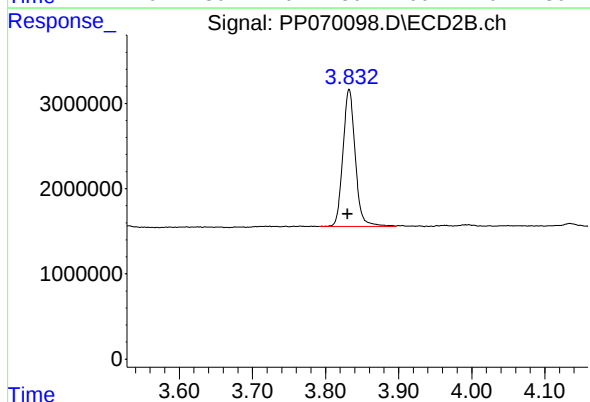


#1 Tetrachloro-m-xylene

R.T.: 3.832 min
Delta R.T.: 0.002 min
Response: 18800625
Conc: 19.67 ng/ml

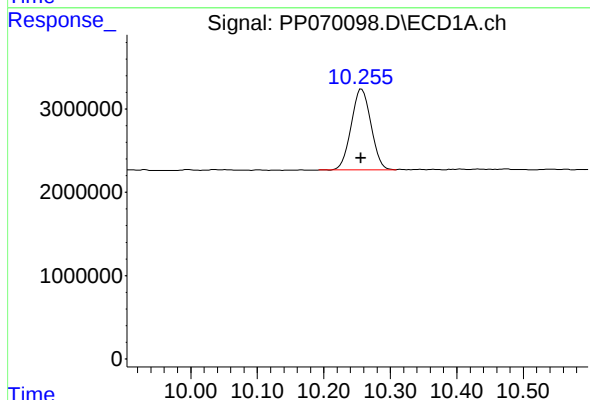

#2 Decachlorobiphenyl

R.T.: 10.257 min
Delta R.T.: 0.000 min
Response: 20088421
Conc: 17.64 ng/ml

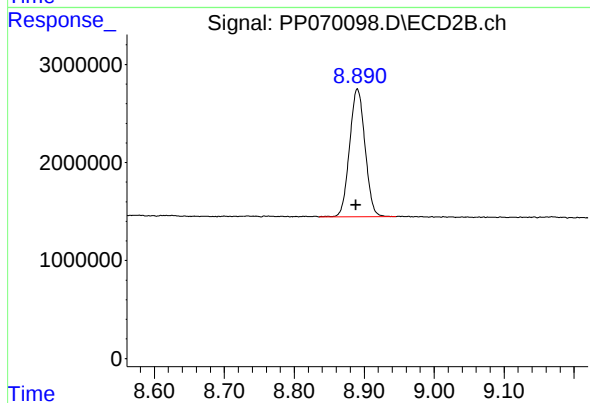

#2 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: 0.002 min
Response: 19985309
Conc: 18.43 ng/ml