

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022725\
 Data File : PP070107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2025 20:10
 Operator : YP\AJ
 Sample : Q1421-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P001-CLAY-CF01-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:28:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.528	3.833	36394976	23673298	24.799	24.762
2) SA Decachlor...	10.259	8.890	26080973	23780326	22.897	21.935

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022725\
Data File : PP070107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2025 20:10
Operator : YP\AJ
Sample : Q1421-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
P001-CLAY-CF01-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:28:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

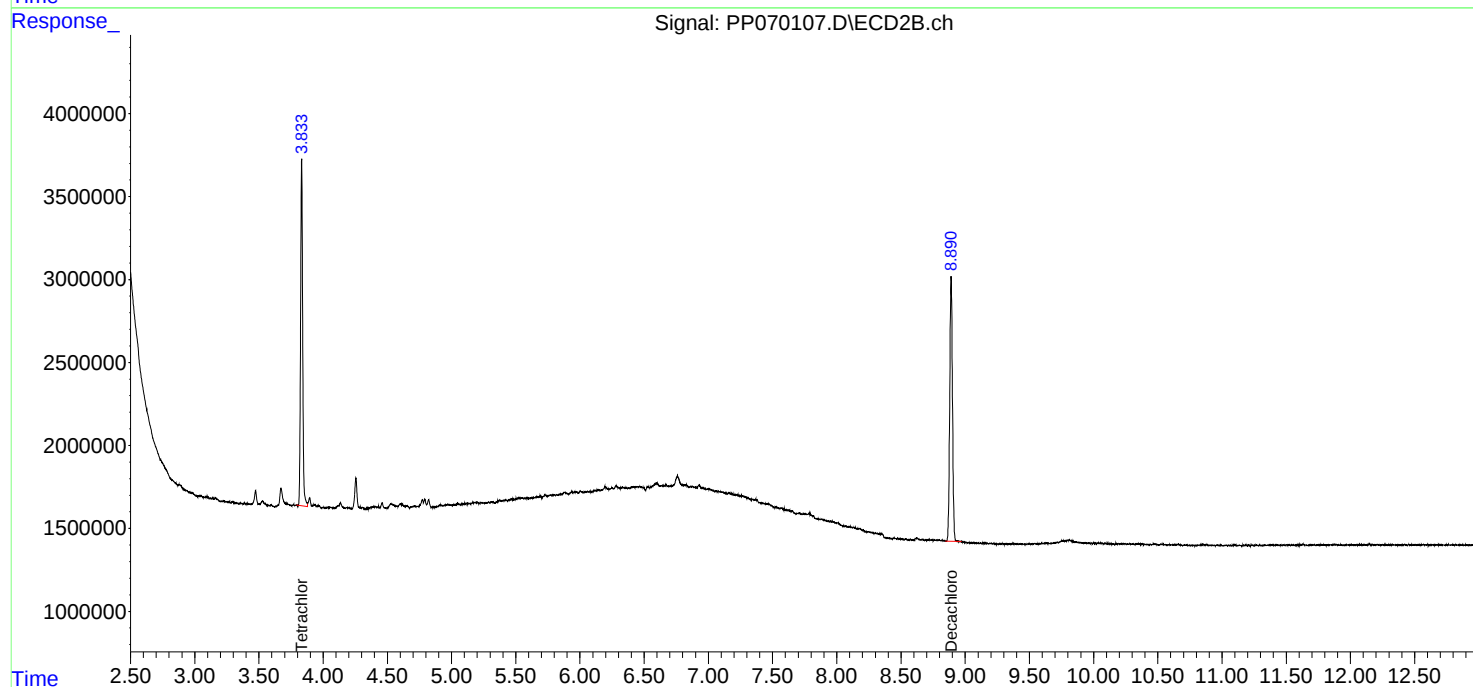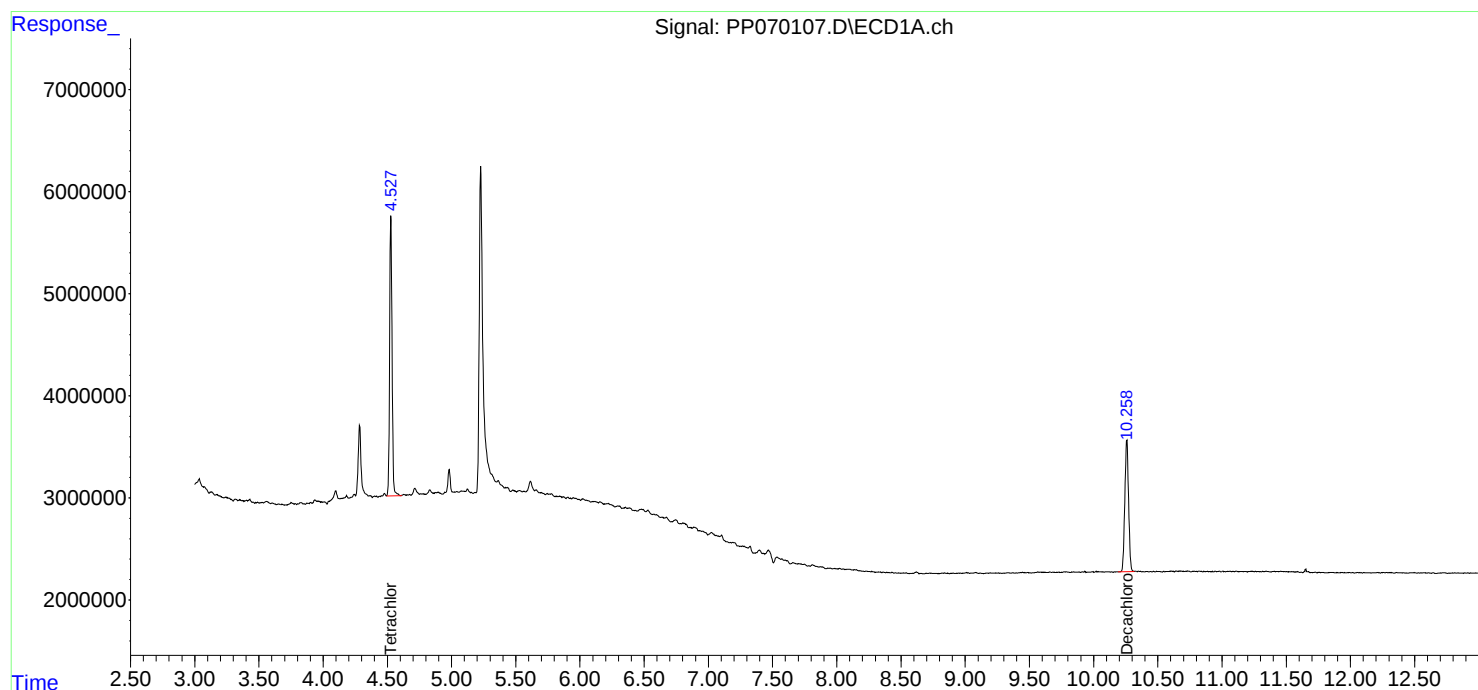


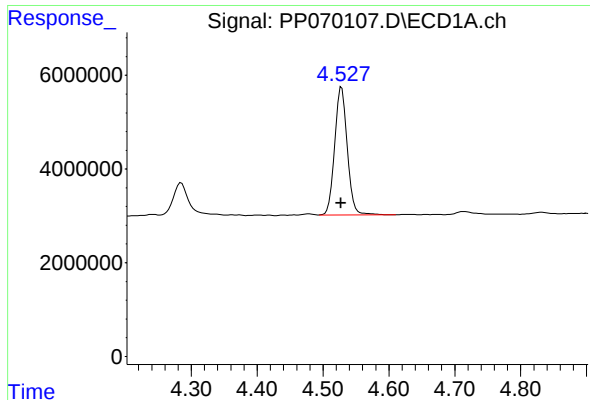

#1 Tetrachloro-m-xylene


R.T.: 4.528 min
Delta R.T.: 0.001 min
Response: 36394976
Conc: 24.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
P001-CLAY-CF01-02

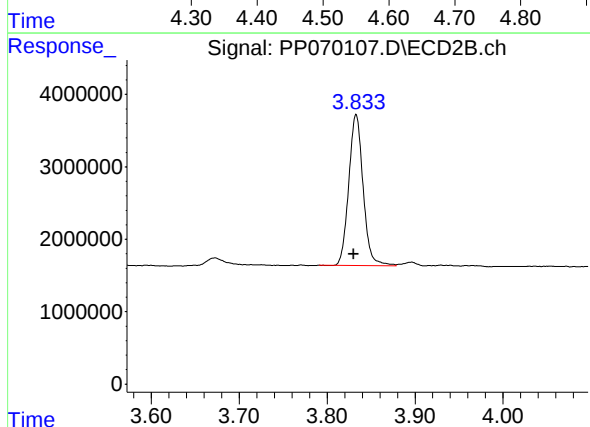


#1 Tetrachloro-m-xylene

R.T.: 3.833 min
Delta R.T.: 0.003 min
Response: 23673298
Conc: 24.76 ng/ml

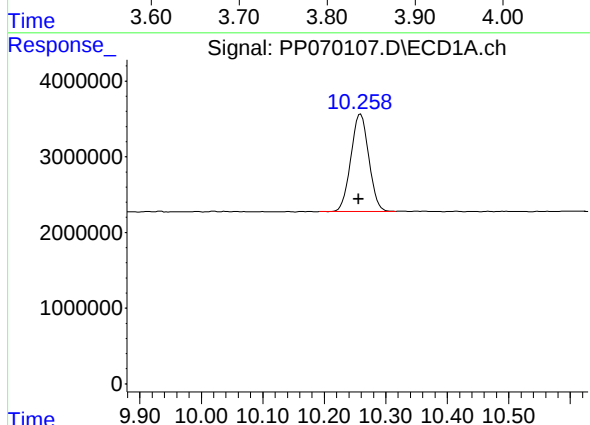

#2 Decachlorobiphenyl

R.T.: 10.259 min
Delta R.T.: 0.003 min
Response: 26080973
Conc: 22.90 ng/ml

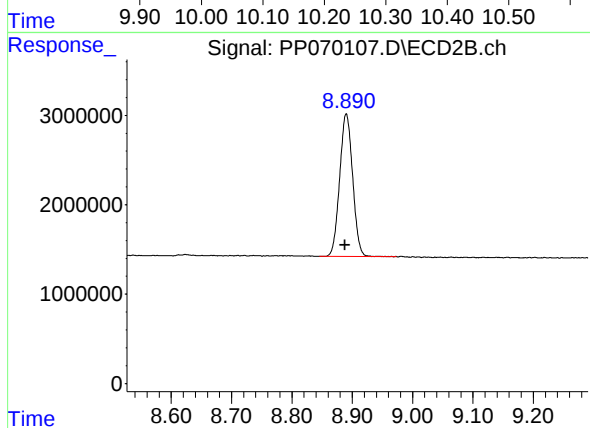

#2 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: 0.002 min
Response: 23780326
Conc: 21.94 ng/ml