

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
 Data File : PL094333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 12:32
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 13:07:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 13:07:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.769	124.0E6	193.5E6	50.000	50.000
28)	SA Decachlor...	9.048	7.903	102.9E6	189.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.695	3.765	61431327	66942088	500.000	500.000
24)	Chlordane-2	5.225	4.342	61194663	76300761	500.000	500.000
25)	Chlordane-3	5.935	4.971	209.0E6	235.5E6	500.000	500.000
26)	Chlordane-4	6.017	5.034	251.5E6	230.8E6	500.000	500.000
27)	Chlordane-5	6.866	5.929	48579793	80746470	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022125\
Data File : PL094333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 12:32
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 13:07:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 13:07:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

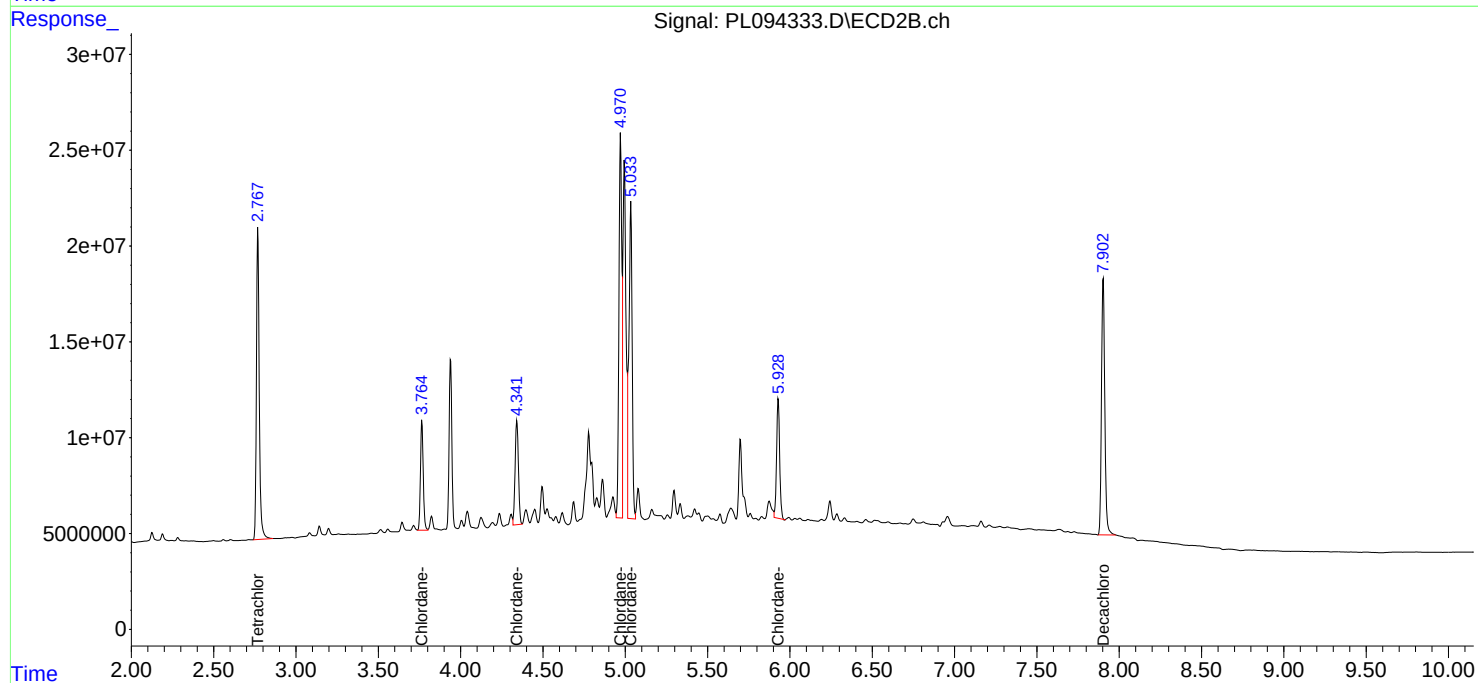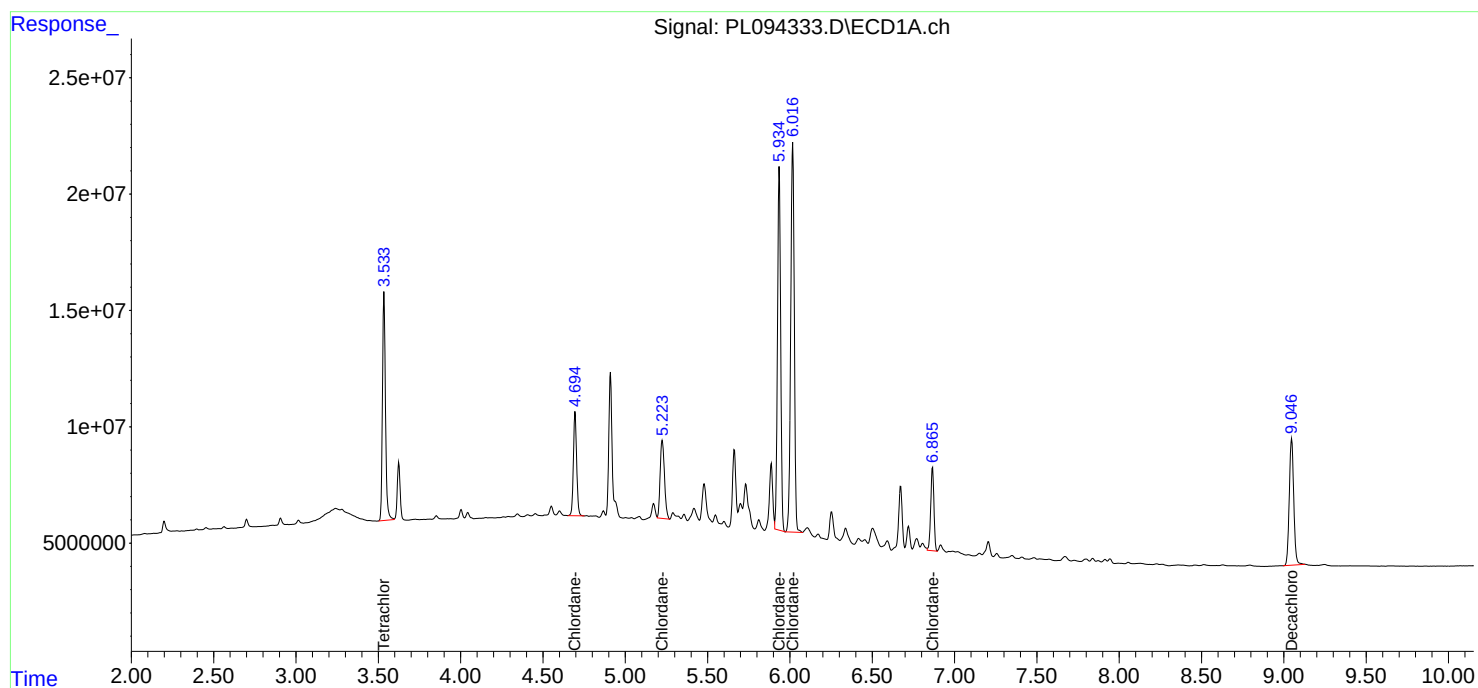


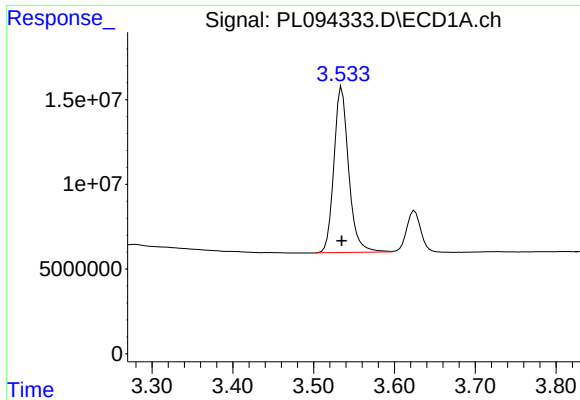

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 124004599
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

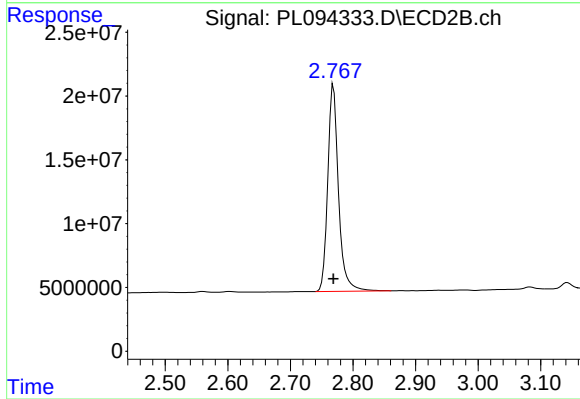


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: 0.000 min
Response: 193525723
Conc: 50.00 ng/ml

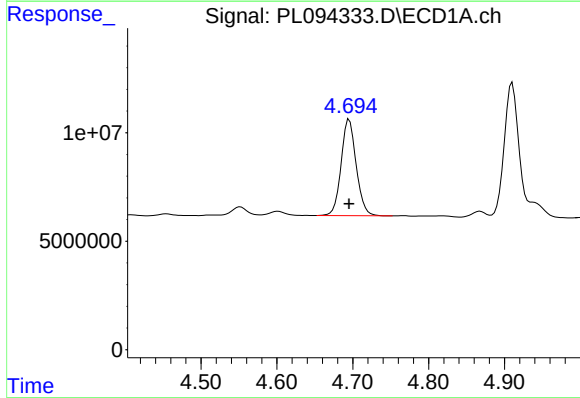


#23 Chlordane-1

R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 61431327
Conc: 500.00 ng/ml

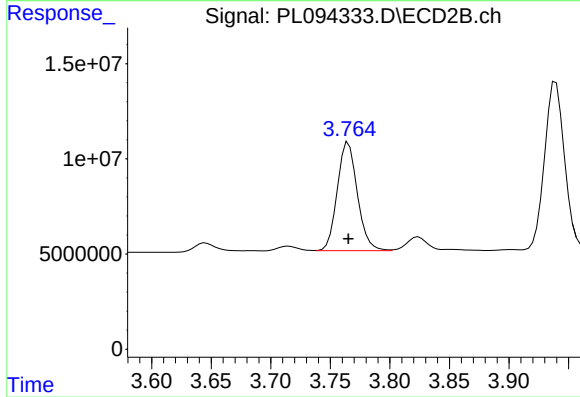

#23 Chlordane-1


R.T.: 3.765 min
Delta R.T.: 0.000 min
Response: 66942088
Conc: 500.00 ng/ml

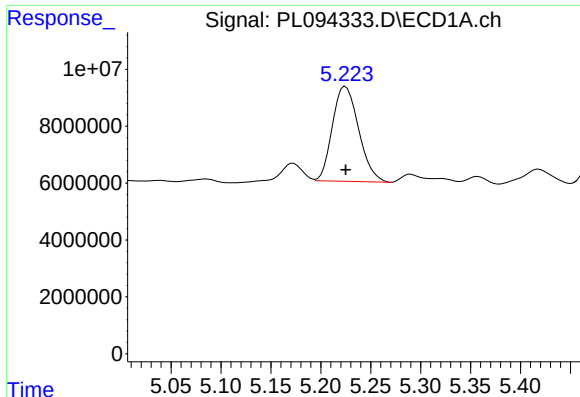

#24 Chlordane-2


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 61194663
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

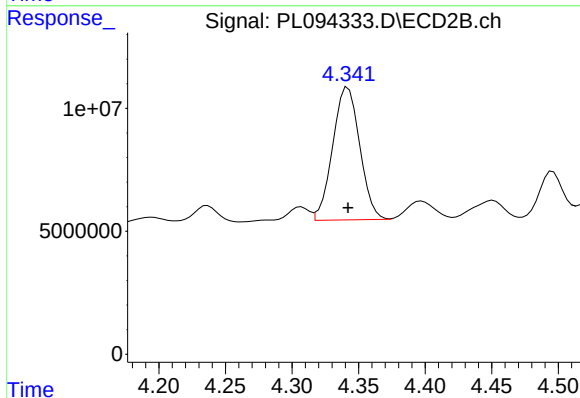


#24 Chlordane-2

R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 76300761
Conc: 500.00 ng/ml

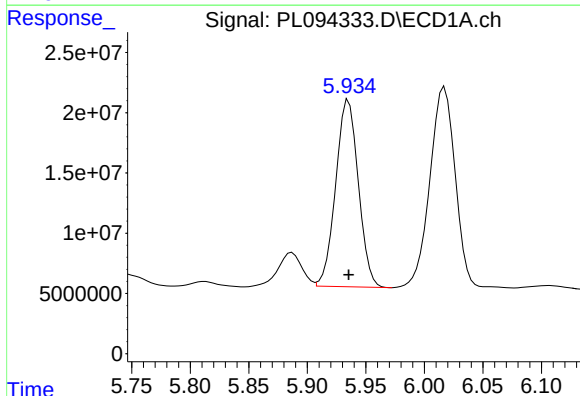


#25 Chlordane-3

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 208985572
Conc: 500.00 ng/ml

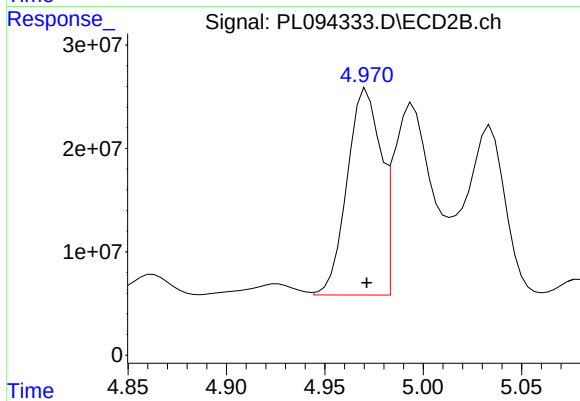

#25 Chlordane-3


R.T.: 4.971 min
Delta R.T.: 0.000 min
Response: 235511580
Conc: 500.00 ng/ml

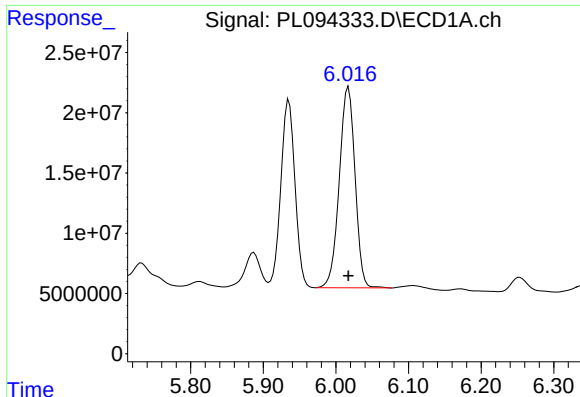

#26 Chlordane-4


R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 251488949
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

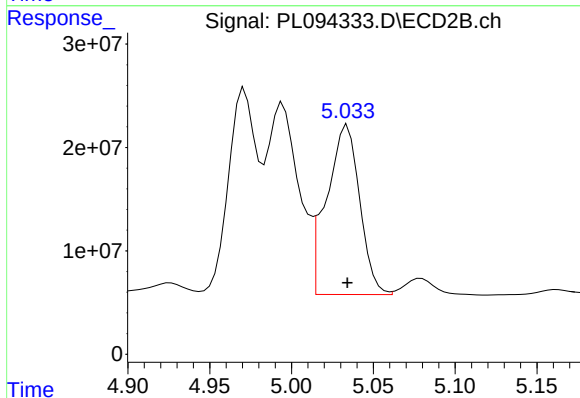


#26 Chlordane-4

R.T.: 5.034 min
Delta R.T.: 0.000 min
Response: 230825646
Conc: 500.00 ng/ml

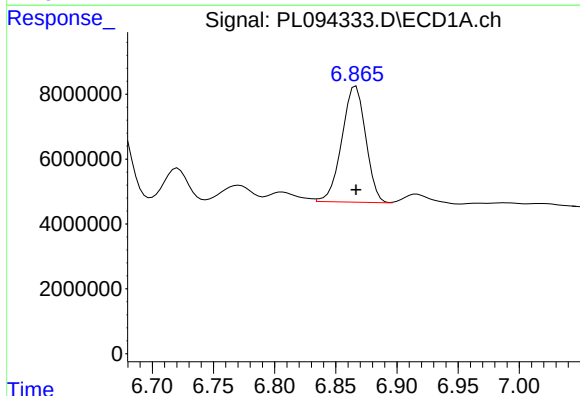


#27 Chlordane-5

R.T.: 6.866 min
Delta R.T.: 0.000 min
Response: 48579793
Conc: 500.00 ng/ml

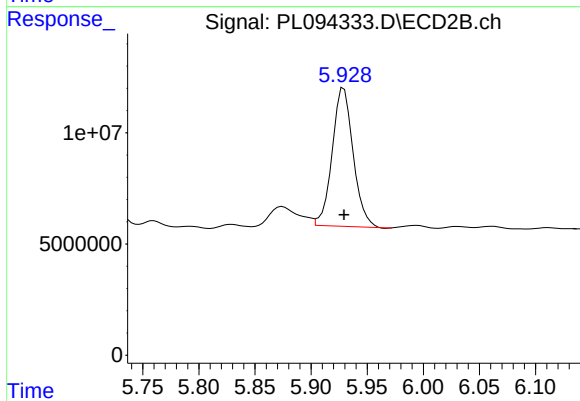

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 80746470
Conc: 500.00 ng/ml

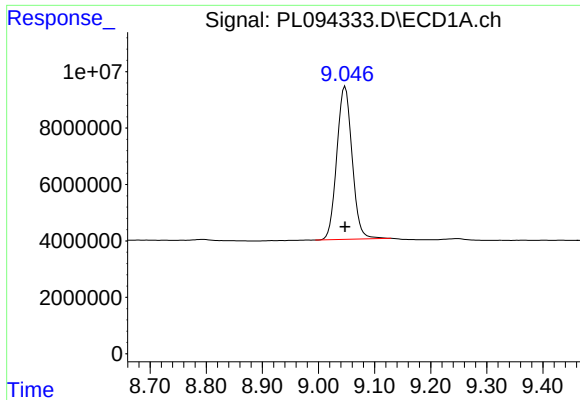

#28 Decachlorobiphenyl

R.T.: 9.048 min
Delta R.T.: 0.000 min
Response: 102855150
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

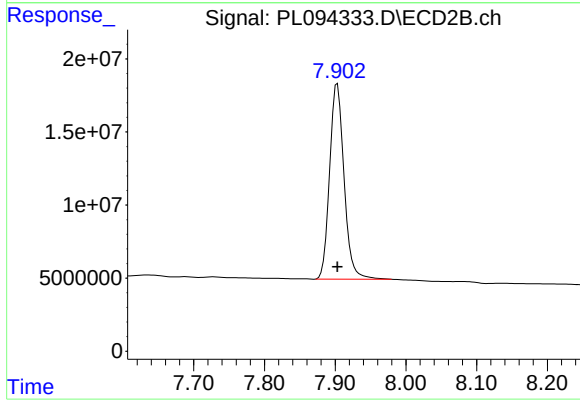

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 189493879
Conc: 50.00 ng/ml