
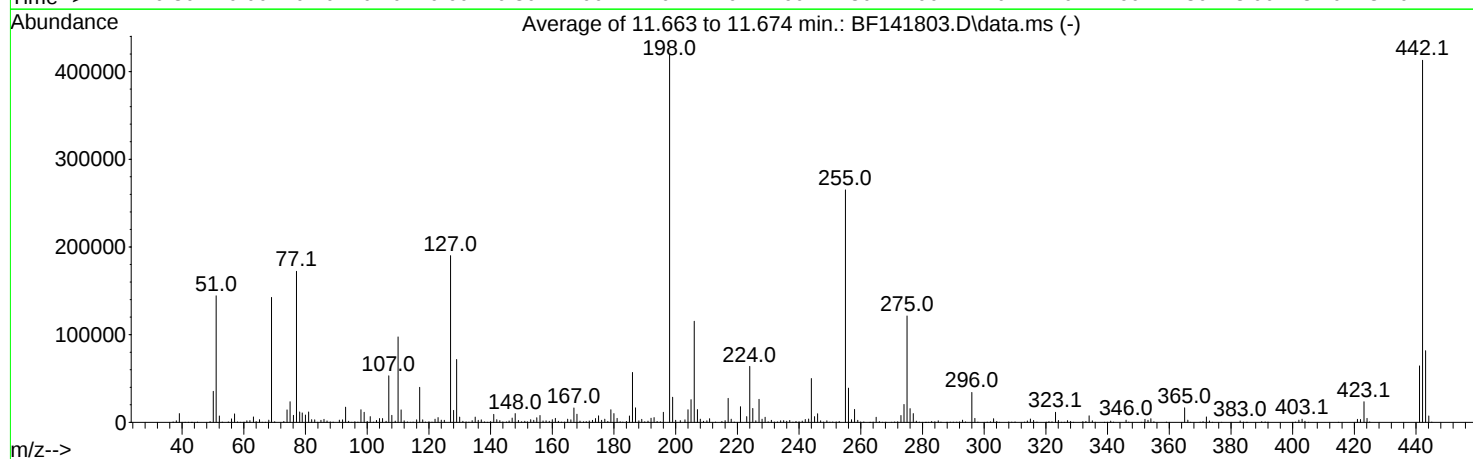


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022825\
Data File : BF141803.D
Acq On : 28 Feb 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 28 01:48:16 2025

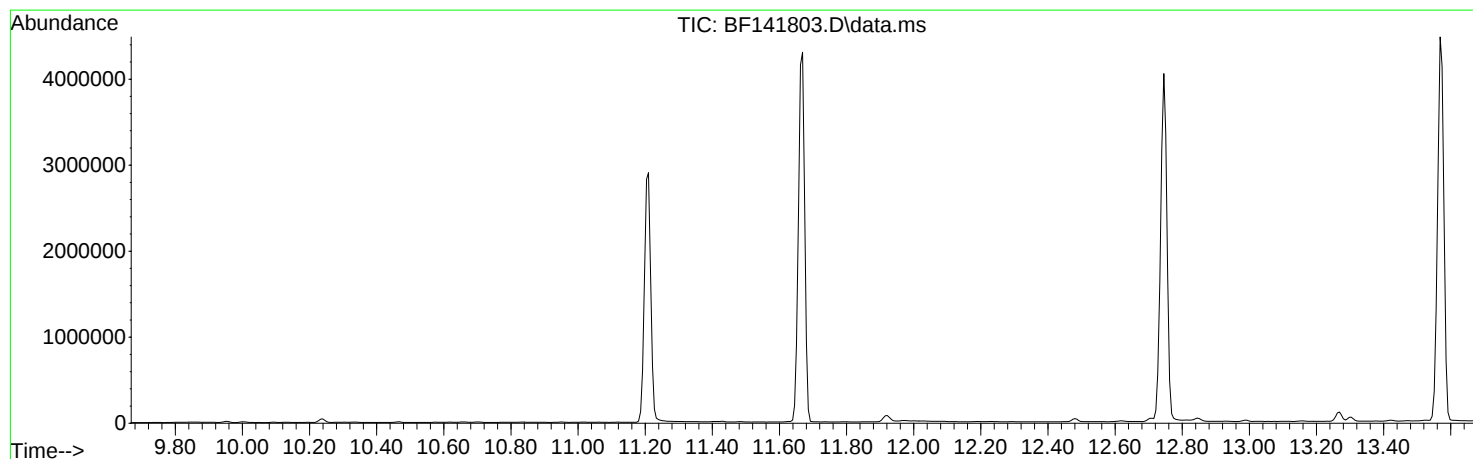

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	144251	PASS
68	69	0.00	2	1.9	2642	PASS
69	198	0.00	100	34.0	142486	PASS
70	69	0.00	2	0.5	772	PASS
127	198	10	80	45.3	190035	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	419456	PASS
199	198	5	9	6.8	28600	PASS
275	198	10	60	28.9	121301	PASS
365	198	1	100	4.0	16652	PASS
441	198	0.01	100	15.4	64435	PASS
442	442	50	100	100.0	412907	PASS
443	442	15	24	19.8	81691	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/28/2025	BNA_F	<u>BF141803.D</u>
Compound Name	Response	Retention Time
DDT	1100459	13.568
DDD	9936	13.268
DDE	542	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10478	1110937	0.94

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022825\
Data File : BF141803.D
Acq On : 28 Feb 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 28 11:14:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

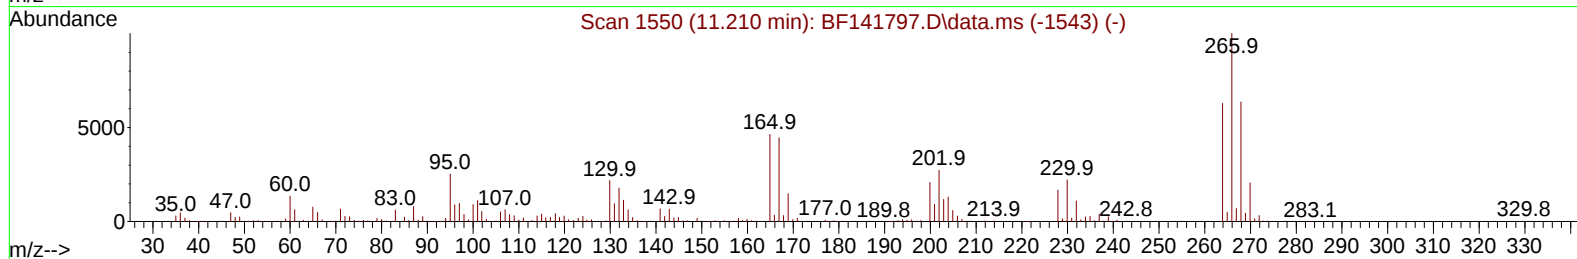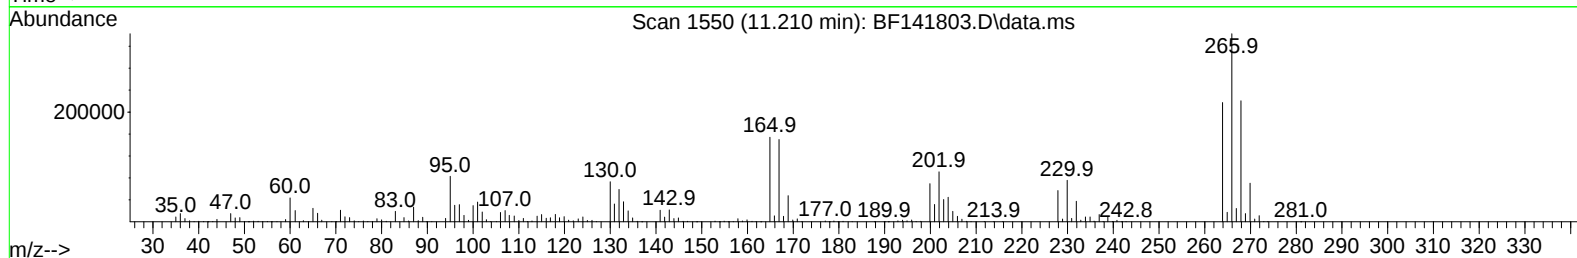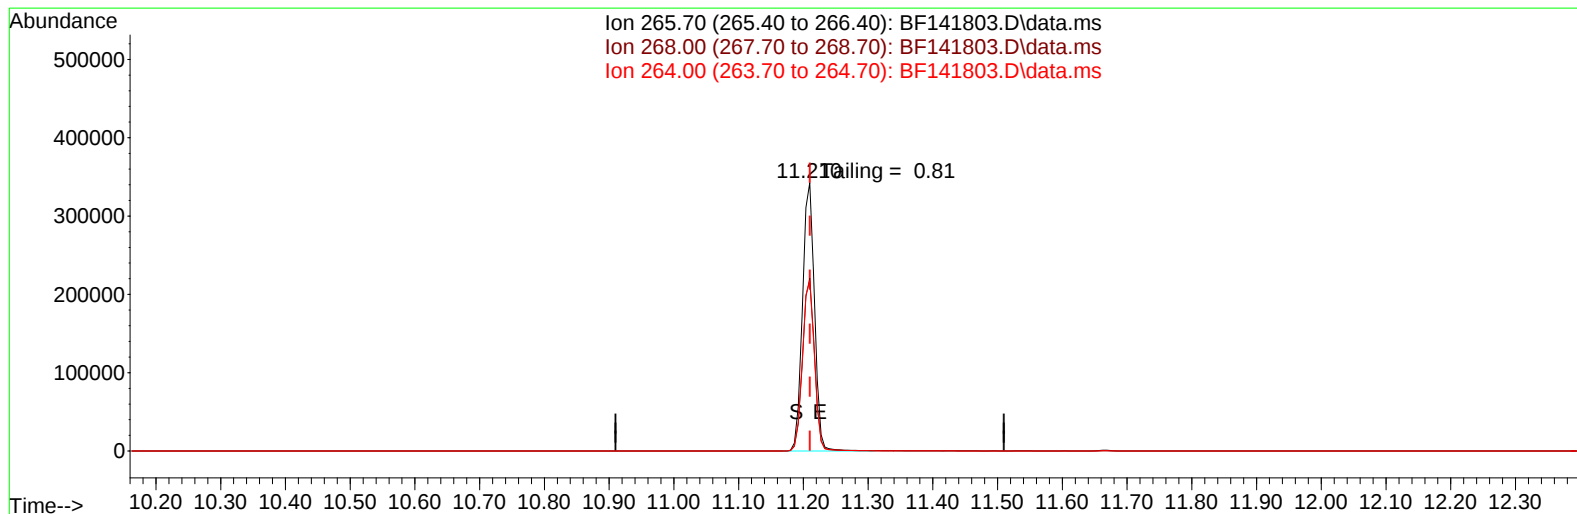

TIC: BF141803.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 17699.40 ng




response 444866

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.33
264.00	62.80	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022825\
Data File : BF141803.D
Acq On : 28 Feb 2025 09:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 28 11:14:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

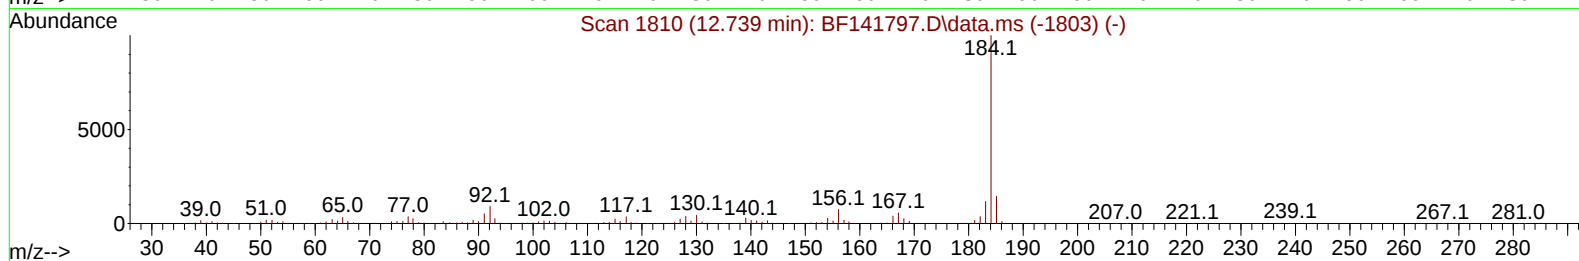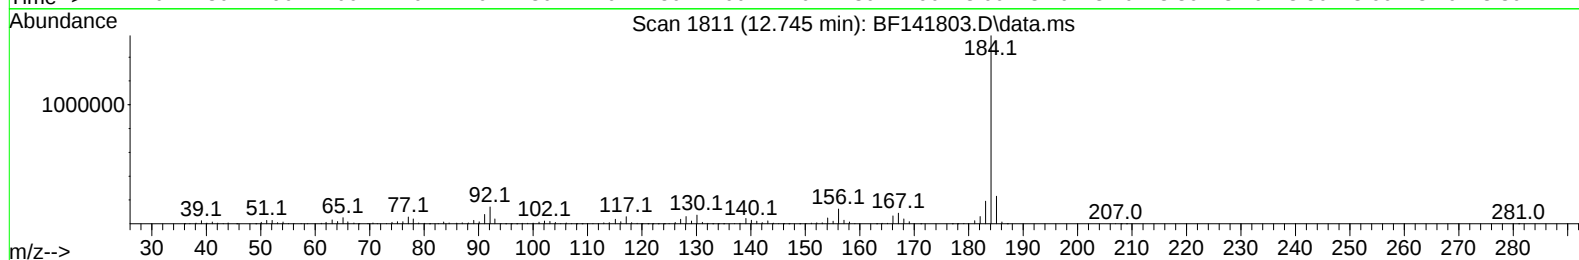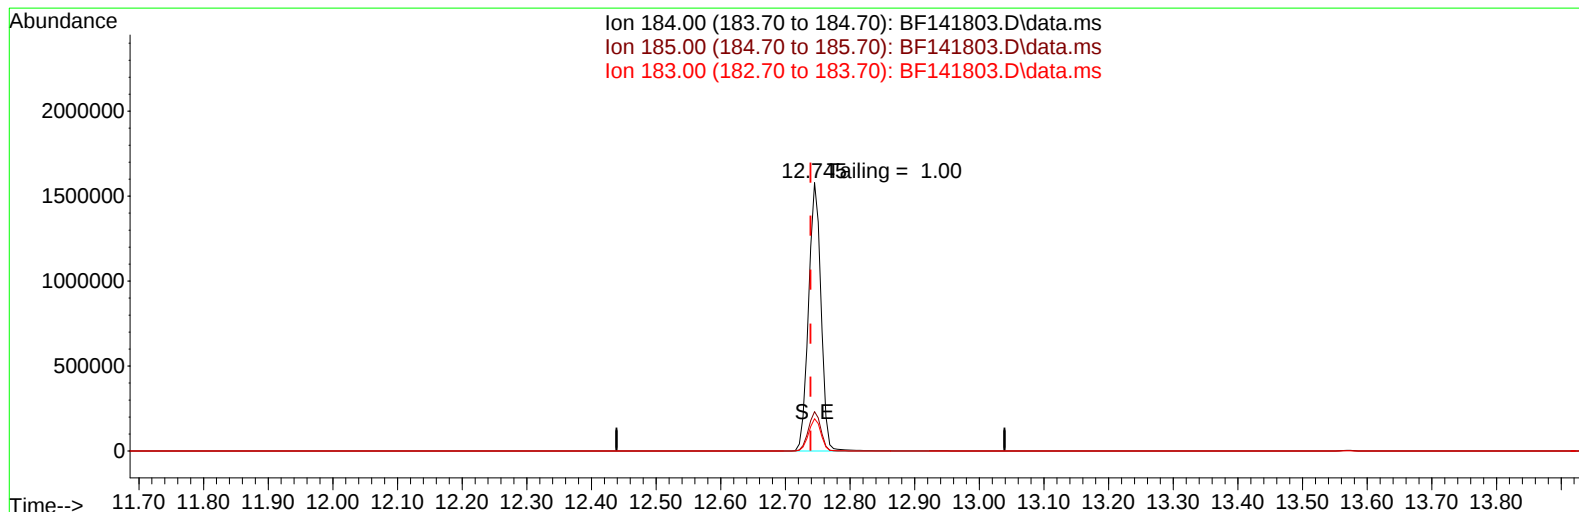

TIC: BF141803.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 81741.12 ng

response 2125556

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.68
183.00	11.70	12.05
0.00	0.00	0.00