
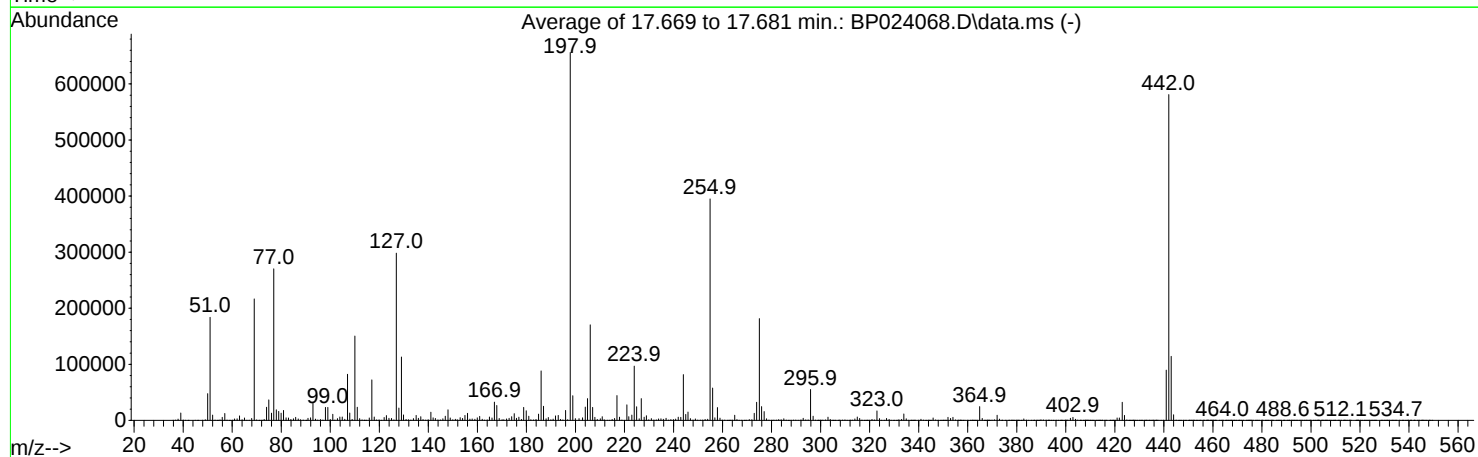


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021725\
Data File : BP024068.D
Acq On : 17 Feb 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 18 02:25:07 2025

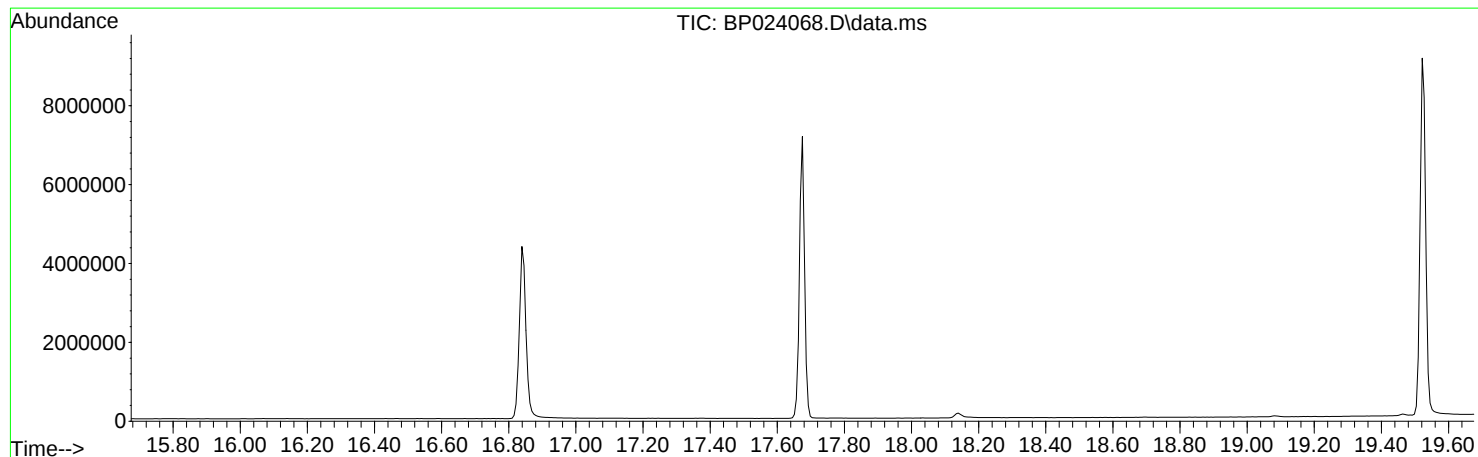

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	183862	PASS
68	69	0.00	2	1.6	3481	PASS
69	198	0.00	100	33.0	216627	PASS
70	69	0.00	2	0.5	1014	PASS
127	198	10	80	45.4	298086	PASS
197	198	0.00	2	0.2	1115	PASS
198	198	100	100	100.0	656087	PASS
199	198	5	9	6.7	44100	PASS
275	198	10	60	27.6	181397	PASS
365	198	1	100	3.8	24643	PASS
441	198	0.01	100	13.7	89573	PASS
442	442	100	100	100.0	580885	PASS
443	442	15	24	19.6	114083	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/17/2024	BNA_P	<u>BP024068.D</u>
Compound Name	Response	Retention Time
DDT	2093633	20.81
DDD	15524	20.41
DDE	198	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15722	2109355	0.75

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021725\
Data File : BP024068.D
Acq On : 17 Feb 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 18 02:37:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

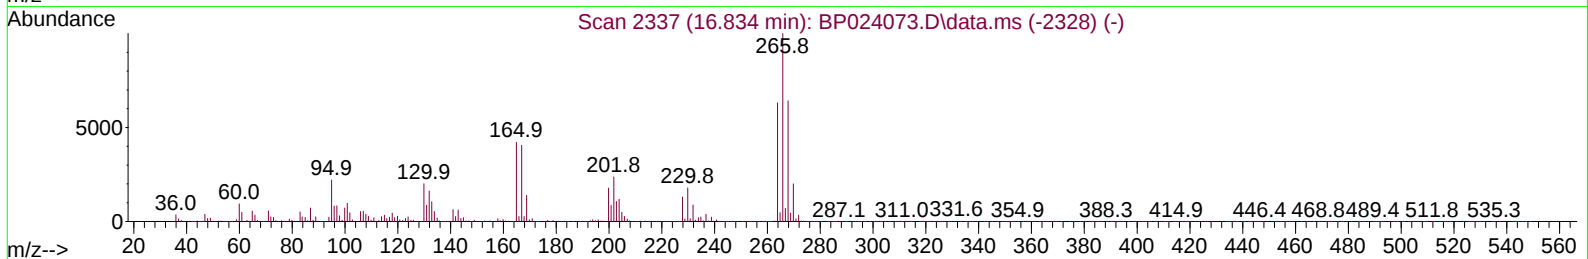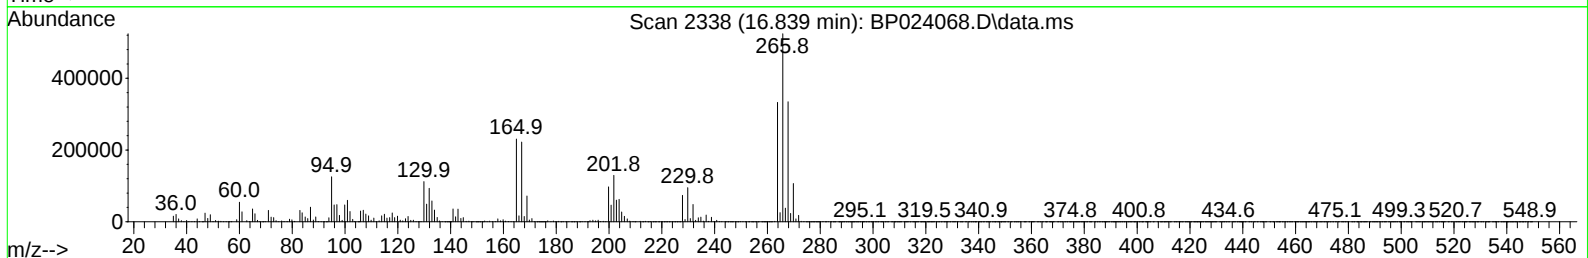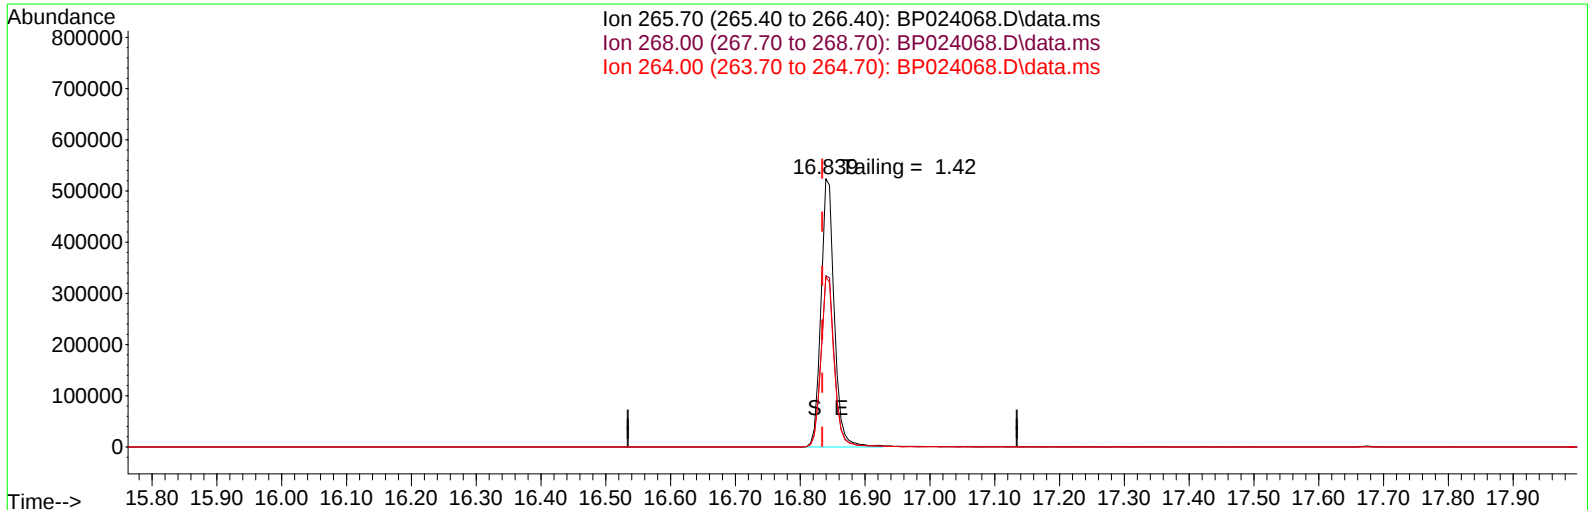

TIC: BP024068.D\data.ms

(70) Pentachlorophenol (C)

16.839min (+ 0.005) 214492.84 ng




response 758401

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.87
264.00	63.10	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021725\
Data File : BP024068.D
Acq On : 17 Feb 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 18 02:37:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

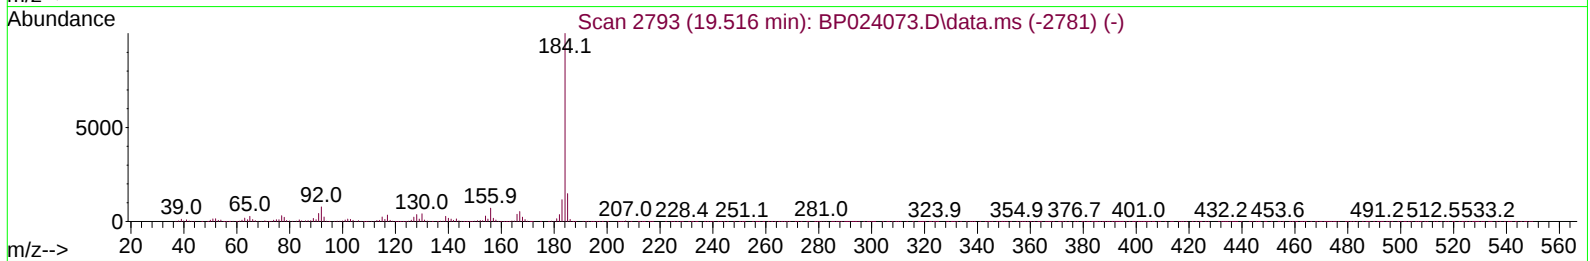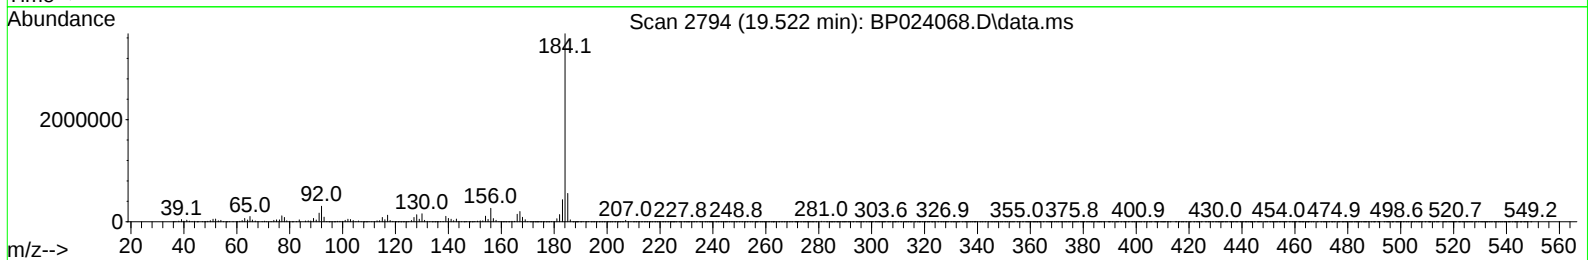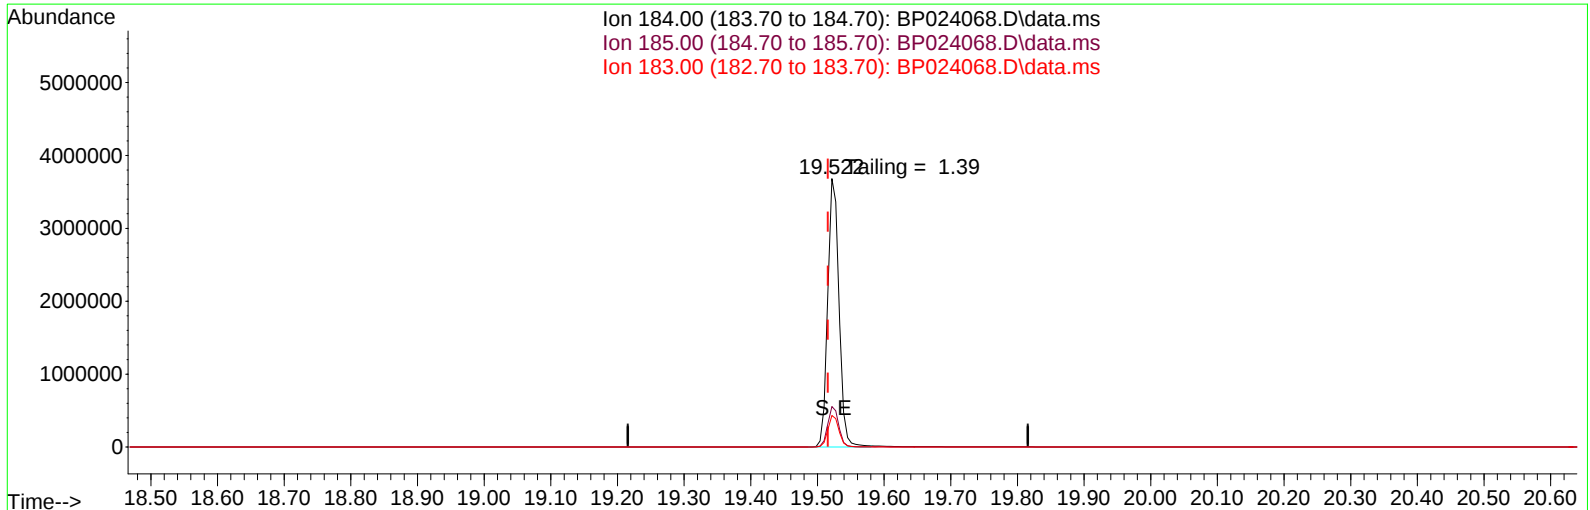

TIC: BP024068.D\data.ms

(77) Benzidine

19.522min (+ 0.006) 903747.62 ng

response 4372031

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.09
183.00	11.60	11.74
0.00	0.00	0.00