
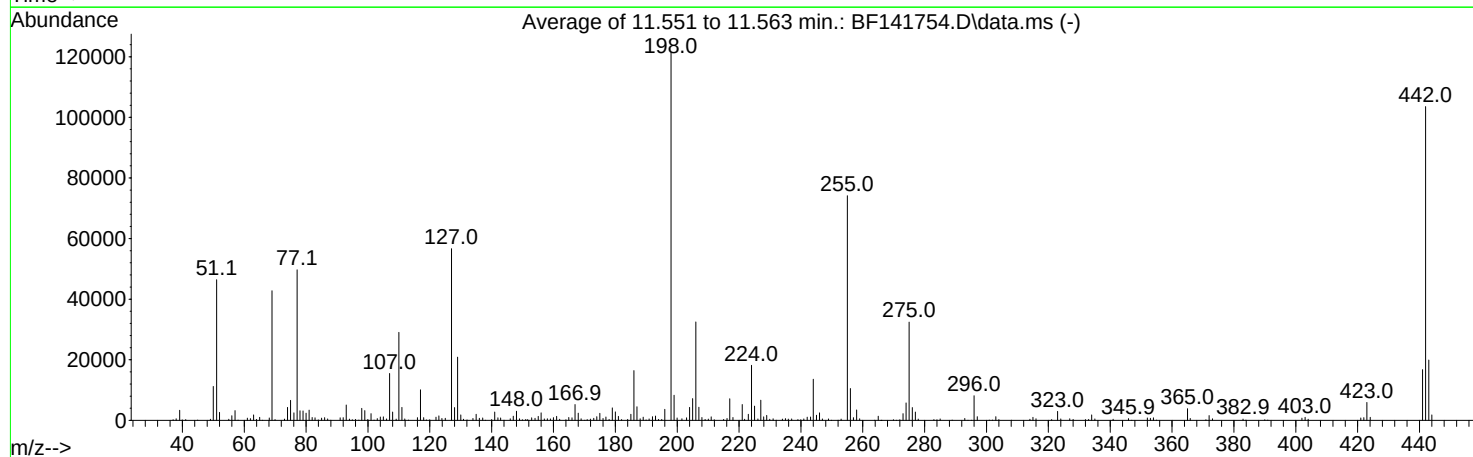


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141754.D
Acq On : 25 Feb 2025 09:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

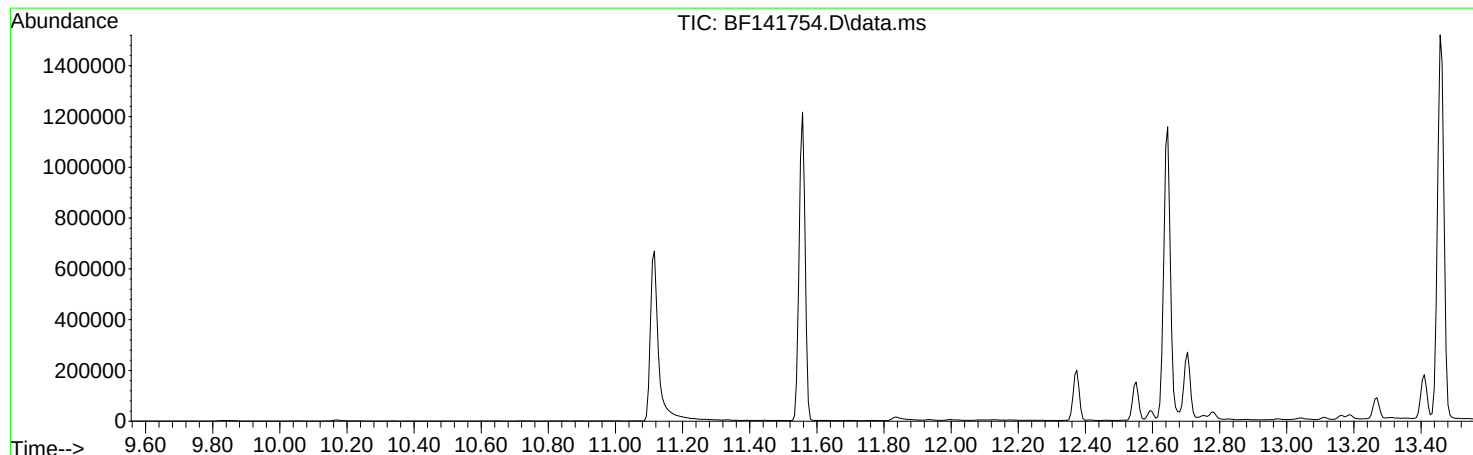

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	46424	PASS
68	69	0.00	2	1.9	816	PASS
69	198	0.00	100	35.2	42755	PASS
70	69	0.00	2	0.6	249	PASS
127	198	10	80	46.7	56675	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121405	PASS
199	198	5	9	6.8	8275	PASS
275	198	10	60	26.7	32403	PASS
365	198	1	100	3.2	3833	PASS
441	198	0.01	100	13.8	16753	PASS
442	442	50	100	100.0	103555	PASS
443	442	15	24	19.2	19914	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/25/2025	BNA_F	<u>BF141754.D</u>
Compound Name	Response	Retention Time
DDT	391181	13.457
DDD	10426	13.186
DDE	753	12.828
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11179	402360	2.78

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141754.D
Acq On : 25 Feb 2025 09:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 25 09:54:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

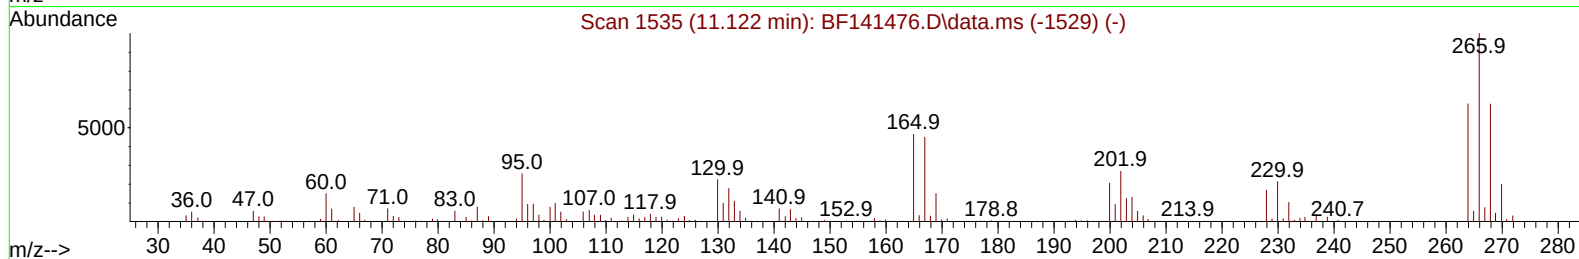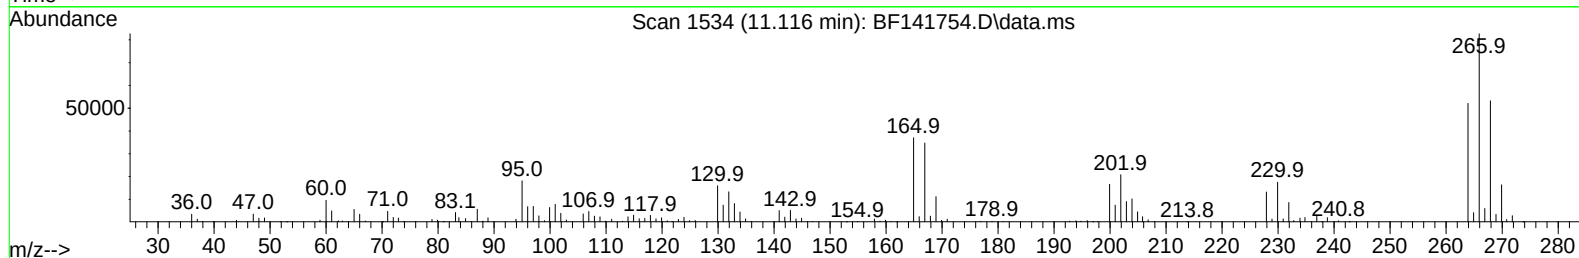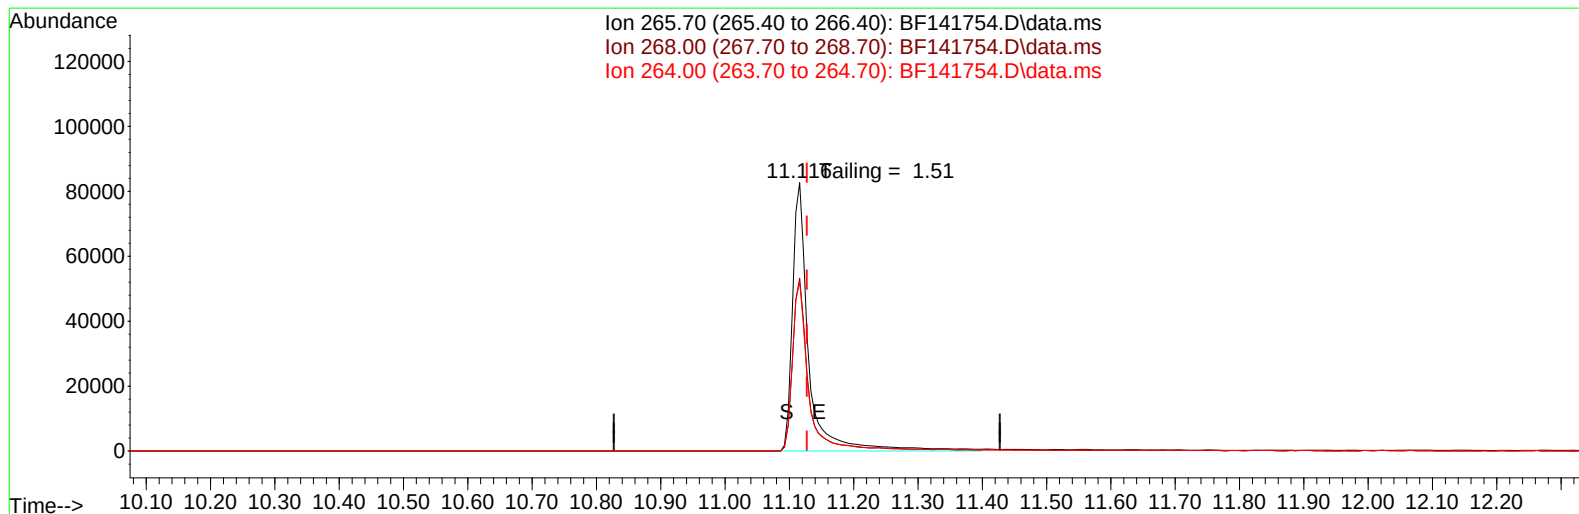

TIC: BF141754.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.011) 155220.49 ng




response 143922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.39
264.00	62.60	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022525\
Data File : BF141754.D
Acq On : 25 Feb 2025 09:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 25 09:54:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

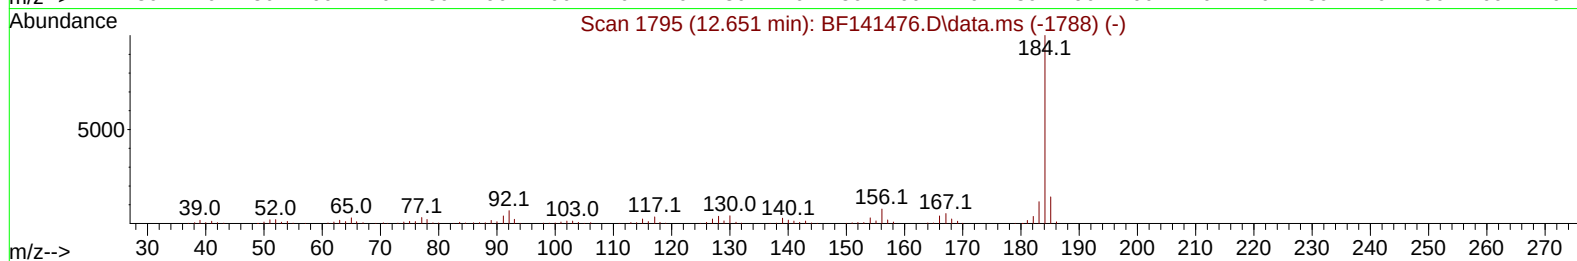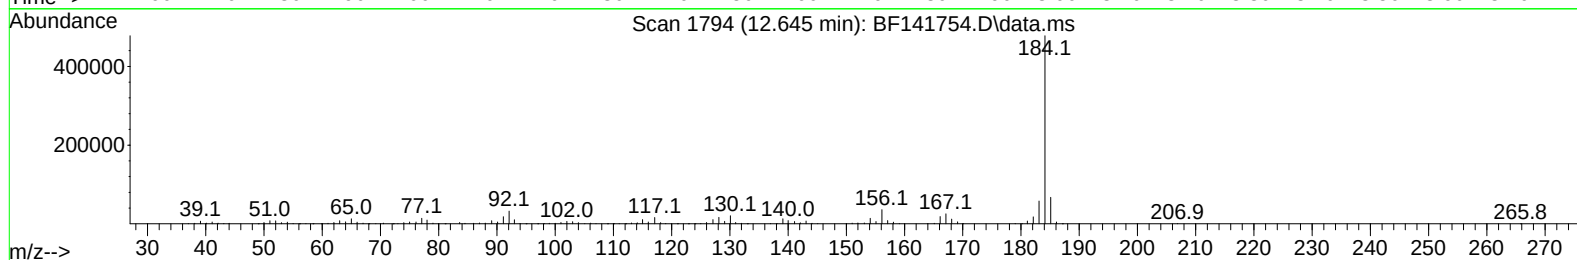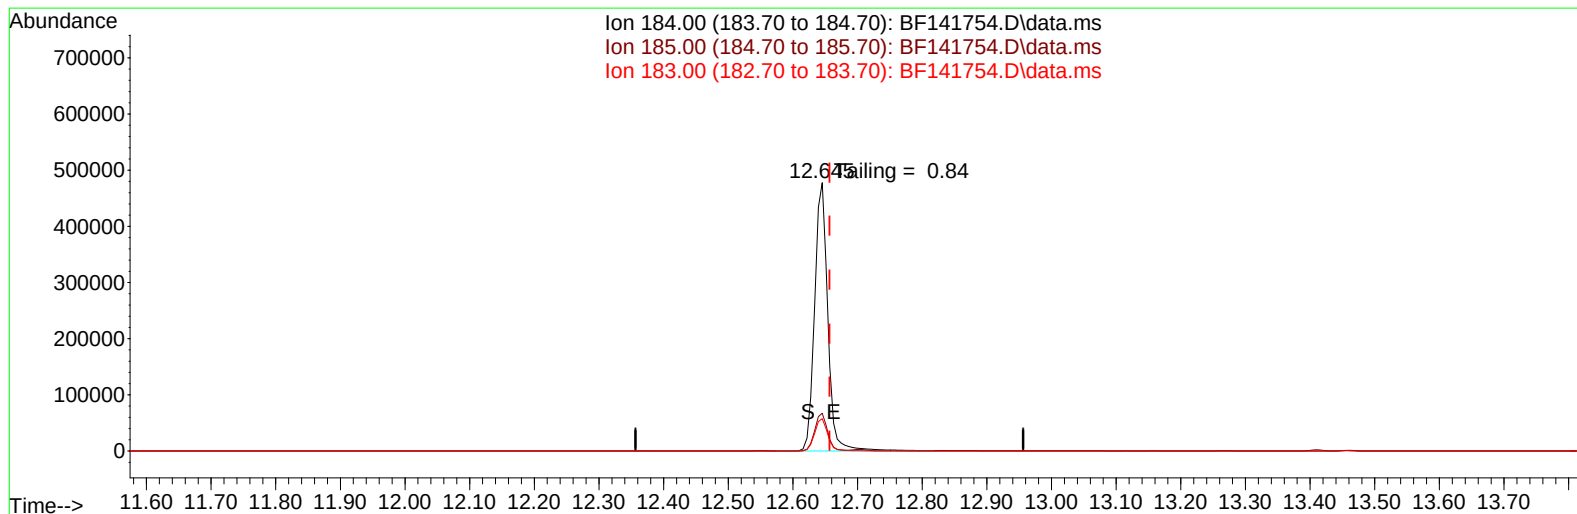

TIC: BF141754.D\data.ms

(77) Benzidine

12.645min (-0.012) 0.00 ng

response 681801

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	11.60	12.08
0.00	0.00	0.00