

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
 Data File : BF141776.D
 Acq On : 26 Feb 2025 11:49
 Operator : RC/JU
 Sample : PB166853BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166853BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	559	564	592	rBV	1791256	2537814	73.52%	13.446%
2	6.428	731	737	771	rBV	1693710	2506219	72.61%	13.279%
3	6.781	792	797	813	rVB	371805	480196	13.91%	2.544%
4	7.345	887	893	922	rBV	1167216	1673975	48.50%	8.869%
5	8.063	1009	1015	1034	rBV	426239	631629	18.30%	3.347%
6	9.134	1191	1197	1231	rBV	2277833	3198026	92.65%	16.945%
7	9.816	1307	1313	1334	rBV	520195	734935	21.29%	3.894%
8	10.604	1442	1447	1479	rBV	1293803	1878893	54.43%	9.955%
9	11.298	1560	1565	1585	rBV	513083	761297	22.06%	4.034%
10	12.886	1829	1835	1840	rBV	2609654	3451671	100.00%	18.288%
11	13.939	2009	2014	2029	rBV	373186	562712	16.30%	2.981%
12	15.386	2254	2260	2272	rBV	243364	456086	13.21%	2.417%




Sum of corrected areas: 18873453

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141776.D
Acq On : 26 Feb 2025 11:49
Operator : RC/JU
Sample : PB166853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166853BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

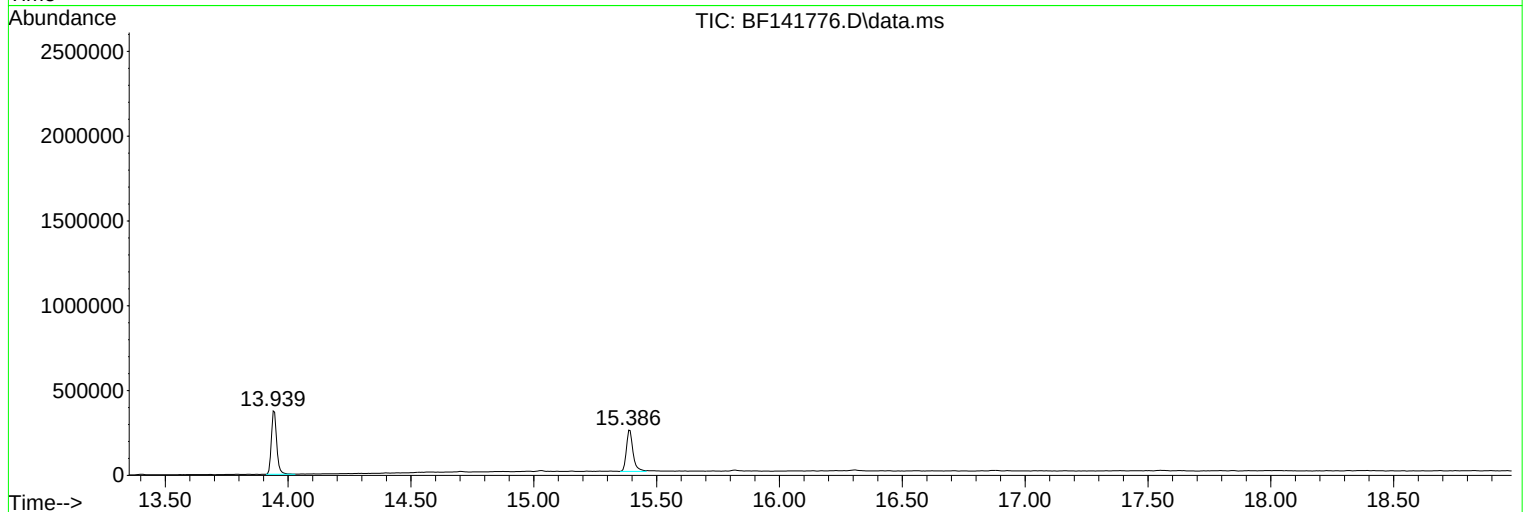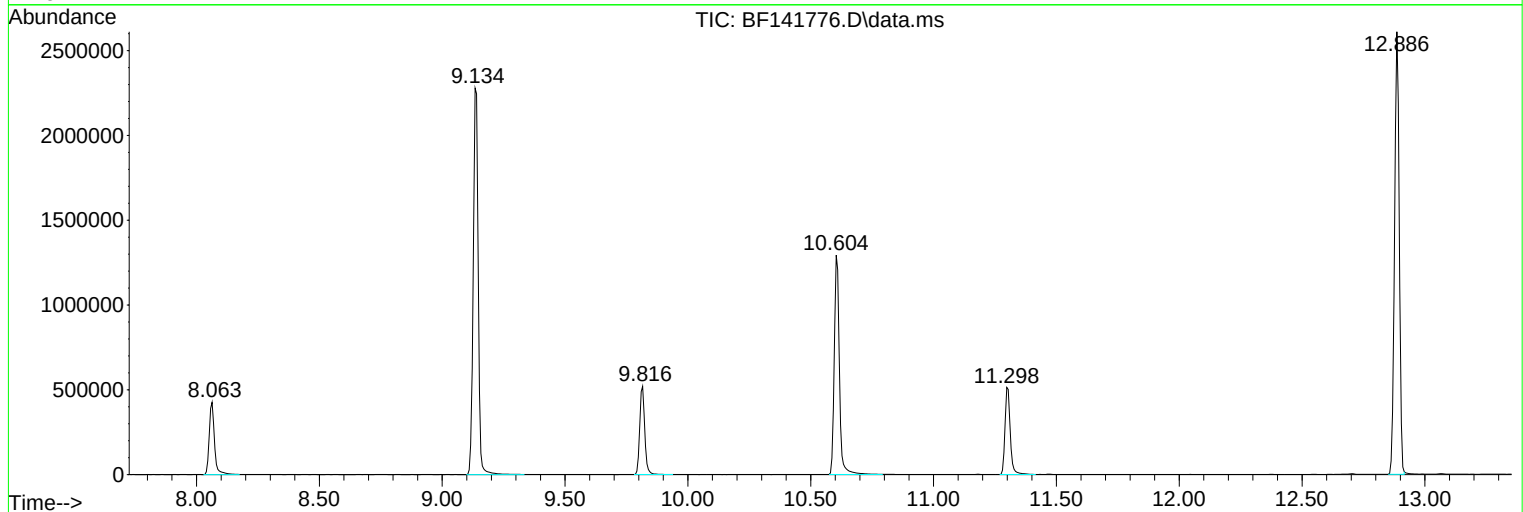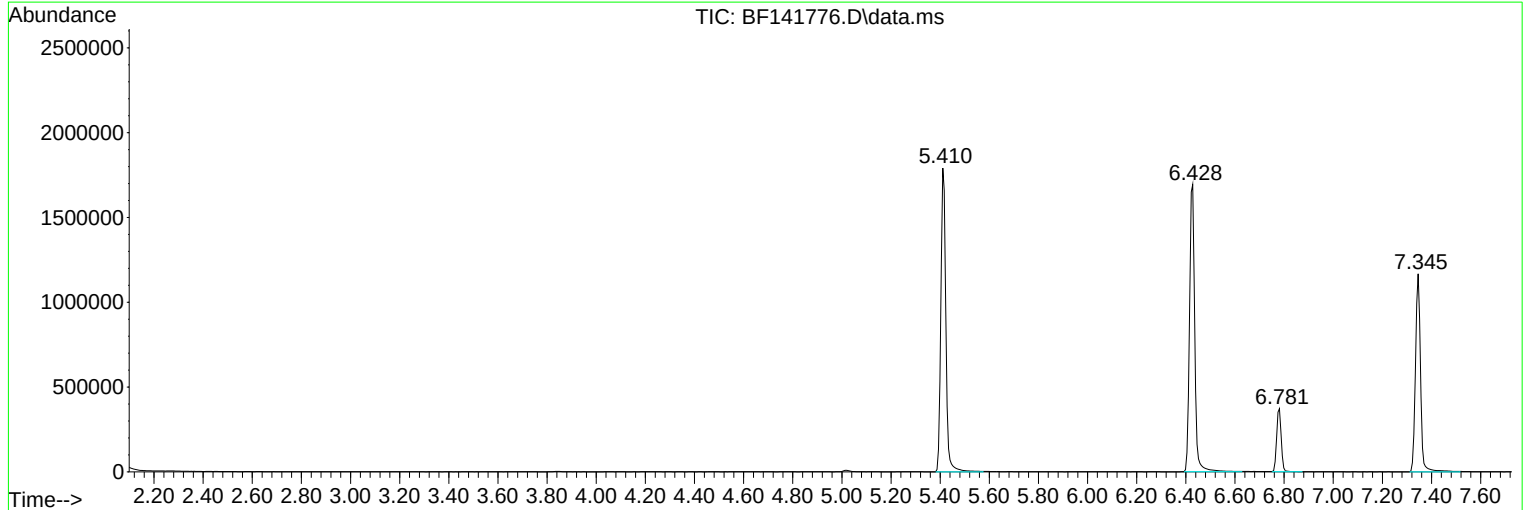

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141776.D
Acq On : 26 Feb 2025 11:49
Operator : RC/JU
Sample : PB166853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166853BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141776.D
Acq On : 26 Feb 2025 11:49
Operator : RC/JU
Sample : PB166853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166853BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------