


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020625\
Data File : BF141471.D
Acq On : 06 Feb 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

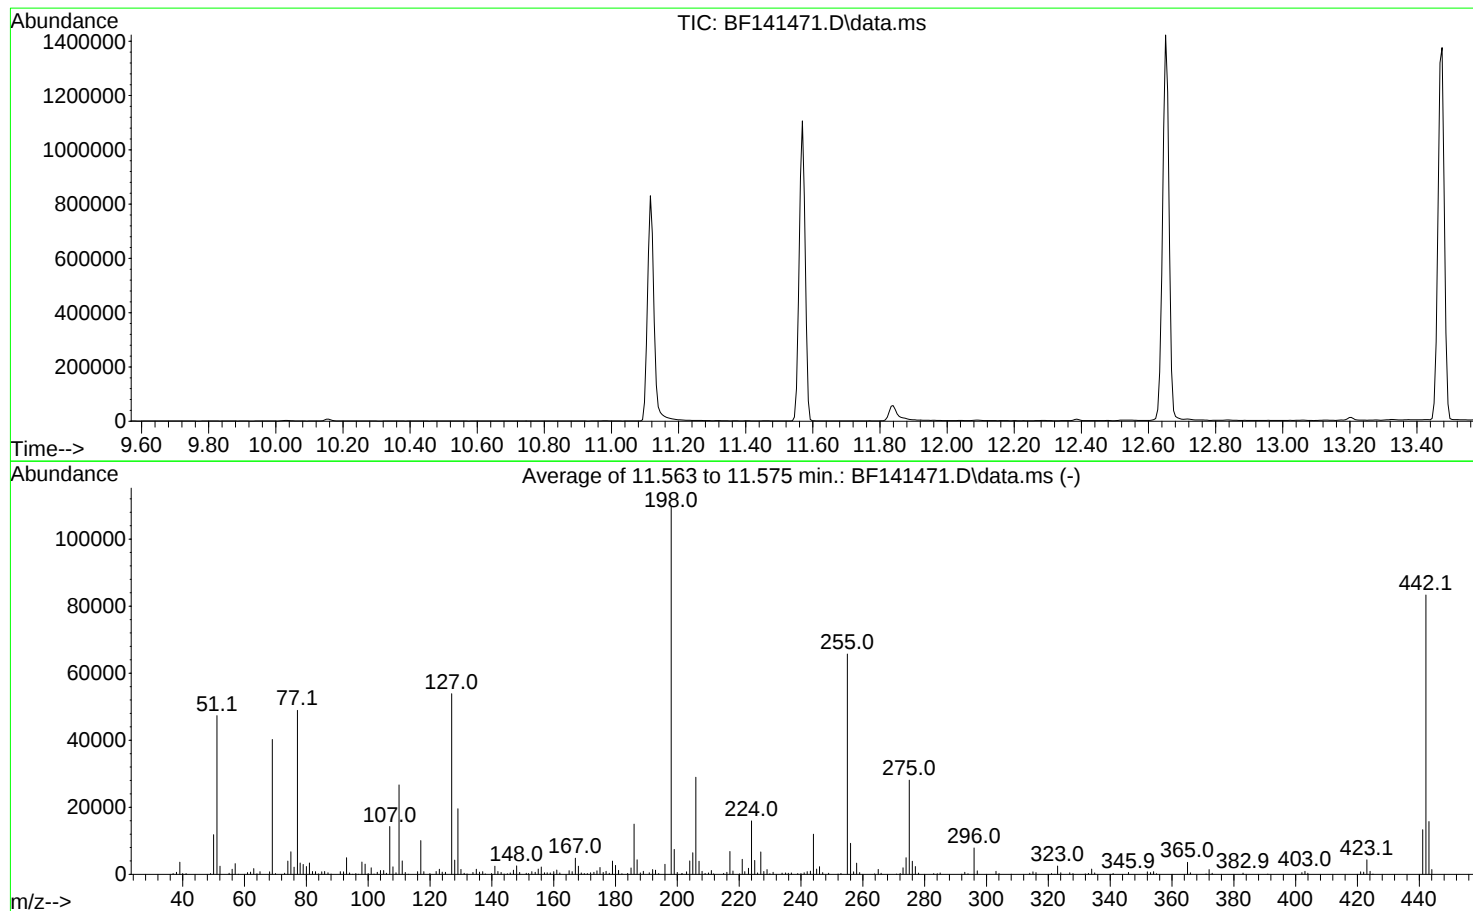

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	43.2	47360	PASS
68	69	0.00	2	1.9	756	PASS
69	198	0.00	100	36.7	40248	PASS
70	69	0.00	2	0.5	221	PASS
127	198	10	80	49.1	53877	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109720	PASS
199	198	5	9	6.8	7444	PASS
275	198	10	60	25.6	28133	PASS
365	198	1	100	3.3	3599	PASS
441	198	0.01	100	12.2	13341	PASS
442	442	50	100	100.0	83323	PASS
443	442	15	24	18.9	15754	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/6/2025	BNA_F	<u>BF141471.D</u>
Compound Name	Response	Retention Time
DDT	348871	13.475
DDD	6398	13.204
DDE	521	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6919	355790	1.94

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020625\
Data File : BF141471.D
Acq On : 06 Feb 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 06 13:09:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 13:08:53 2025
Response via : Initial Calibration

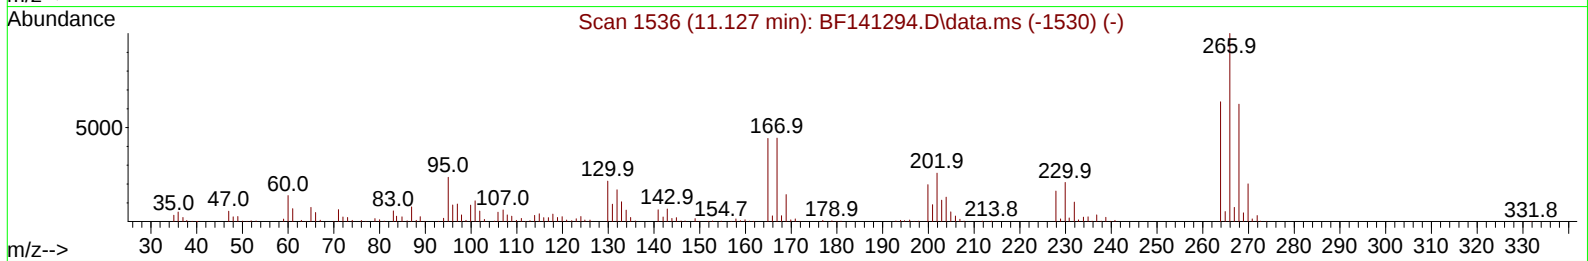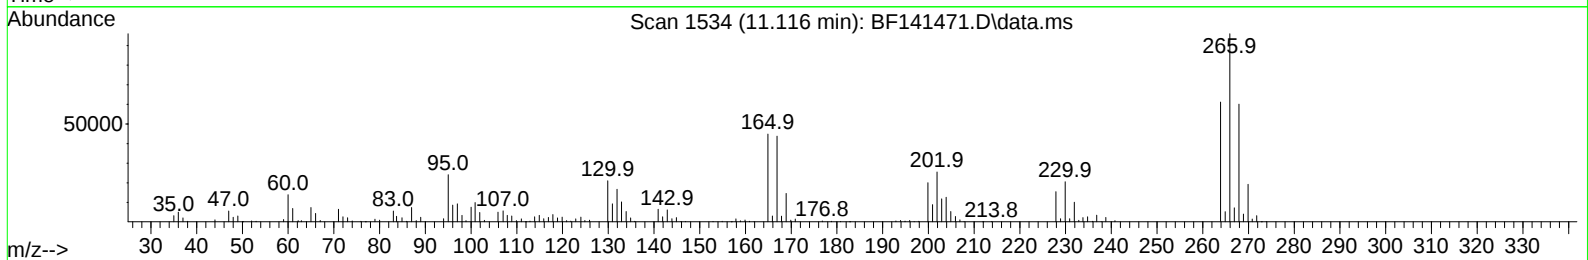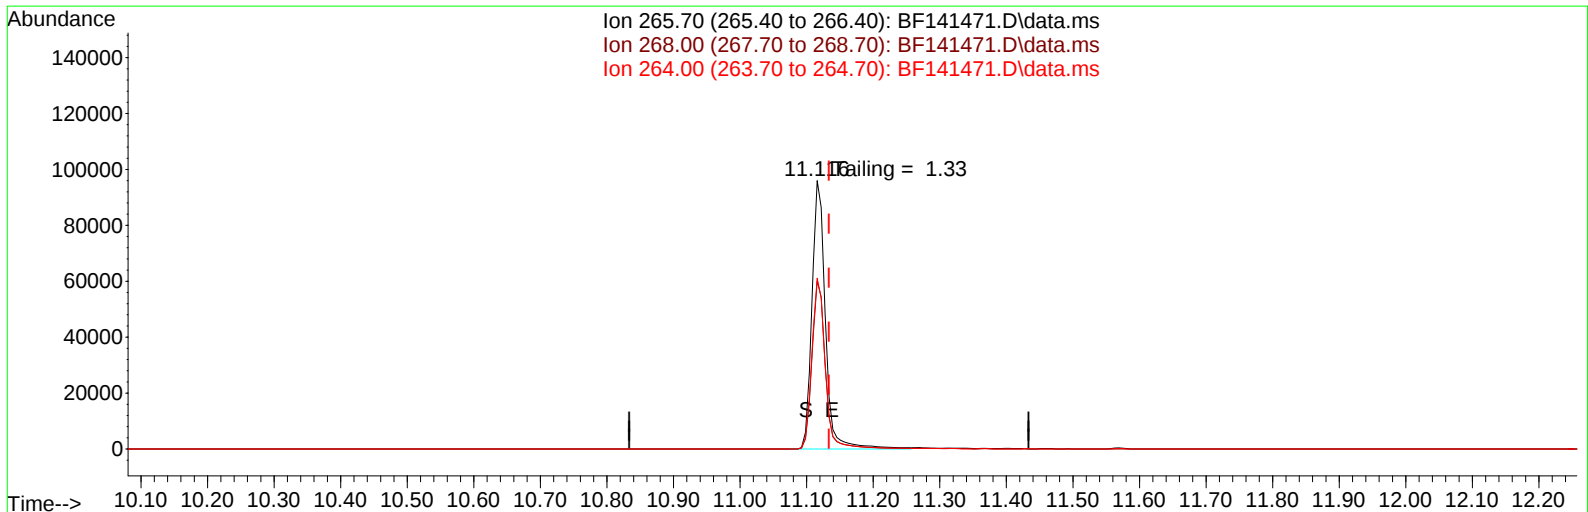

TIC: BF141471.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.018) 32915.33 ng




response 135048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.59
264.00	63.70	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020625\
Data File : BF141471.D
Acq On : 06 Feb 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 06 13:09:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 13:08:53 2025
Response via : Initial Calibration

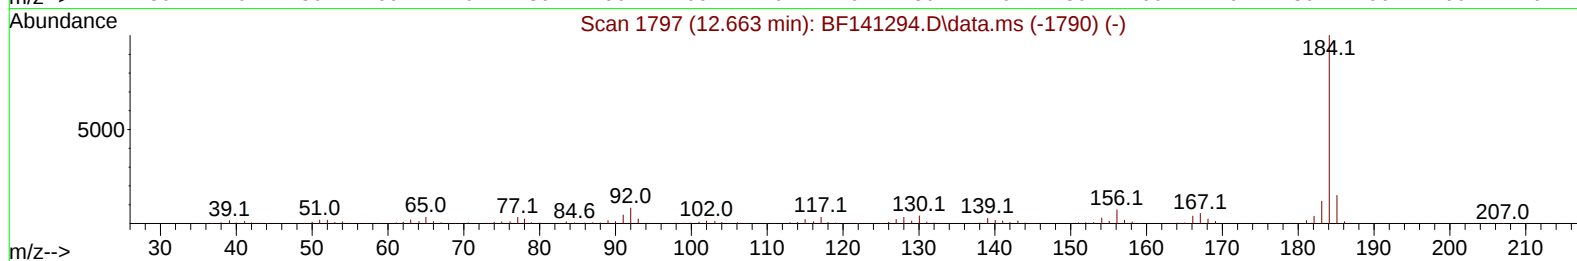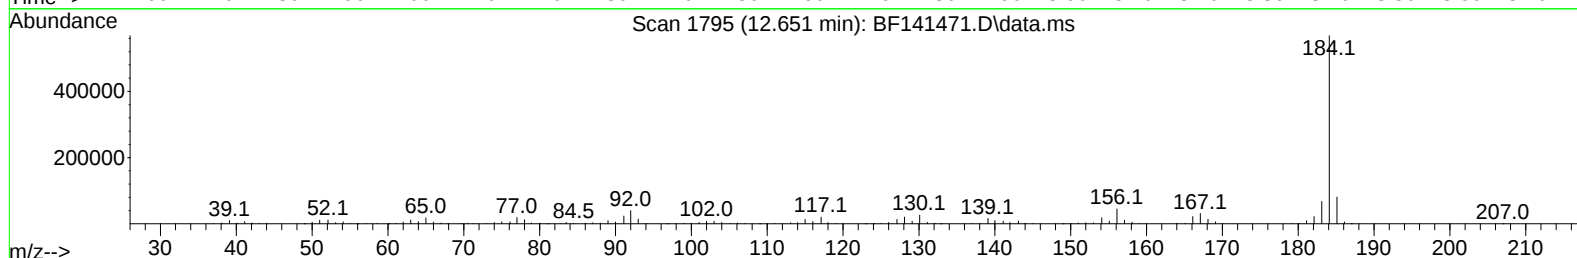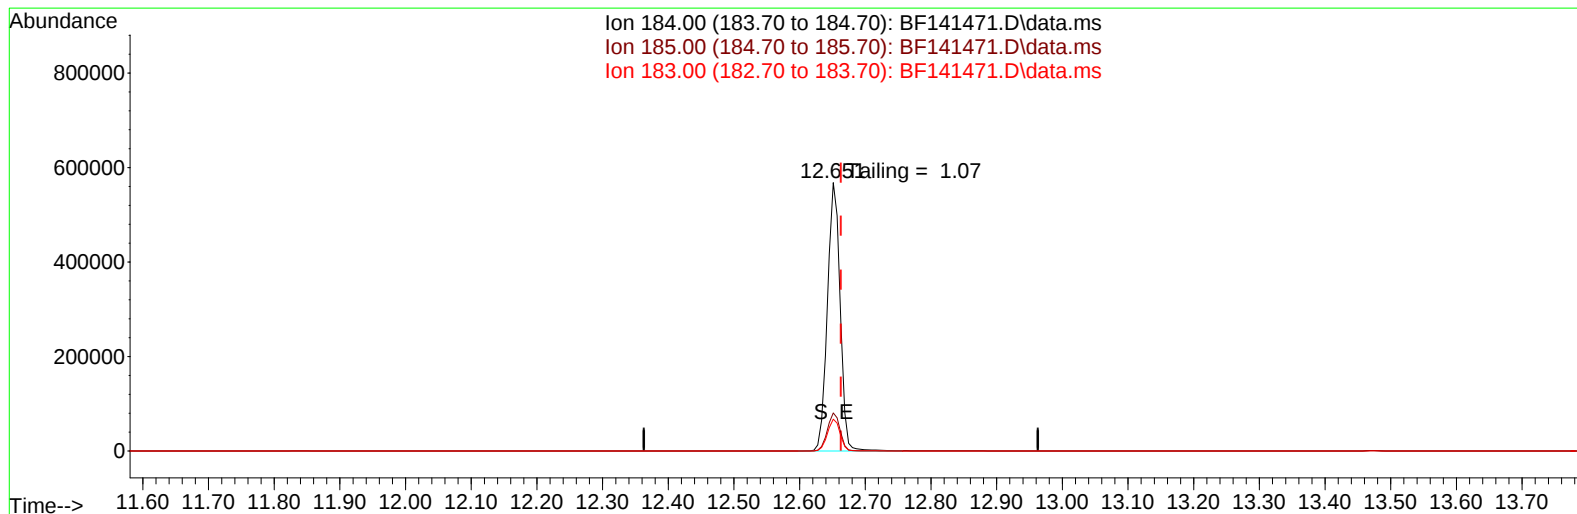

TIC: BF141471.D\data.ms

(77) Benzidine

12.651min (-0.012) 0.00 ng

response 764582

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.21
183.00	11.90	11.88
0.00	0.00	0.00