
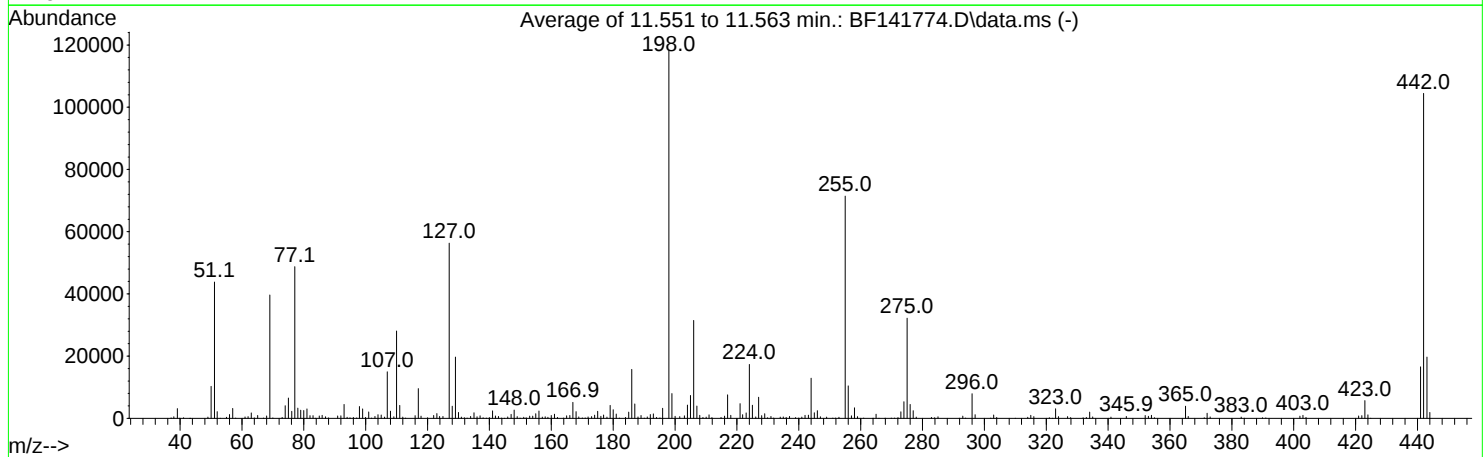


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141774.D
Acq On : 26 Feb 2025 10:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

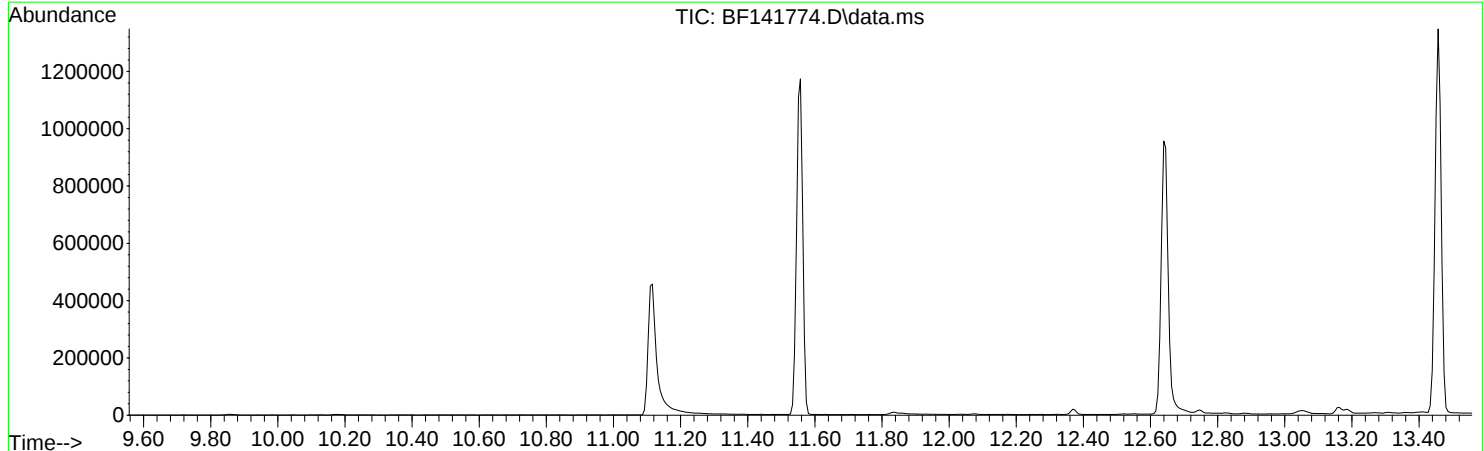

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1601

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	37.0	43792	PASS
68	69	0.00	2	1.9	769	PASS
69	198	0.00	100	33.5	39664	PASS
70	69	0.00	2	0.4	146	PASS
127	198	10	80	47.6	56291	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118229	PASS
199	198	5	9	6.8	7983	PASS
275	198	10	60	27.2	32213	PASS
365	198	1	100	3.3	3888	PASS
441	198	0.01	100	14.0	16583	PASS
442	442	50	100	100.0	104443	PASS
443	442	15	24	18.9	19701	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/26/2025	BNA_F	<u>BF141774.D</u>
Compound Name	Response	Retention Time
DDT	345364	13.457
DDD	14023	13.163
DDE	1091	12.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15114	360478	4.19

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141774.D
Acq On : 26 Feb 2025 10:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 26 11:20:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

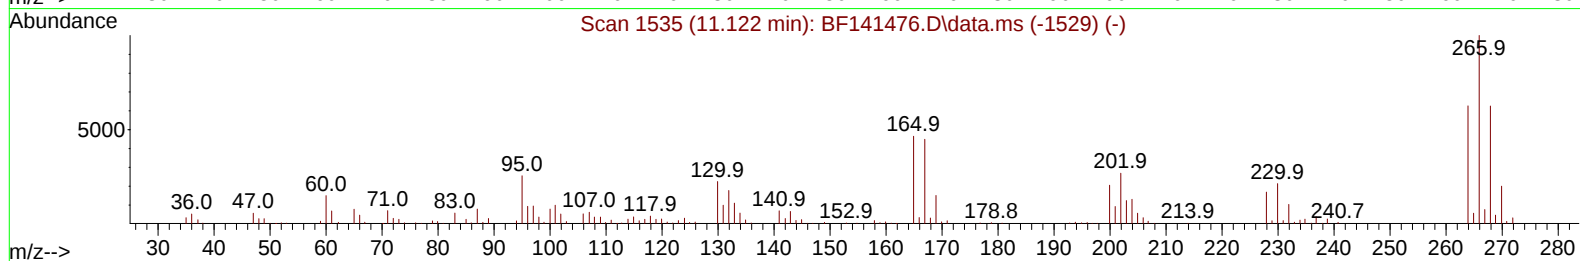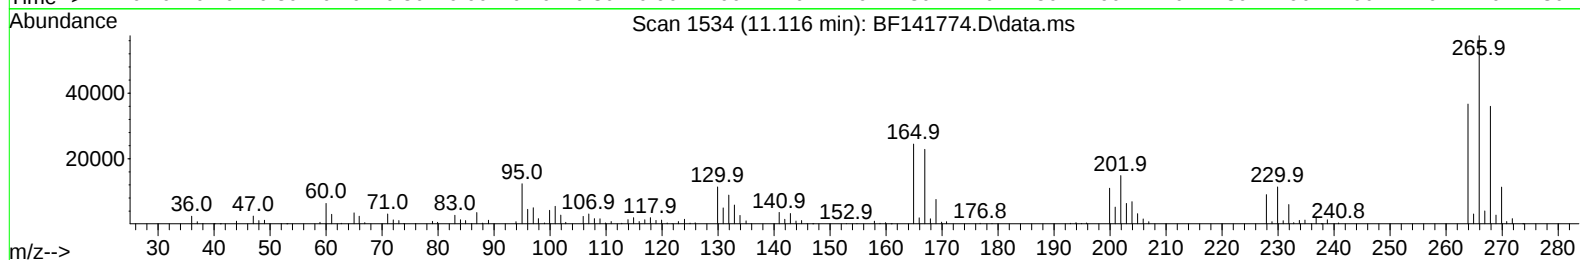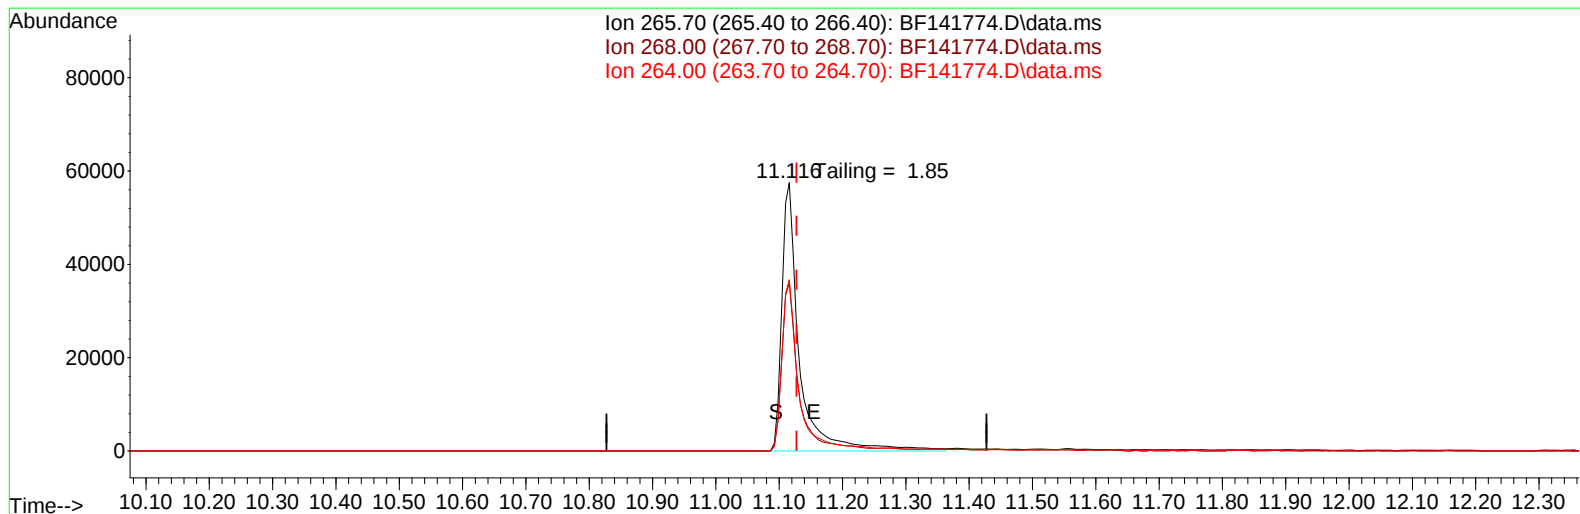

TIC: BF141774.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.012) 20690.83 ng




response 111911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.57
264.00	62.60	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022625\
Data File : BF141774.D
Acq On : 26 Feb 2025 10:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 26 11:20:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

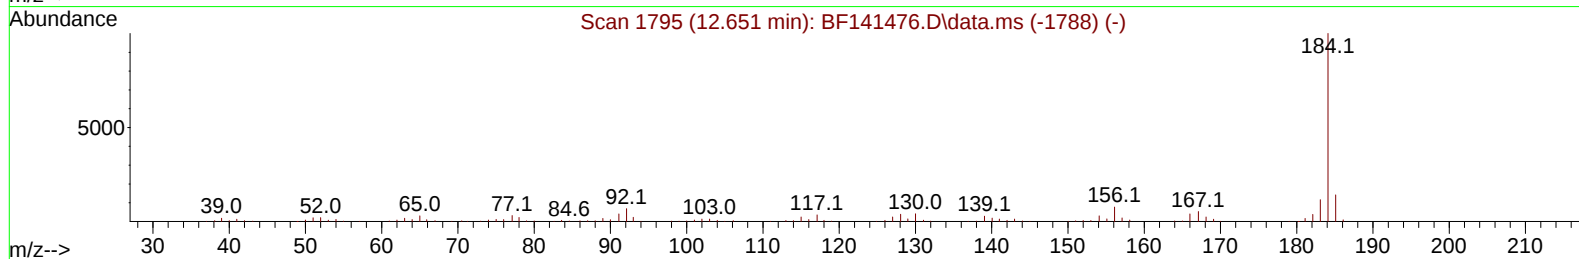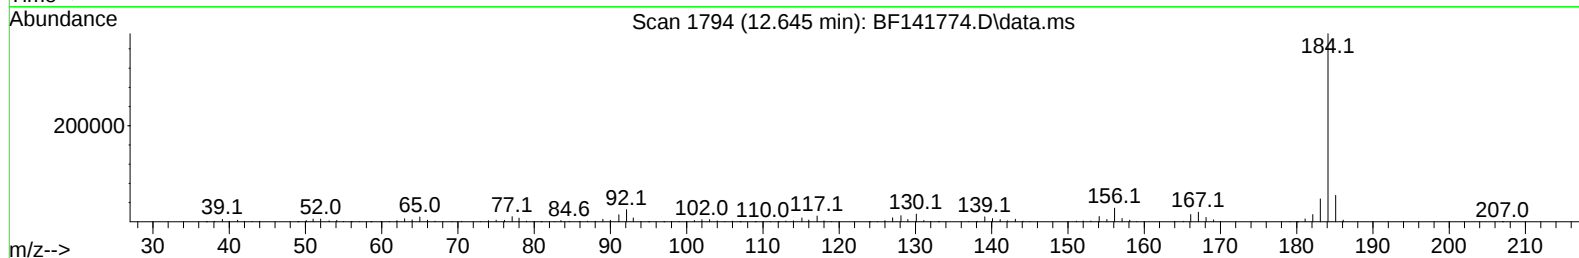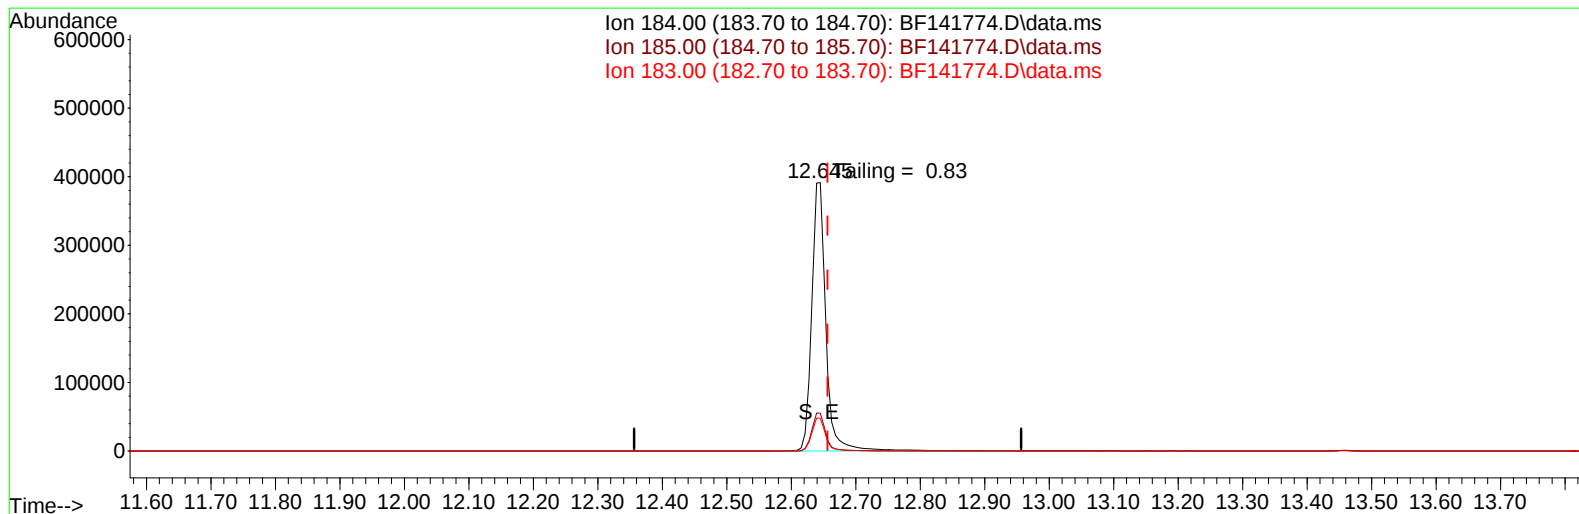

TIC: BF141774.D\data.ms

(77) Benzidine

12.645min (-0.012) 57427.54 ng

response 596534

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.12
183.00	11.60	12.25
0.00	0.00	0.00