


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022625\
Data File : BN036507.D
Acq On : 26 Feb 2025 13:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 11 01:17:14 2025

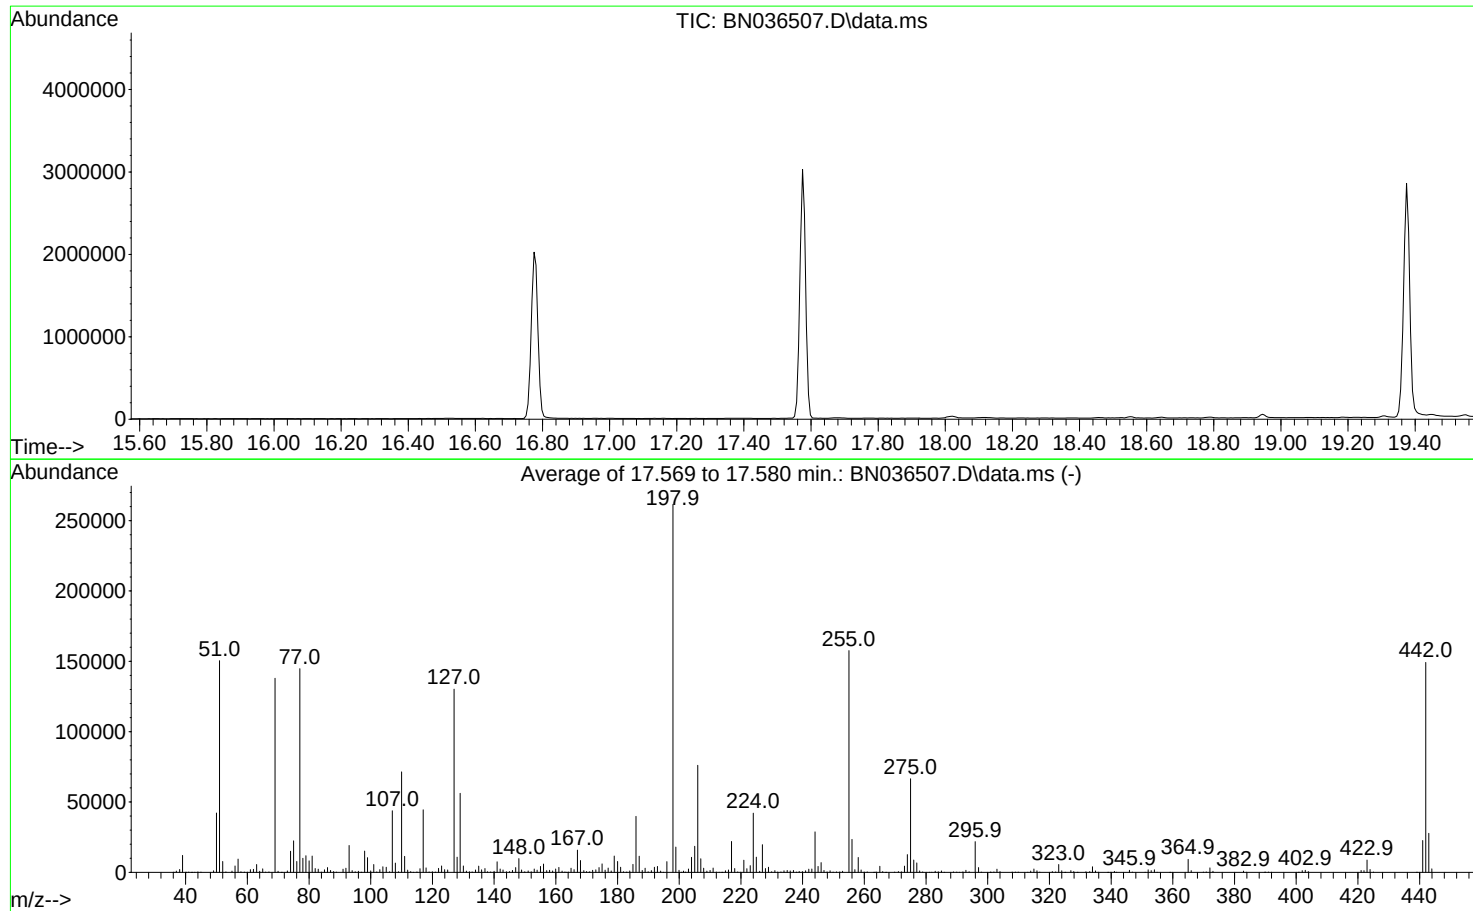

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	150493	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.7	137916	PASS
70	69	0.00	2	0.6	786	PASS
127	198	10	80	49.8	130195	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	261483	PASS
199	198	5	9	6.9	17983	PASS
275	198	10	60	25.4	66488	PASS
365	198	1	100	3.5	9279	PASS
441	198	0.01	100	8.7	22672	PASS
442	442	50	100	100.0	149224	PASS
443	442	15	24	18.6	27735	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/26/2025	BNA_N	<u>BN036507.D</u>
Compound Name	Response	Retention Time
DDT	887081	20.616
DDD	9813	20.227
DDE	276	19.663
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10089	897170	1.12

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022625\
Data File : BN036507.D
Acq On : 26 Feb 2025 13:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 14:31:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

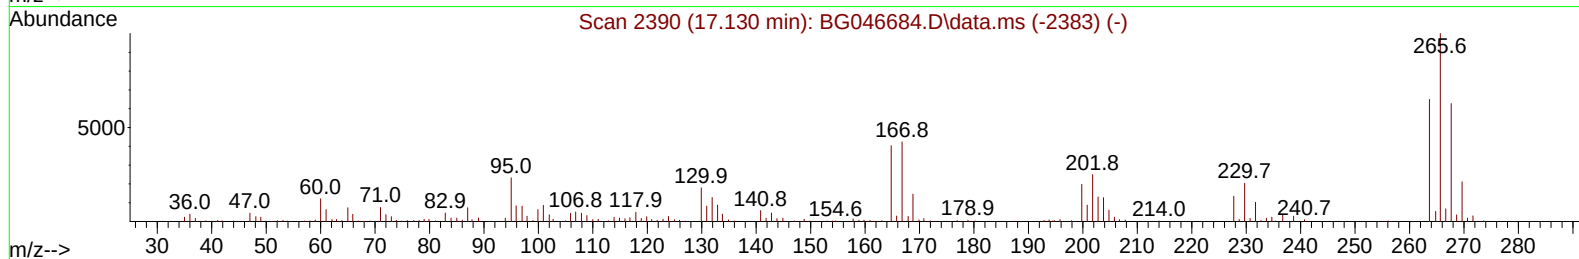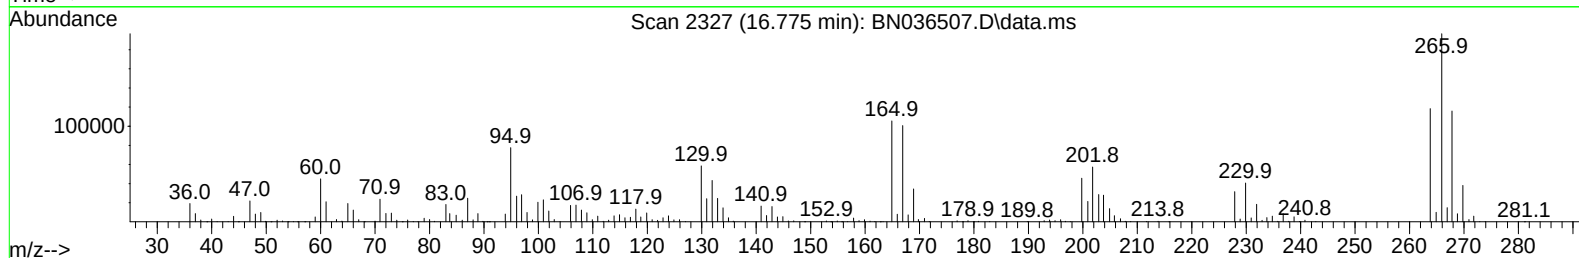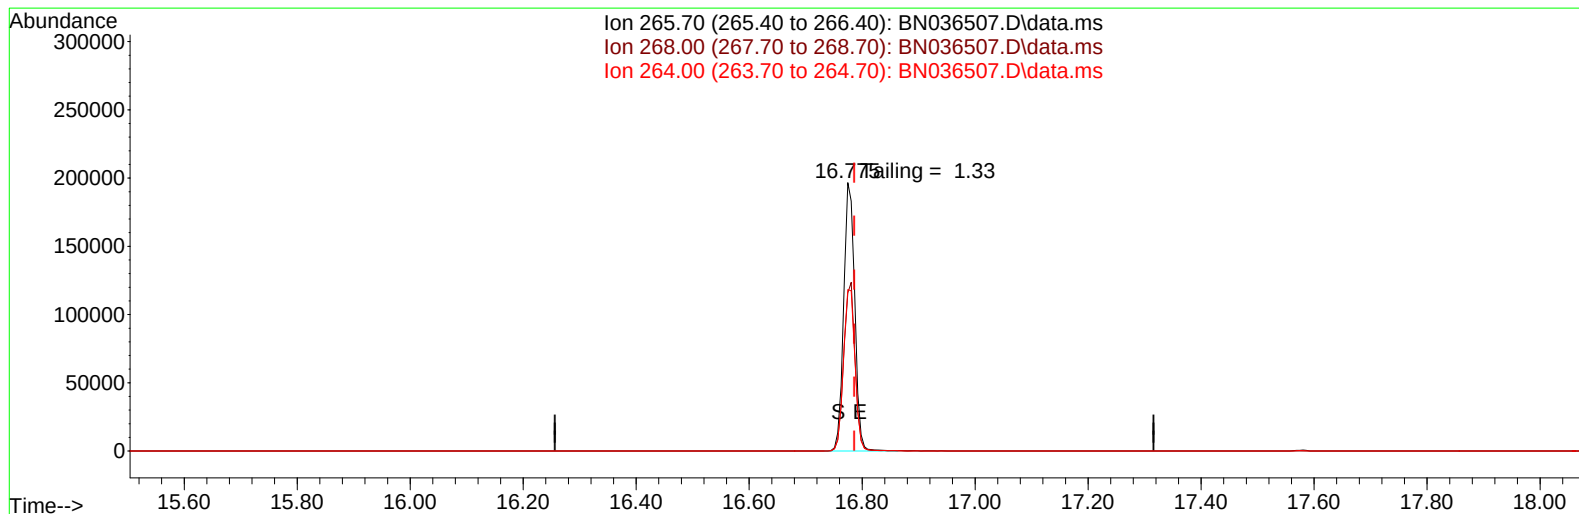

TIC: BN036507.D\data.ms

(70) Pentachlorophenol (C)

16.775min (-0.011) 18096.47 ng




response 266565

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.93
264.00	61.60	60.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022625\
Data File : BN036507.D
Acq On : 26 Feb 2025 13:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 14:31:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

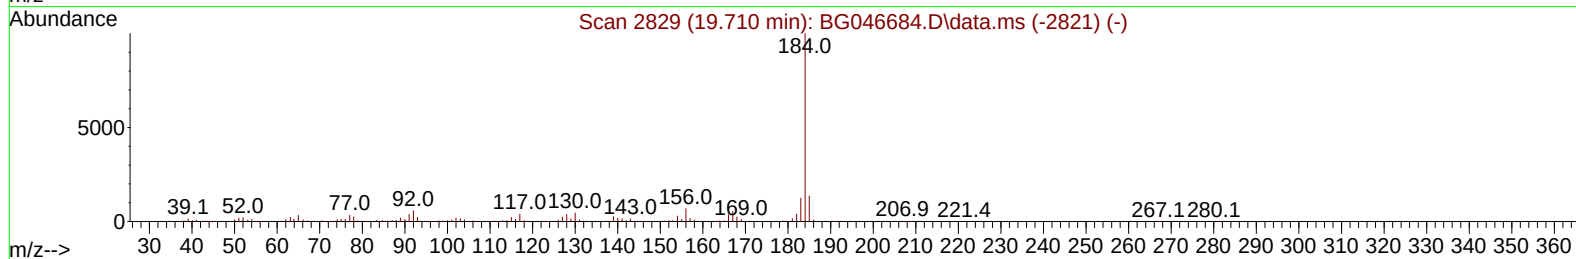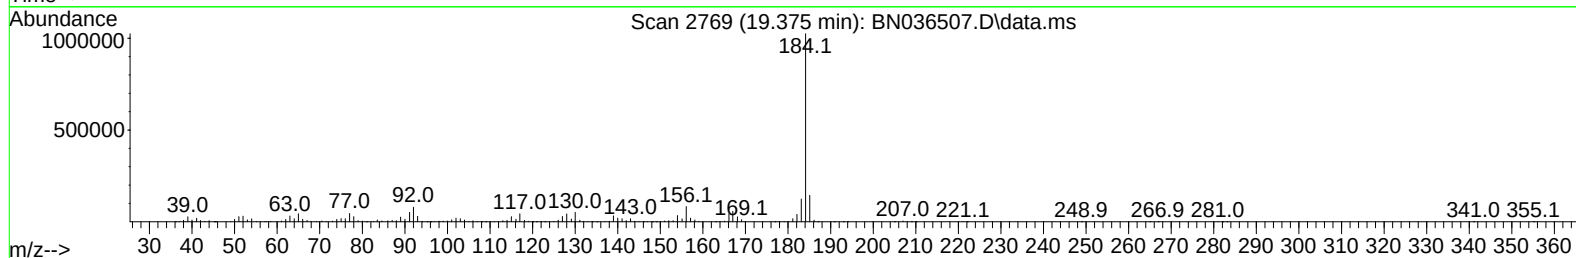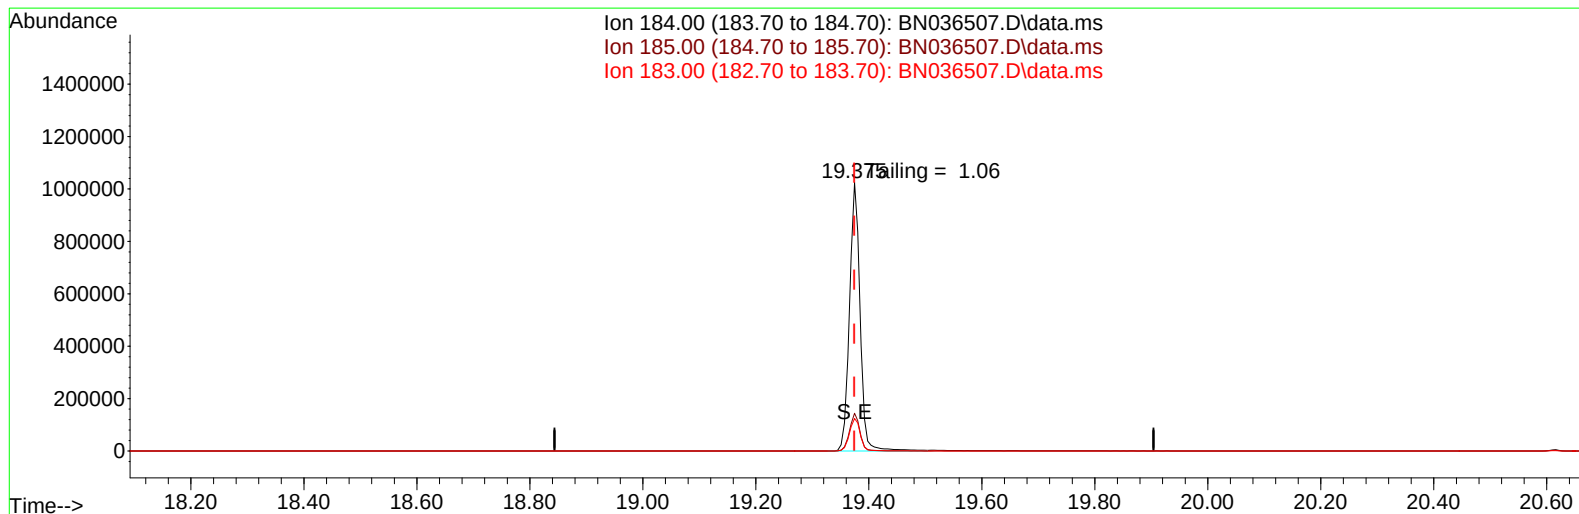

TIC: BN036507.D\data.ms

(77) Benzidine

19.375min (+ 0.000) 0.00 ng

response 1337406

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	12.12
0.00	0.00	0.00