

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045084.D
 Acq On : 28 Feb 2025 13:23
 Operator : JC/MD
 Sample : Q1423-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-192-TB-20250220

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Title : SW846 8260

Signal : TIC: VX045084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	19	rVB	16474	16891	3.56%	0.671%
2	1.240	21	25	28	rBV	9087	12266	2.58%	0.487%
3	1.368	41	46	53	rBV3	5988	8576	1.81%	0.341%
4	1.447	56	59	65	rBV	7229	9155	1.93%	0.364%
5	1.581	72	81	82	rBV3	4585	10956	2.31%	0.435%
6	2.380	206	212	219	rBV	6444	11107	2.34%	0.441%
7	5.379	693	704	720	rBV2	54568	162678	34.24%	6.460%
8	5.550	720	732	746	rBV	74114	213893	45.02%	8.494%
9	5.952	789	798	812	rBV	62612	165710	34.88%	6.580%
10	6.757	921	930	946	rBV	135249	331907	69.87%	13.180%
11	8.647	1233	1240	1258	rBV	293552	475057	100.00%	18.865%
12	9.531	1381	1385	1391	rBV4	2904	4778	1.01%	0.190%
13	10.049	1465	1470	1485	rBV	289509	410216	86.35%	16.290%
14	10.774	1585	1589	1596	rBV2	3764	6396	1.35%	0.254%
15	10.860	1599	1603	1613	rVB3	4598	7218	1.52%	0.287%
16	11.079	1634	1639	1653	rBV	232094	291703	61.40%	11.584%
17	11.482	1700	1705	1715	rVB3	4139	7519	1.58%	0.299%
18	11.841	1760	1764	1771	rBV2	3726	6181	1.30%	0.245%
19	11.933	1775	1779	1785	rVV3	4360	6977	1.47%	0.277%
20	12.018	1788	1793	1807	rBV	274115	345880	72.81%	13.735%
21	12.768	1912	1916	1925	rBV5	3095	6077	1.28%	0.241%
22	12.859	1927	1931	1936	rVV3	4688	7074	1.49%	0.281%




Sum of corrected areas: 2518215

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045084.D
Acq On : 28 Feb 2025 13:23
Operator : JC/MD
Sample : Q1423-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

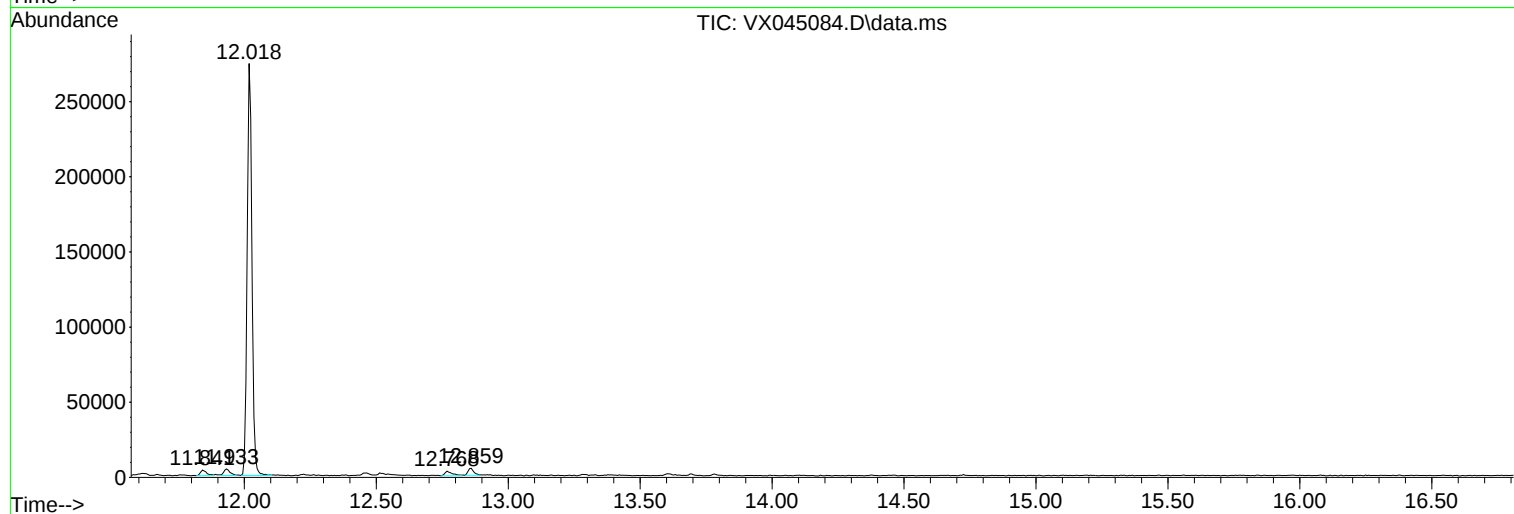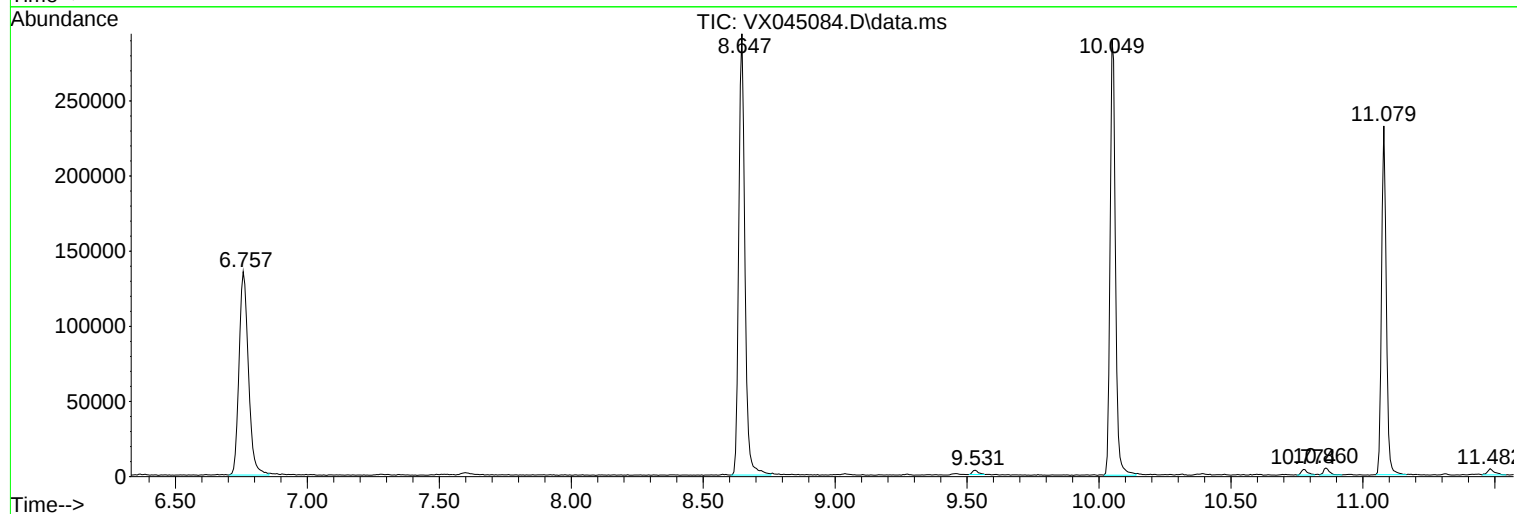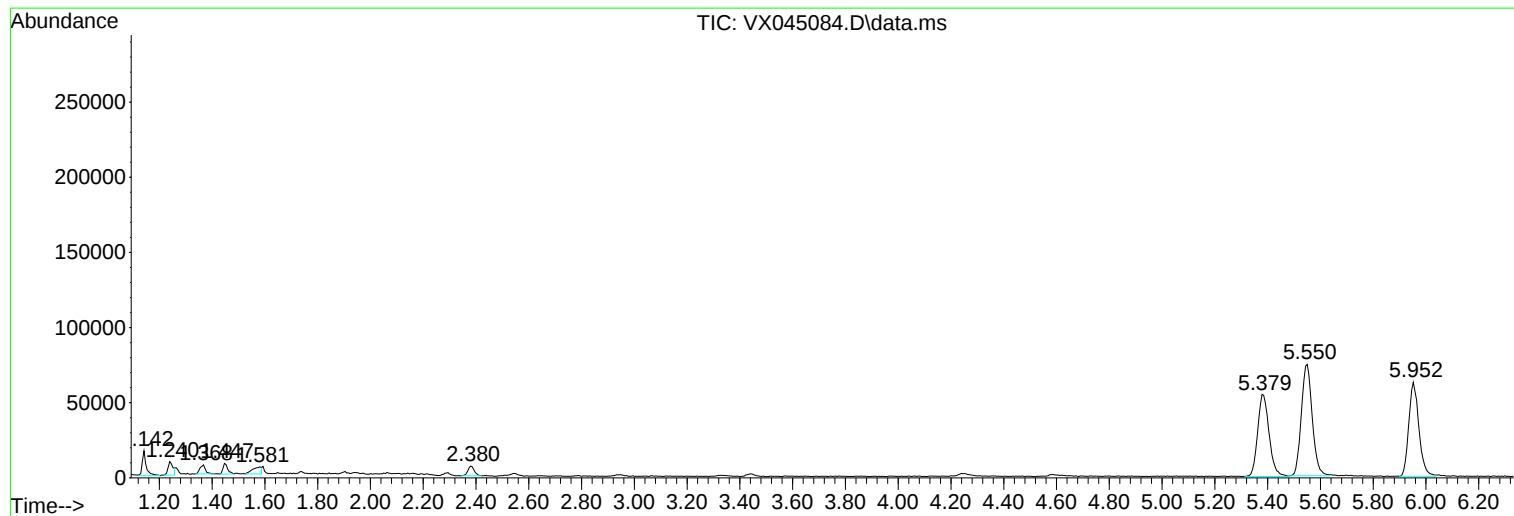

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045084.D
Acq On : 28 Feb 2025 13:23
Operator : JC/MD
Sample : Q1423-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045084.D
Acq On : 28 Feb 2025 13:23
Operator : JC/MD
Sample : Q1423-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc