


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030325\
Data File : BF141810.D
Acq On : 03 Mar 2025 13:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 28 01:48:16 2025

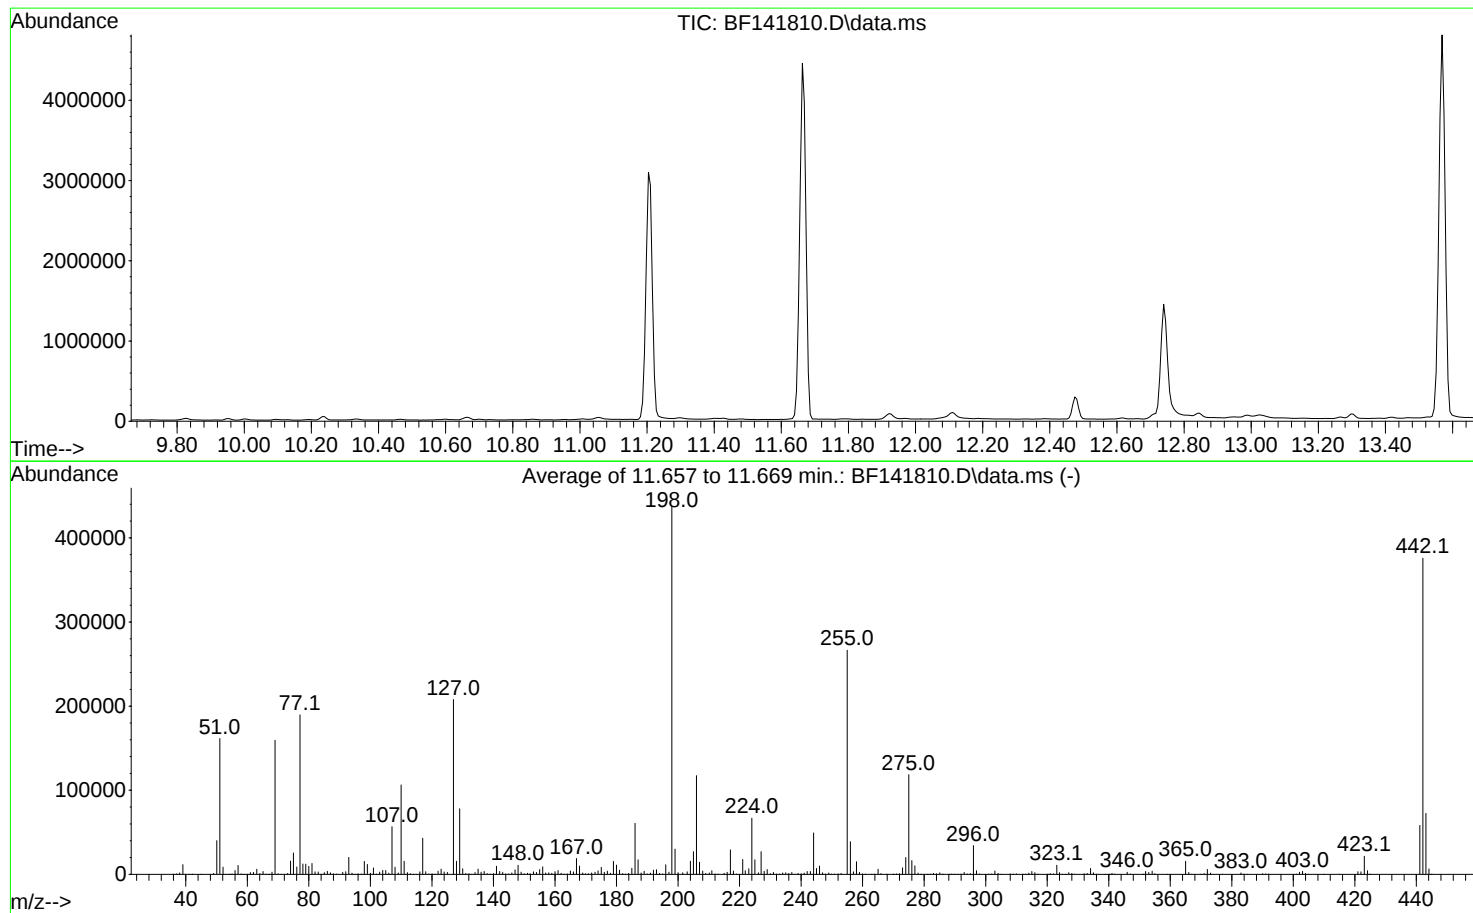




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	161527	PASS
68	69	0.00	2	1.7	2647	PASS
69	198	0.00	100	36.4	159355	PASS
70	69	0.00	2	0.4	717	PASS
127	198	10	80	47.5	207936	PASS
197	198	0.00	2	0.6	2683	PASS
198	198	100	100	100.0	437355	PASS
199	198	5	9	6.9	29989	PASS
275	198	10	60	27.1	118512	PASS
365	198	1	100	3.6	15686	PASS
441	198	0.01	100	13.3	58189	PASS
442	442	50	100	100.0	375872	PASS
443	442	15	24	19.3	72480	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030325\
Data File : BF141810.D
Acq On : 03 Mar 2025 13:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 03 15:43:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

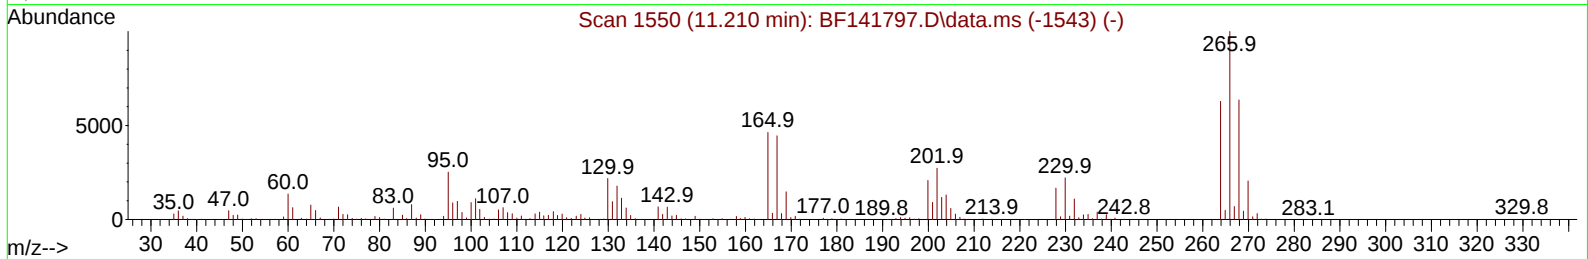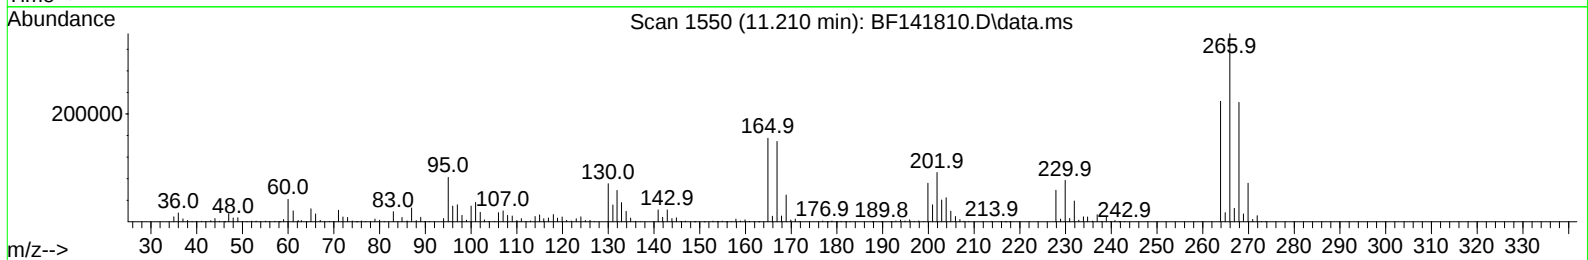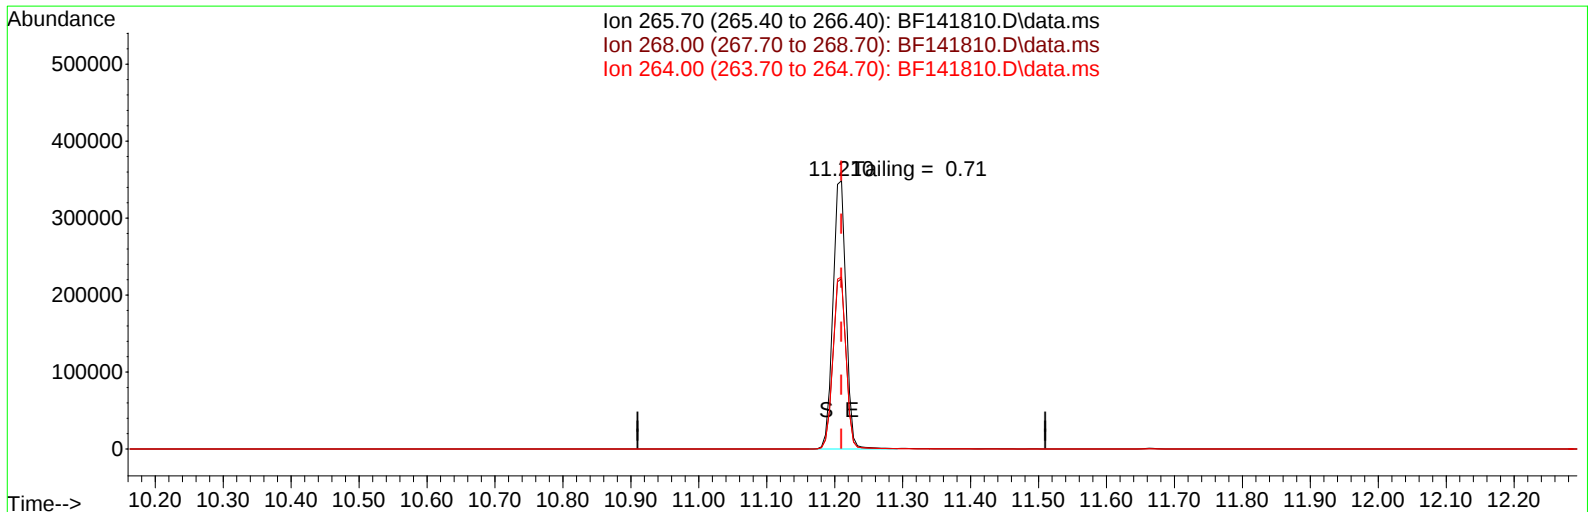

TIC: BF141810.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 14361.45 ng




response 467023

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.48
264.00	62.80	64.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030325\
Data File : BF141810.D
Acq On : 03 Mar 2025 13:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 03 15:43:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

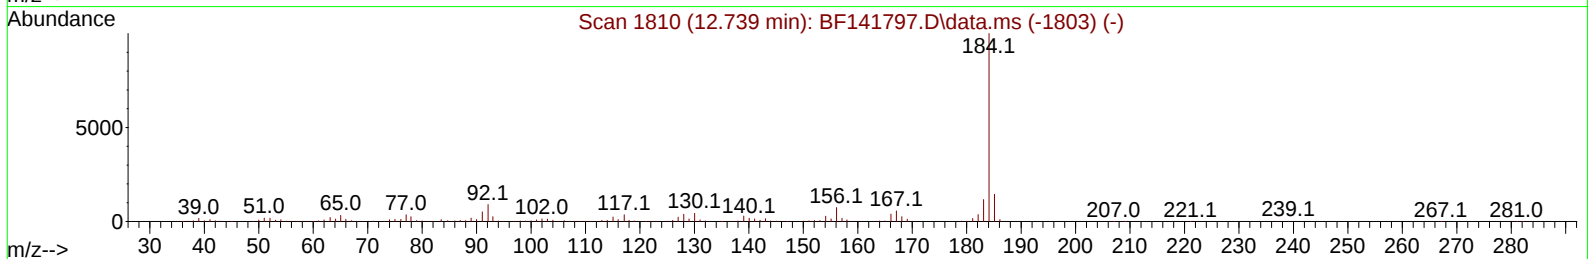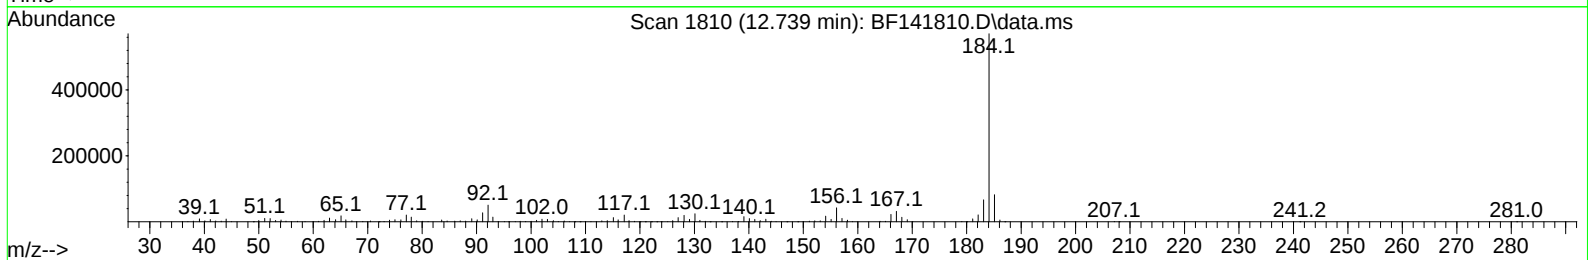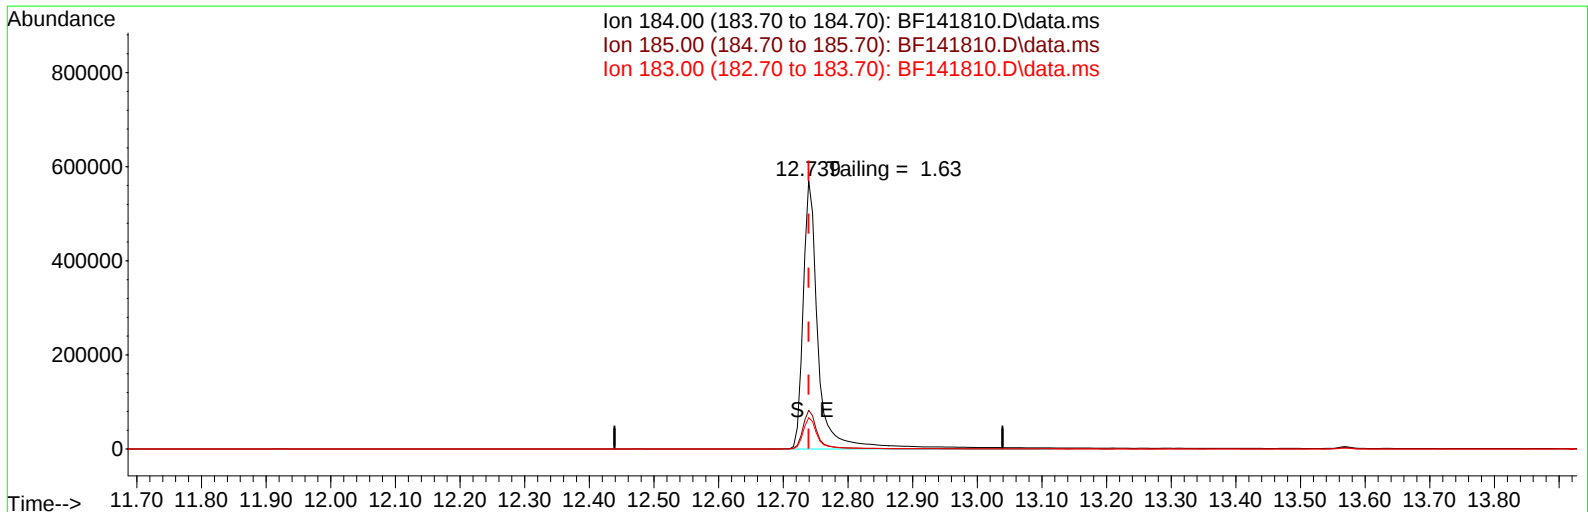

TIC: BF141810.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 25512.33 ng

response 914517

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.46
183.00	11.70	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/3/2025	BNA_F	<u>BF141810.D</u>
Compound Name	Response	Retention Time
DDT	1099767	13.569
DDD	14757	13.298
DDE	11303	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26060	1125827	2.31

Instrument :
BNA_F
ClientSampleId :
DFTPP