

SOP ID:	M625.1-BNA-20		
Clean Up SOP #:	N/A	Extraction Start Date :	02/28/2025
Matrix :	Water	Extraction Start Time :	08:40
Weight By:	N/A	Extraction By:	RS
Balance check:	N/A	Filter By:	RS
Balance ID:	N/A	pH Meter ID:	N/A
pH Strip Lot#:	E3574	Hood ID:	4,6,7
Extraction Method:	☒ Separatory Funnel	☐ Continuous Liquid/Liquid	☐ Sonication
		☐ Waste Dilution	☐ Soxhlet
		Extraction End Date :	02/28/2025
		Extraction End Time :	13:30
		Concentration By:	EH
		Supervisor By :	RUPESH

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	50/100 PPM	SP6720
Surrogate	1.0ML	100 PPM	SP6640
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3874
Baked Na2SO4	N/A	EP2581
10N NaoH	N/A	EP2559
H2SO4 1:1	N/A	EP2565
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

1.5 ML Vial lot# 2210673. pH Adjusted<2 with 1:1 H2SO4 & >11 with10N NaOH.


KD Bath ID:	Water bath -01	Envap ID:	NEVAP-02
KD Bath Temperature:	60 °C	Envap Temperature:	40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
2/28/25	RS (E44 lab)	RC/svac
13:35	Preparation Group	Analysis Group

Analytical Method: M625.1-BNA-20

Concentration Date: 02/28/2025

Sample ID	Client Sample ID	Test	g / ml	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB166933BL	SBLK933	SVOCMS Group1	1000	6	RUPESH	ritesh	1			SEP-1
PB166933BS	SLCS933	SVOCMS Group1	1000	6	RUPESH	ritesh	1			2
PB166933BS D	SLCSD933	SVOCMS Group1	1000	6	RUPESH	ritesh	1			3
Q1456-02	EFF-WASTE WATER	SVOCMS Group1	870	6	RUPESH	ritesh	1	C		4

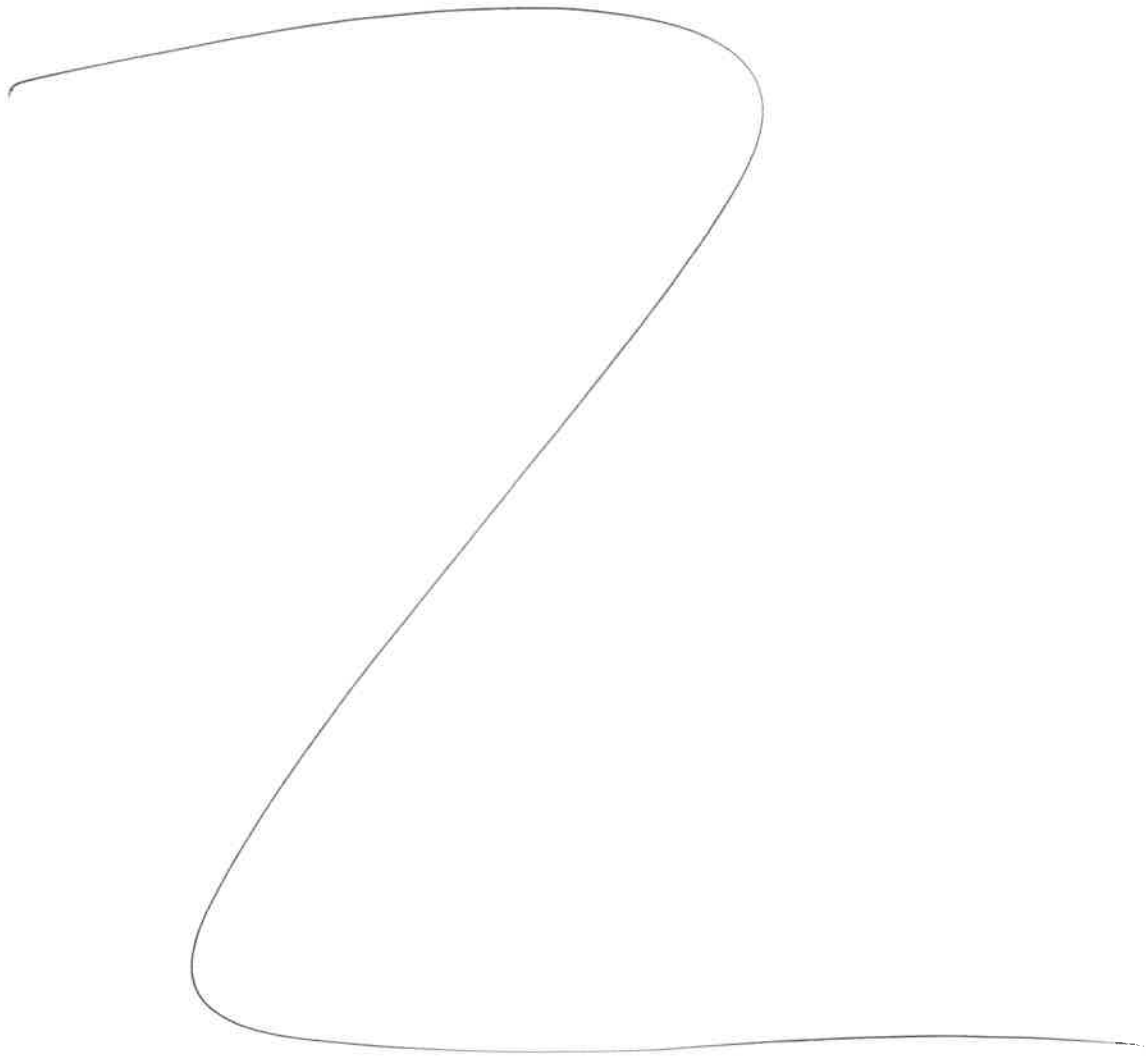

Rs
2/28