
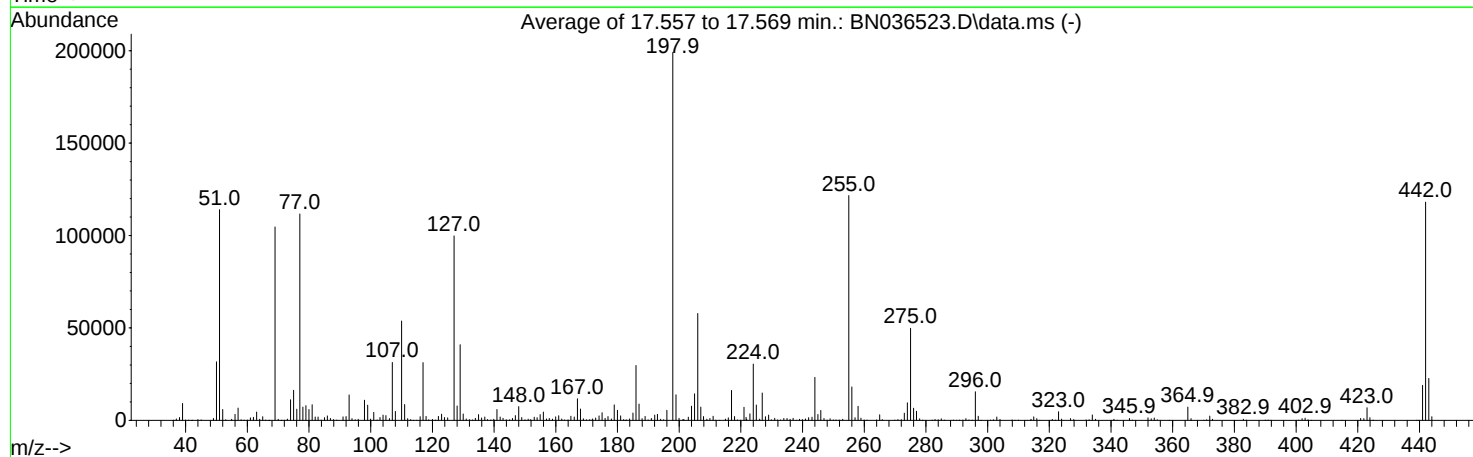


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030525\
Data File : BN036523.D
Acq On : 05 Mar 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 16:08:57 2025

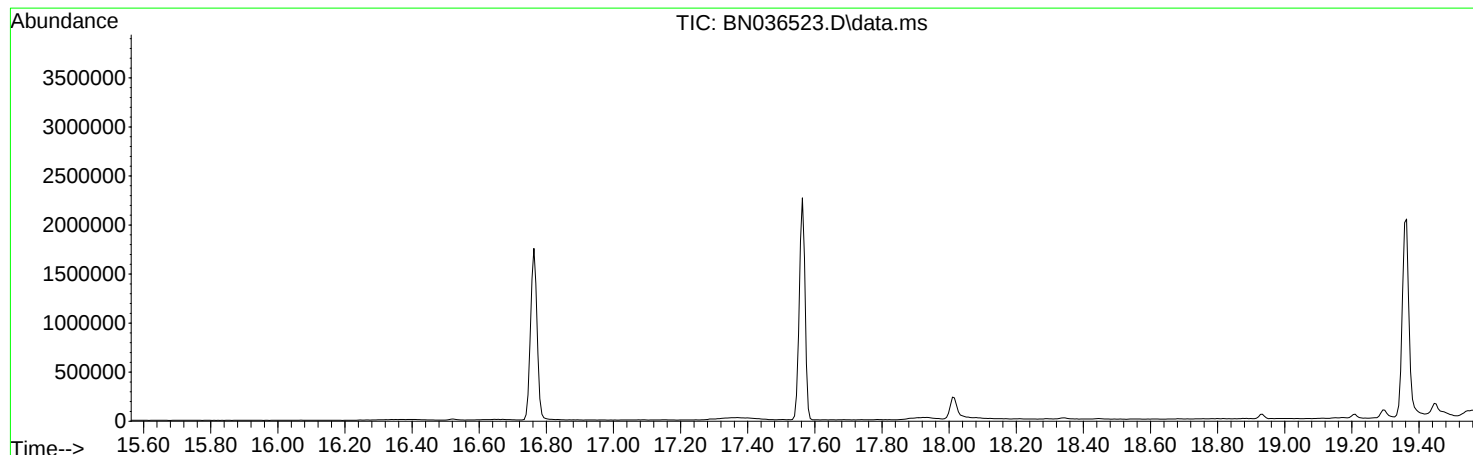

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.3	113984	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.6	104689	PASS
70	69	0.00	2	0.6	639	PASS
127	198	10	80	50.2	99840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	199040	PASS
199	198	5	9	7.0	13866	PASS
275	198	10	60	25.0	49821	PASS
365	198	1	100	3.6	7186	PASS
441	198	0.01	100	9.5	18995	PASS
442	442	50	100	100.0	118091	PASS
443	442	15	24	19.2	22664	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/5/2025	BNA_N	<u>BN036523.D</u>
Compound Name	Response	Retention Time
DDT	725032	20.598
DDD	9634	20.21
DDE	159	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9793	734825	1.33

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030525\
Data File : BN036523.D
Acq On : 05 Mar 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 05 16:03:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

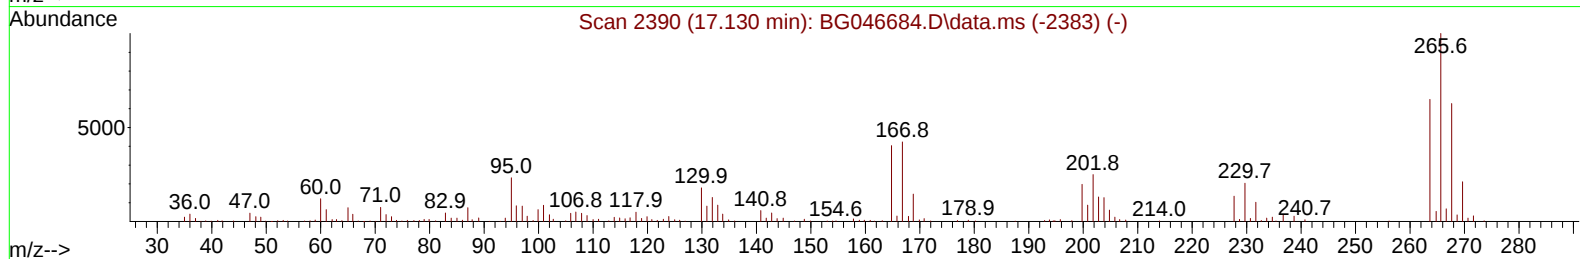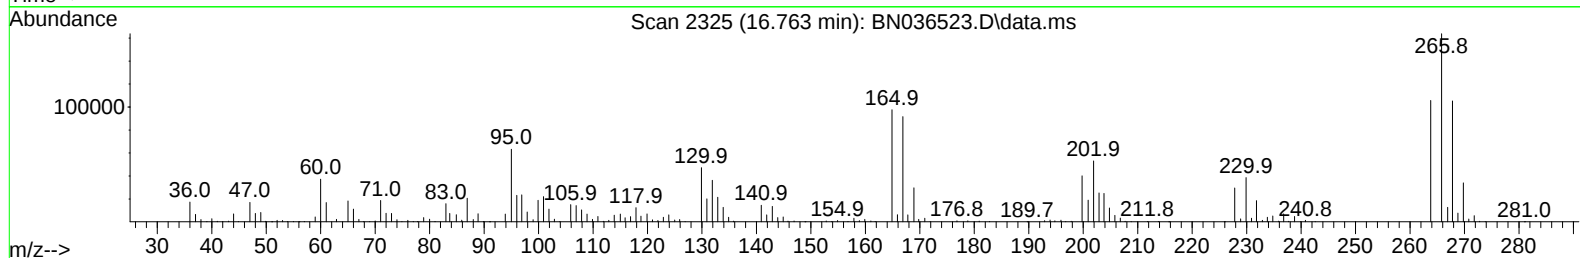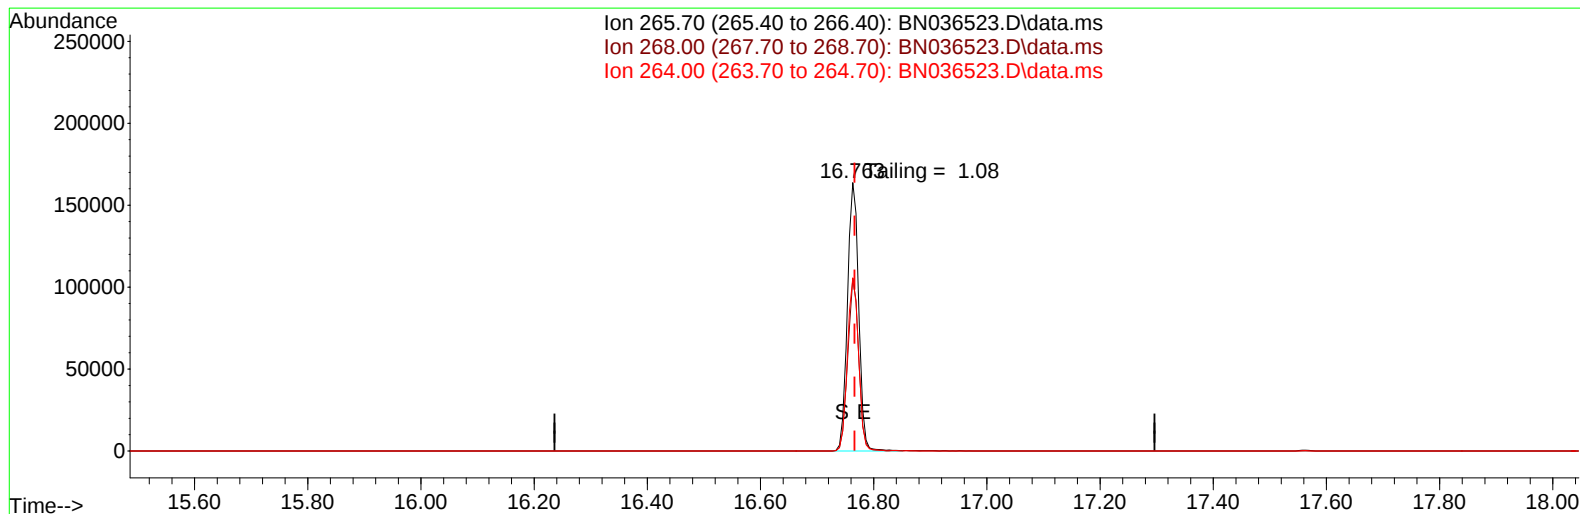

TIC: BN036523.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.003) 22410.75 ng




response 227405

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.26
264.00	61.60	64.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030525\
Data File : BN036523.D
Acq On : 05 Mar 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 05 16:03:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

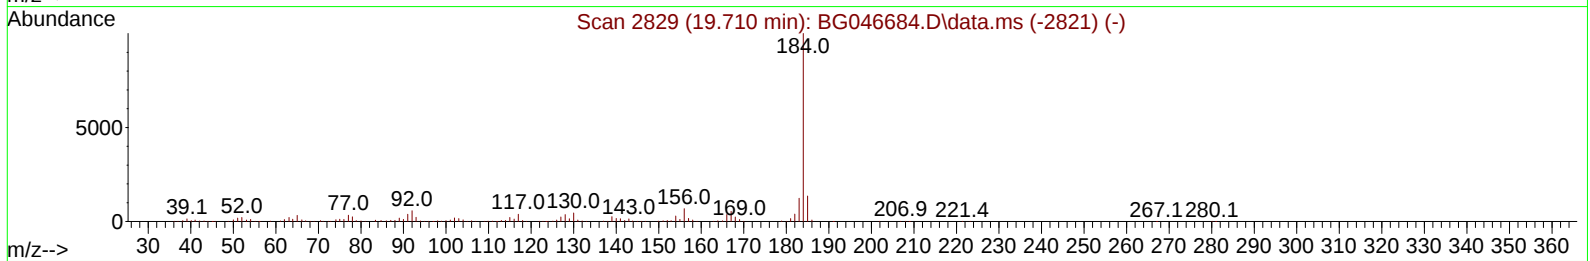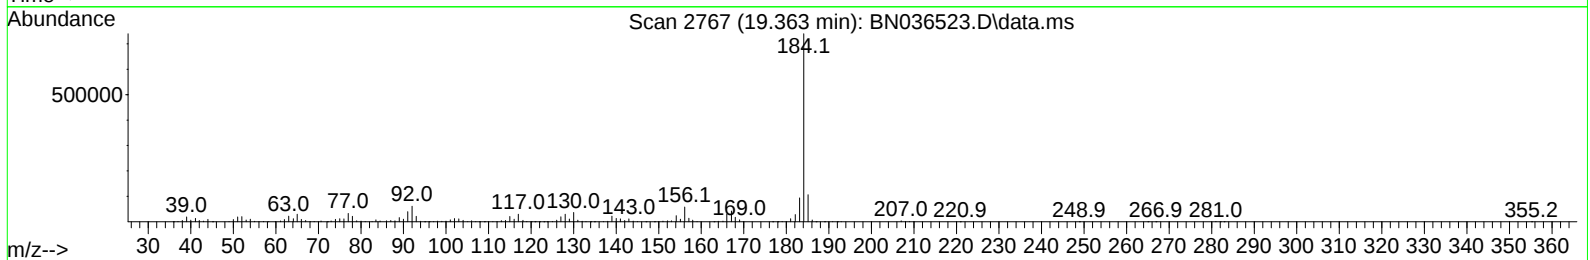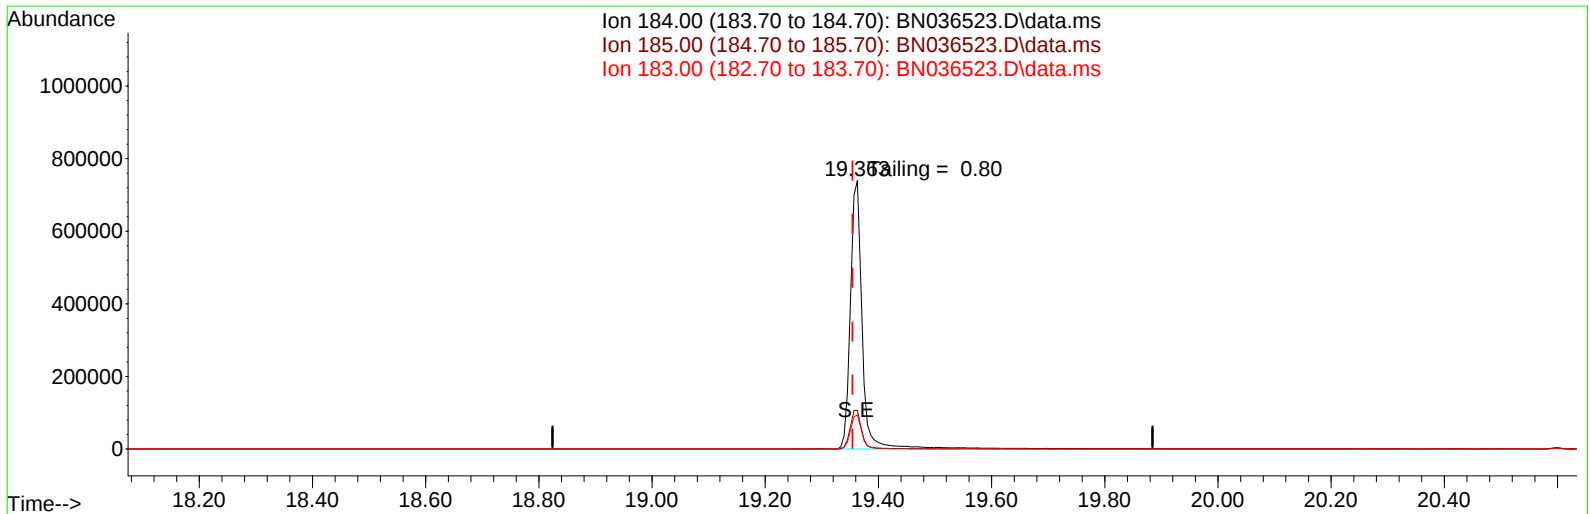

TIC: BN036523.D\data.ms

(77) Benzidine

19.363min (+ 0.009) 0.00 ng

response 1065965

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.43
183.00	13.20	12.74
0.00	0.00	0.00