

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030625\
 Data File : BF141861.D
 Acq On : 06 Mar 2025 11:21
 Operator : RC/JU
 Sample : PB166982BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166982BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.246	16	26	32	rVB	55435	102945	1.11%	0.208%
2	5.510	574	581	586	rBV	4362587	6158250	66.30%	12.413%
3	6.504	743	750	755	rBV	4124259	6130832	66.00%	12.358%
4	6.887	809	815	820	rBV	1012818	1272257	13.70%	2.565%
5	7.445	903	910	915	rBV	2856844	4193404	45.14%	8.453%
6	8.163	1026	1032	1037	rBV	1313313	1694537	18.24%	3.416%
7	9.239	1208	1215	1220	rBV	5935221	8109581	87.30%	16.347%
8	9.916	1324	1330	1343	rBV	1547614	1993087	21.46%	4.018%
9	10.704	1457	1464	1469	rBV	4189751	5504064	59.25%	11.095%
10	11.404	1577	1583	1588	rBV	1582941	2040421	21.97%	4.113%
11	12.992	1846	1853	1858	rBV	6829406	9289114	100.00%	18.724%
12	14.039	2025	2031	2036	rBV	1339299	1749387	18.83%	3.526%
13	15.510	2274	2281	2297	rBV	850460	1372181	14.77%	2.766%




Sum of corrected areas: 49610060

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030625\
Data File : BF141861.D
Acq On : 06 Mar 2025 11:21
Operator : RC/JU
Sample : PB166982BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166982BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

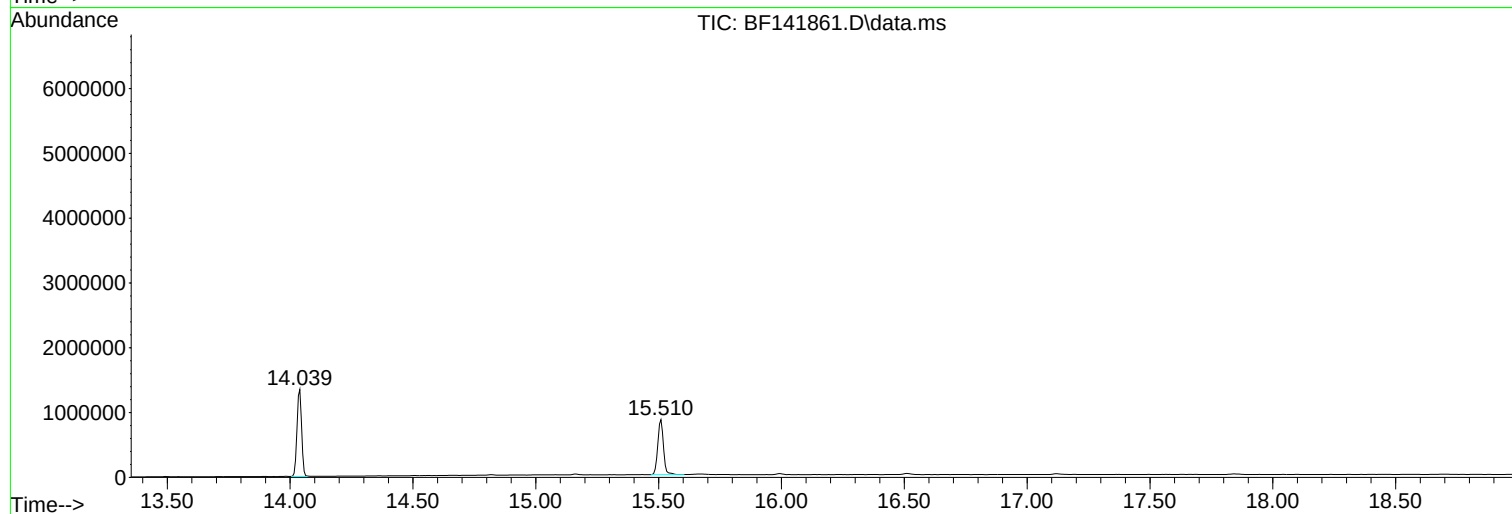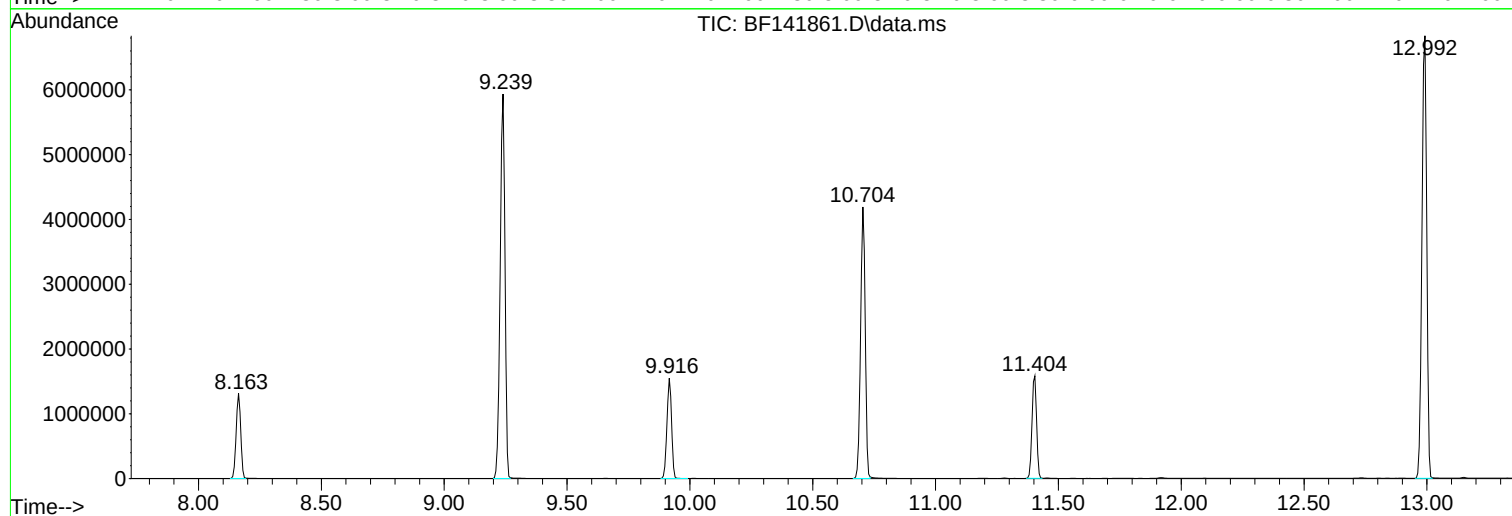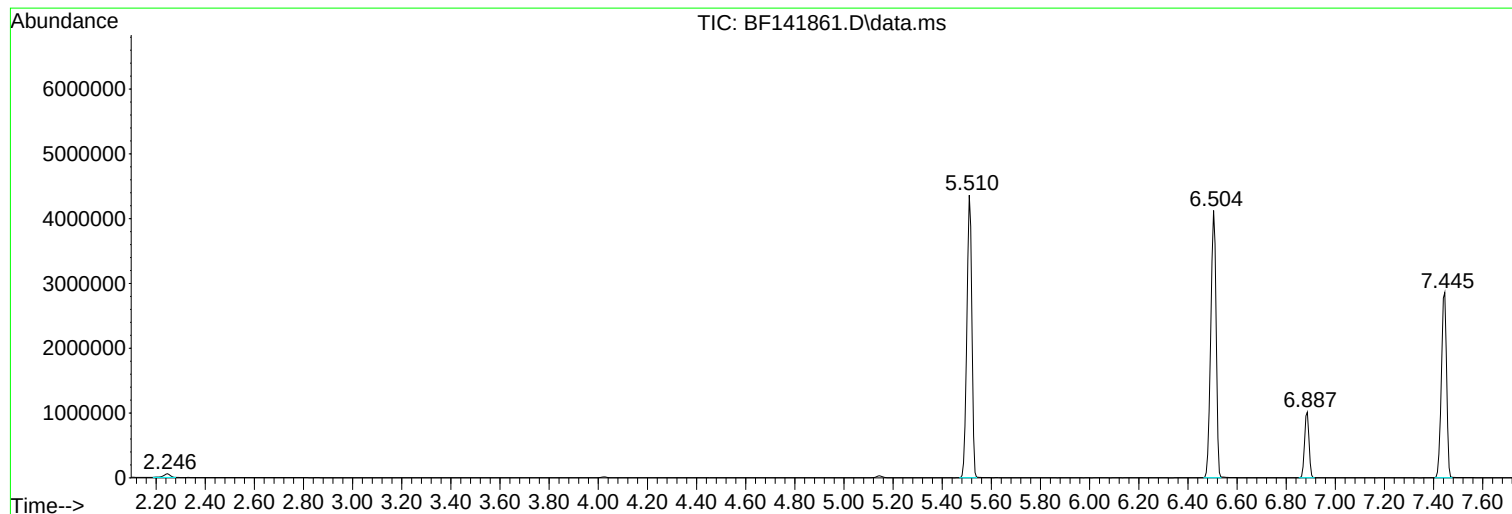

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030625\
Data File : BF141861.D
Acq On : 06 Mar 2025 11:21
Operator : RC/JU
Sample : PB166982BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166982BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030625\
Data File : BF141861.D
Acq On : 06 Mar 2025 11:21
Operator : RC/JU
Sample : PB166982BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166982BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------