
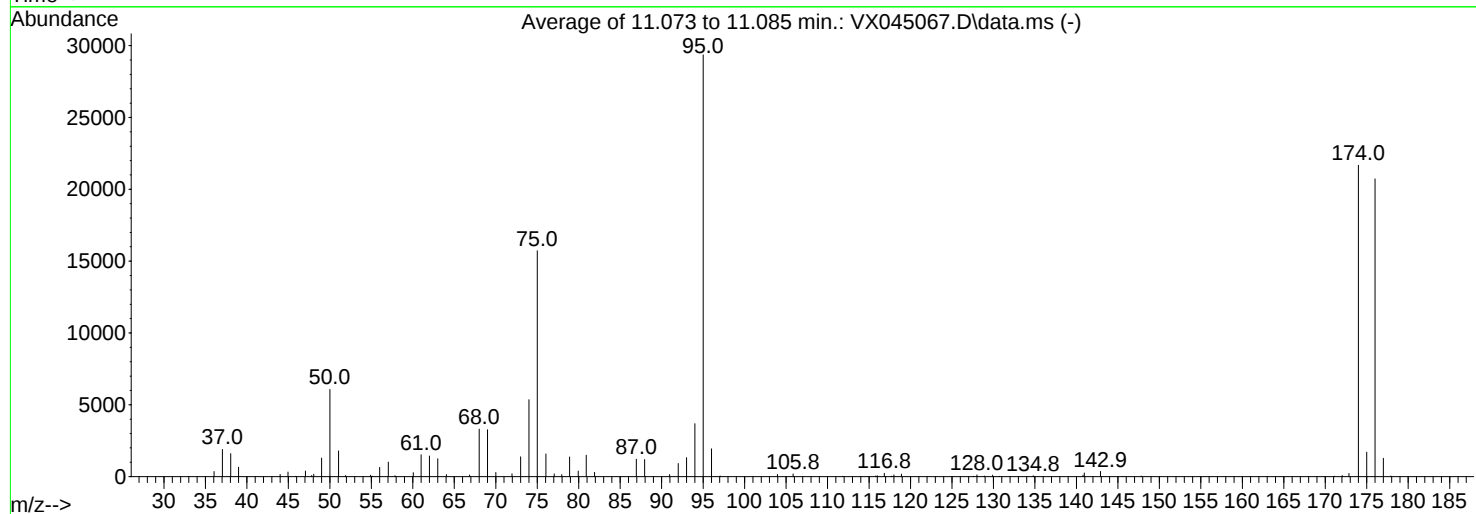


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045067.D
Acq On : 28 Feb 2025 01:03
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Title : SW846 8260
Last Update : Fri Feb 28 06:45:16 2025

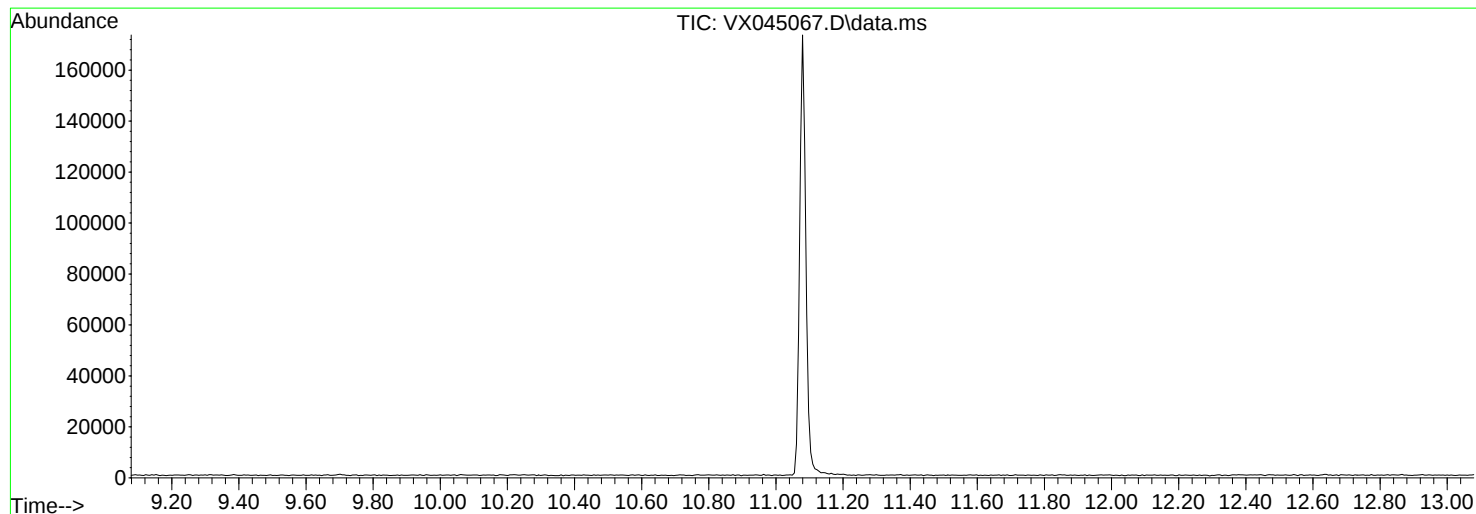

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	6072	PASS
75	95	30	60	53.6	15726	PASS
95	95	100	100	100.0	29360	PASS
96	95	5	9	6.6	1942	PASS
173	174	0.00	2	1.0	219	PASS
174	95	50	100	73.8	21677	PASS
175	174	5	9	7.9	1702	PASS
176	174	95	101	95.6	20723	PASS
177	176	5	9	6.2	1277	PASS