


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030525\
Data File : VX045126.D
Acq On : 05 Mar 2025 08:40
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Title : SW846 8260
Last Update : Fri Feb 28 06:45:16 2025

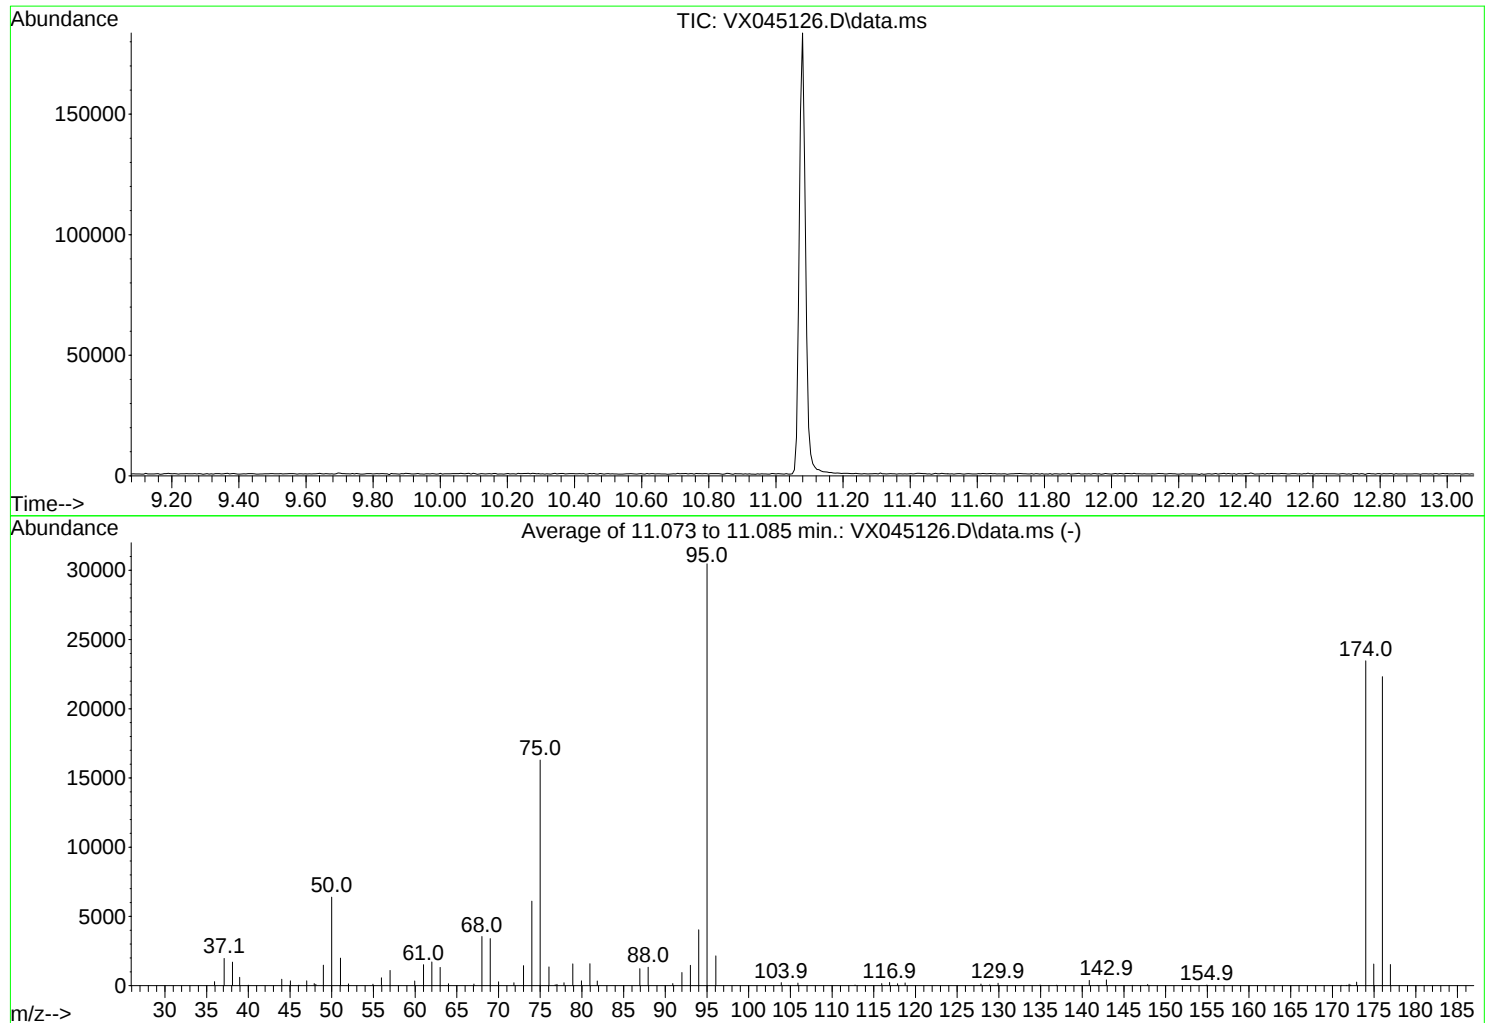

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	6391	PASS
75	95	30	60	53.5	16301	PASS
95	95	100	100	100.0	30469	PASS
96	95	5	9	7.1	2150	PASS
173	174	0.00	2	1.1	256	PASS
174	95	50	100	77.0	23464	PASS
175	174	5	9	6.7	1563	PASS
176	174	95	101	95.1	22320	PASS
177	176	5	9	6.9	1531	PASS