
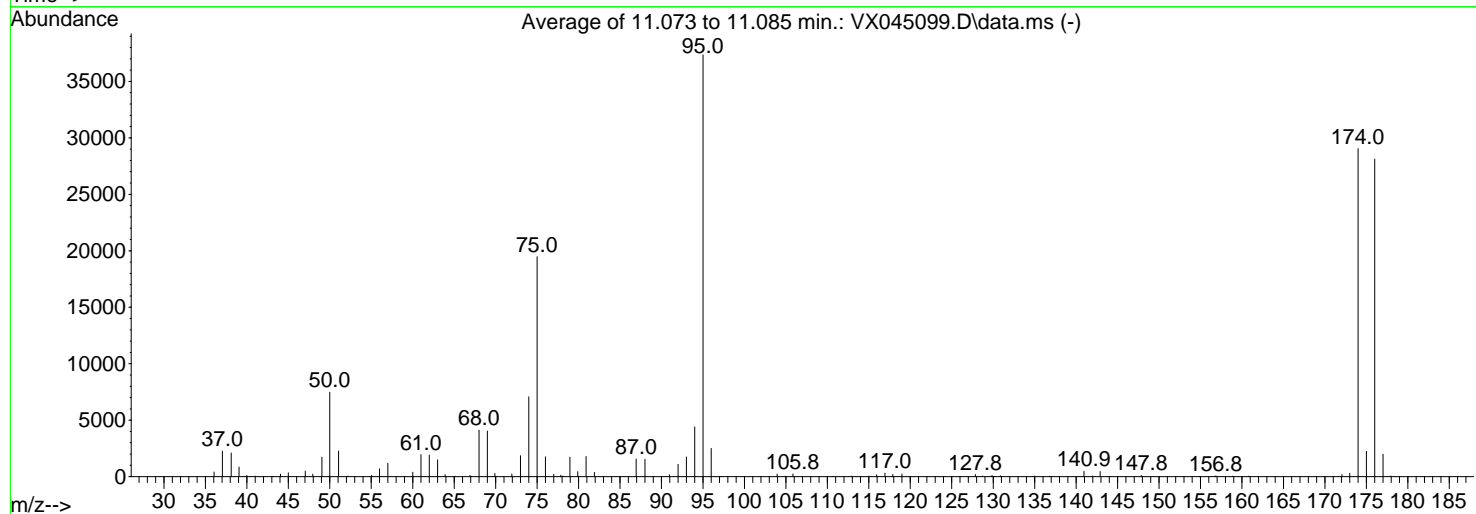


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX030325\  
 Data File : VX045099.D  
 Acq On : 03 Mar 2025 08:18  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022825W.M  
 Title : SW846 8260  
 Last Update : Fri Feb 28 06:45:16 2025

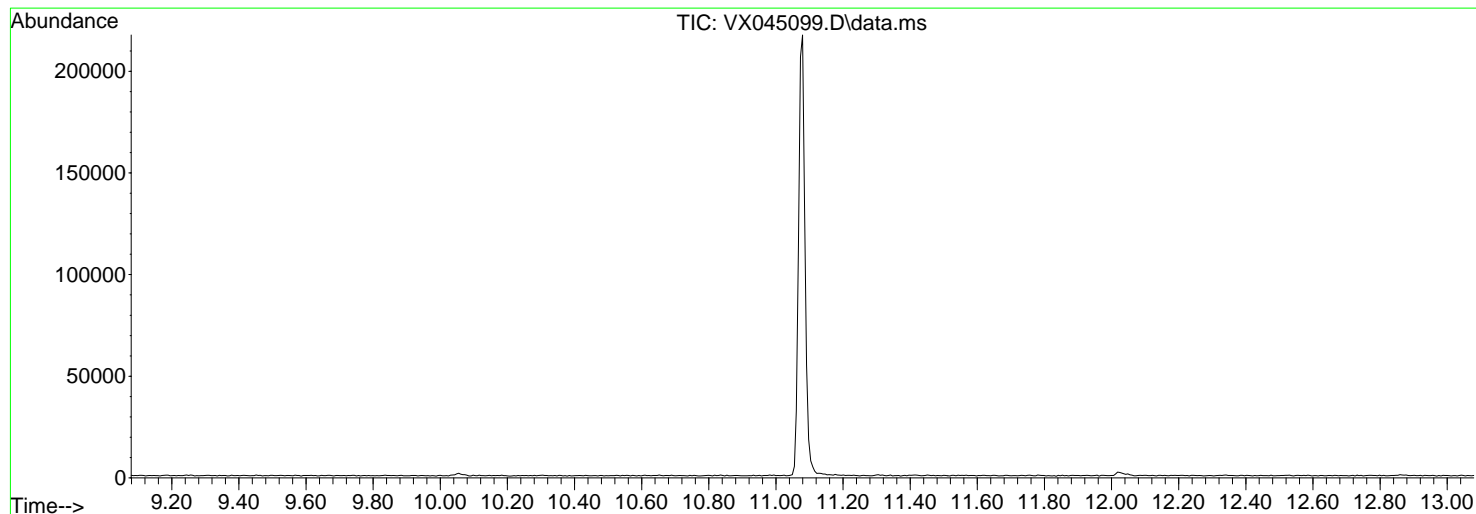

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	7470	PASS
75	95	30	60	52.2	19490	PASS
95	95	100	100	100.0	37352	PASS
96	95	5	9	6.7	2511	PASS
173	174	0.00	2	1.0	299	PASS
174	95	50	100	77.8	29043	PASS
175	174	5	9	7.7	2240	PASS
176	174	95	101	96.8	28125	PASS
177	176	5	9	7.1	1985	PASS