


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030625\
Data File : BF141857.D
Acq On : 06 Mar 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 28 01:48:16 2025

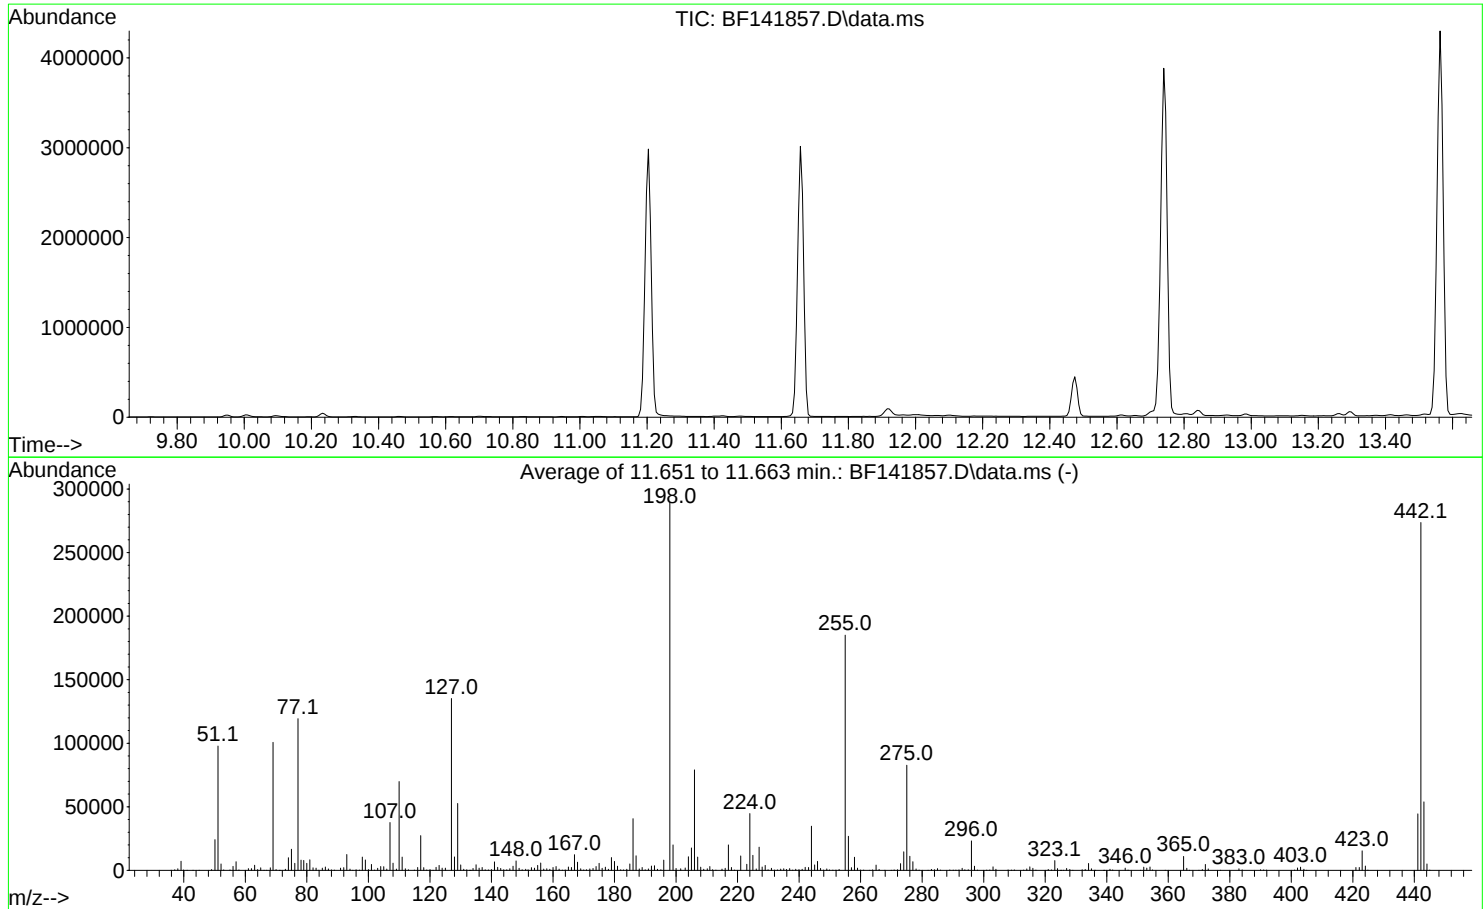

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	97827	PASS
68	69	0.00	2	2.0	1989	PASS
69	198	0.00	100	34.8	100752	PASS
70	69	0.00	2	0.7	703	PASS
127	198	10	80	46.7	135227	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	289387	PASS
199	198	5	9	6.9	20075	PASS
275	198	10	60	28.6	82683	PASS
365	198	1	100	3.8	11013	PASS
441	198	0.01	100	15.3	44419	PASS
442	442	50	100	100.0	273621	PASS
443	442	15	24	19.7	53861	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/6/2025	BNA_F	<u>BF141857.D</u>
Compound Name	Response	Retention Time
DDT	1093424	13.563
DDD	17368	13.292
DDE	1071	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18439	1111863	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030625\
Data File : BF141857.D
Acq On : 06 Mar 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 06 17:12:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

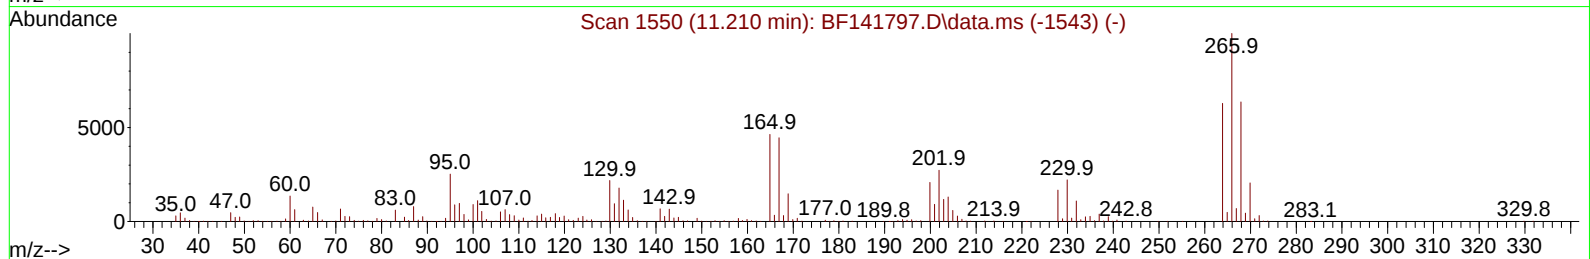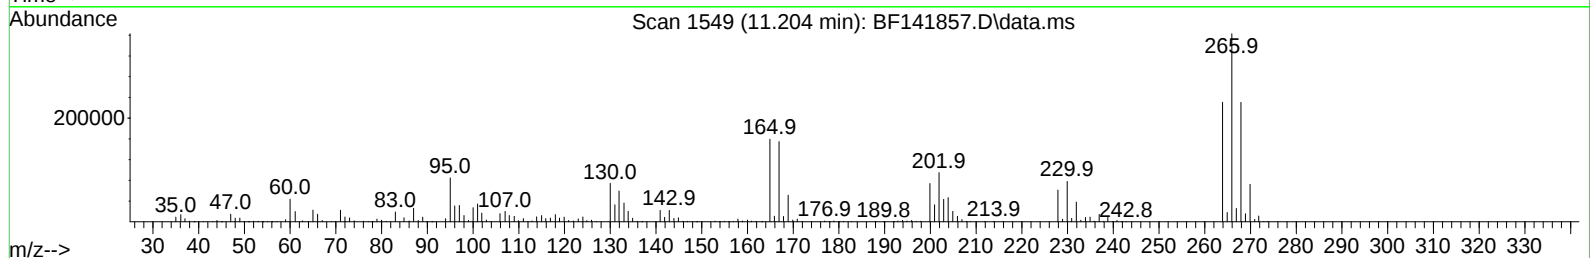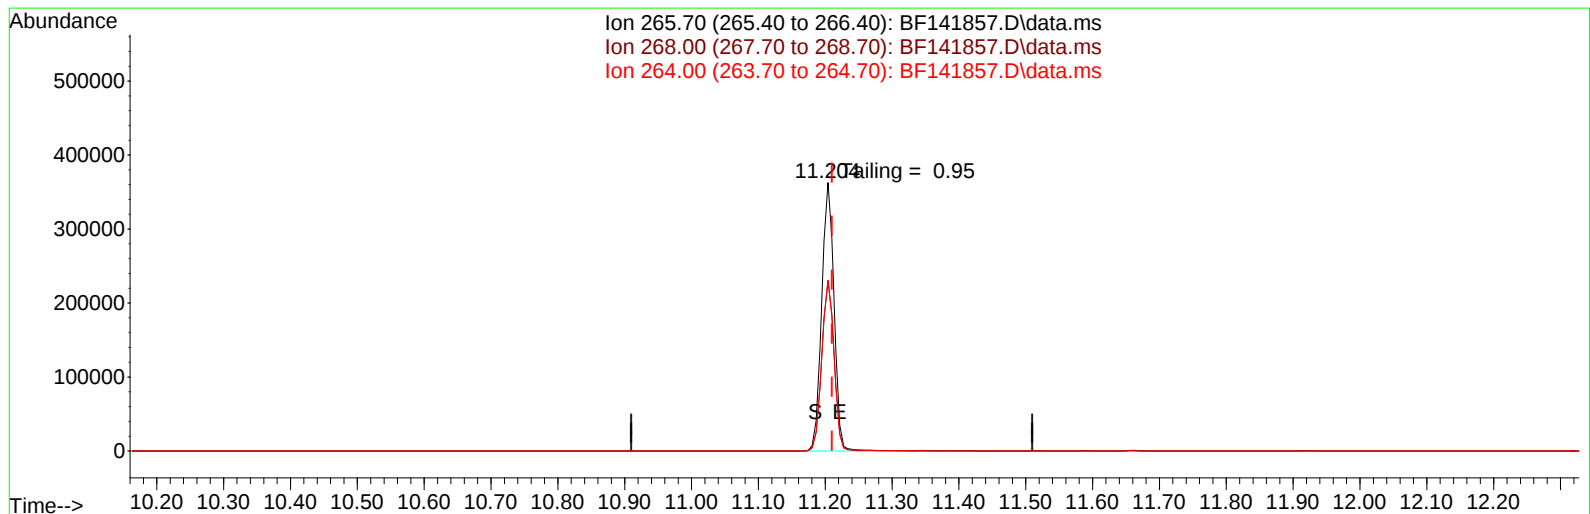

TIC: BF141857.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 17552.30 ng




response 465884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.51
264.00	62.80	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030625\
Data File : BF141857.D
Acq On : 06 Mar 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 06 17:12:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

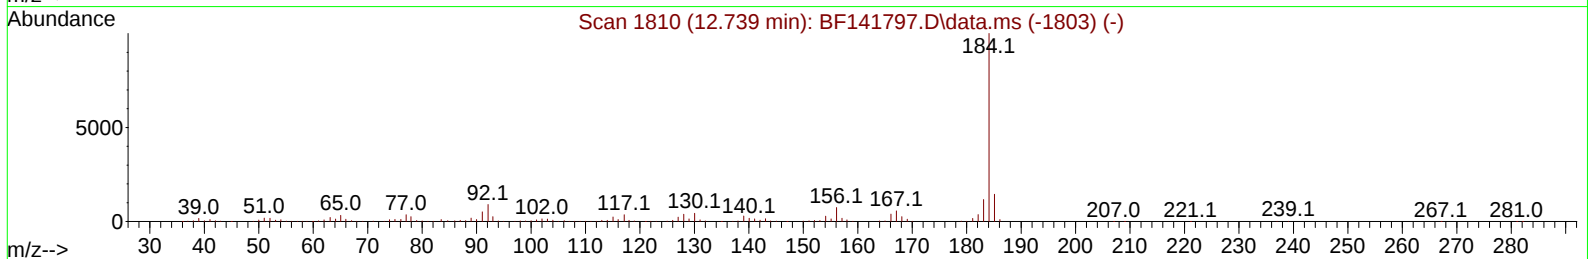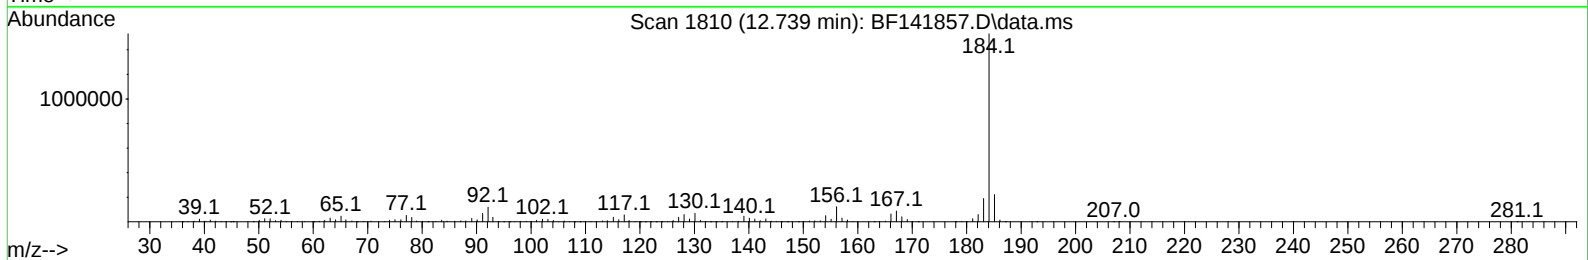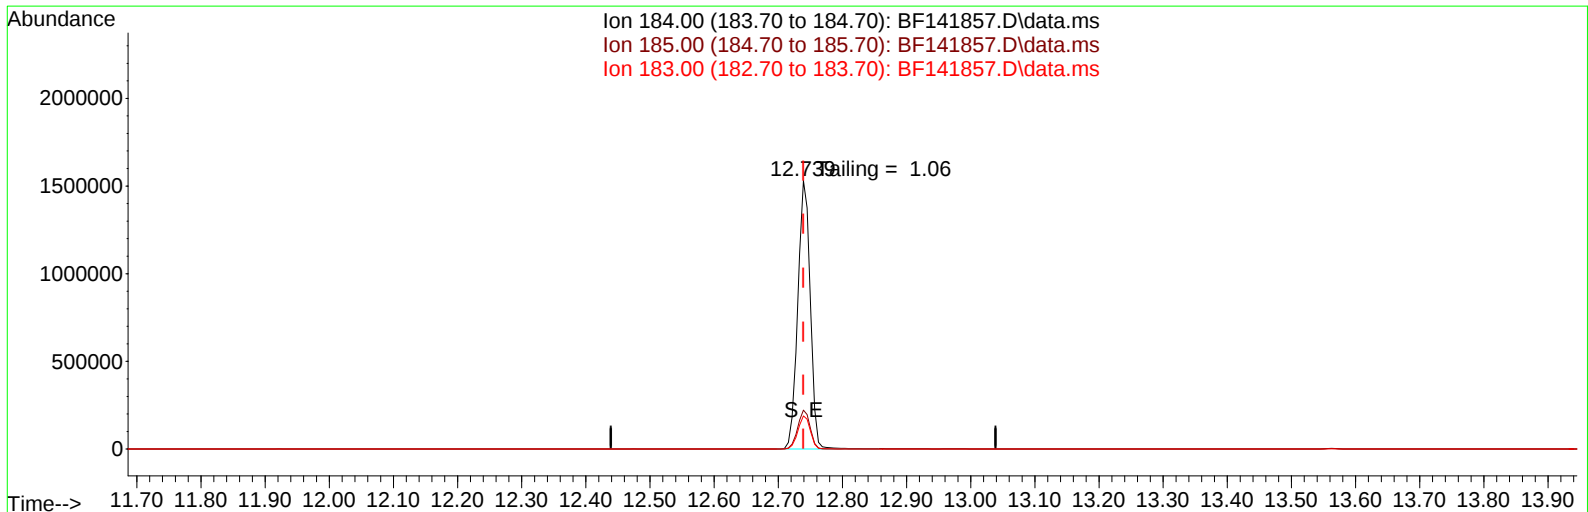

TIC: BF141857.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 49273.09 ng

response 2084395

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.51
183.00	11.70	12.37
0.00	0.00	0.00