

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030525\
 Data File : PL094518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2025 19:22
 Operator : AR\AJ
 Sample : Q1486-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DN-B-40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 01:00:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.770	39889005	51010709	15.710m	15.985
28) SA Decachlor...	9.053	7.907	36434002	53711359	17.127m	13.967
Target Compounds						
10) B gamma-Chl...	5.936	4.973	2216570	1454563	0.755m	0.335m#
11) B alpha-Chl...	6.019	5.035	3554598	2406724	1.227m	0.557m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030525\
Data File : PL094518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2025 19:22
Operator : AR\AJ
Sample : Q1486-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DN-B-40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 01:00:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

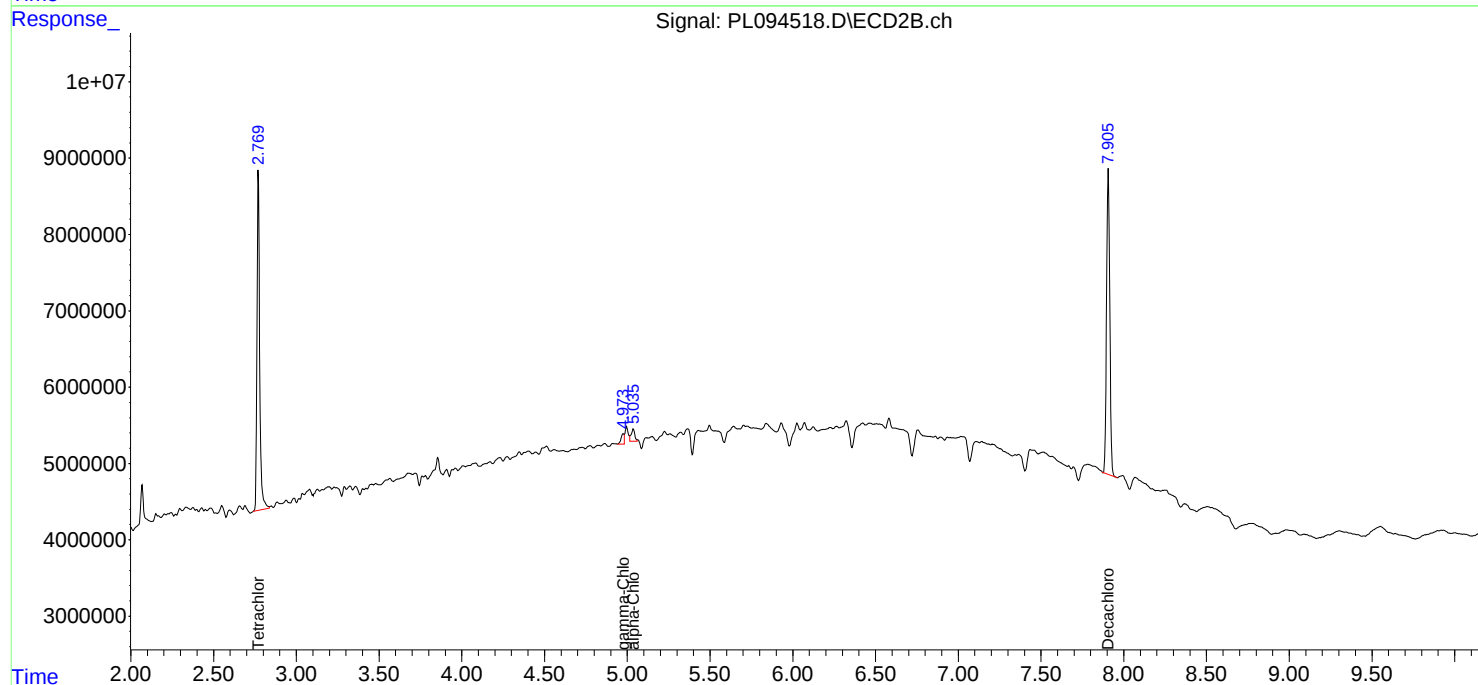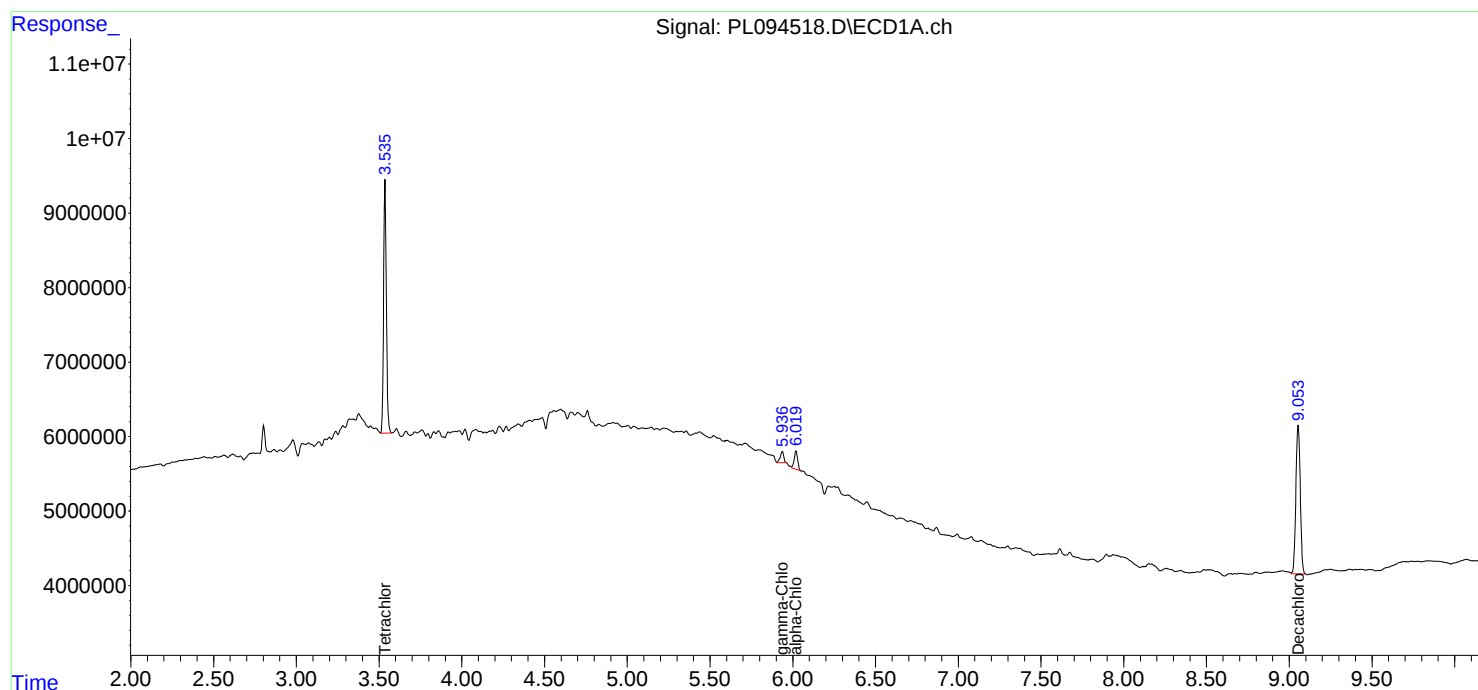


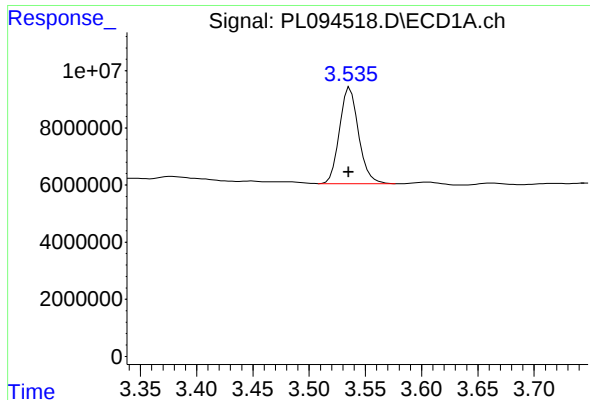

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 39889005
Conc: 15.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
DN-B-40

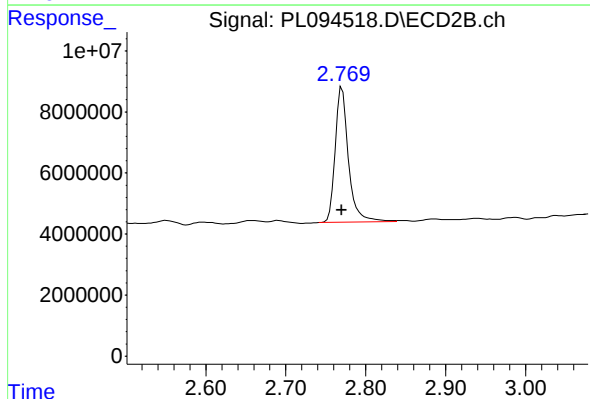


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 51010709
Conc: 15.98 ng/ml

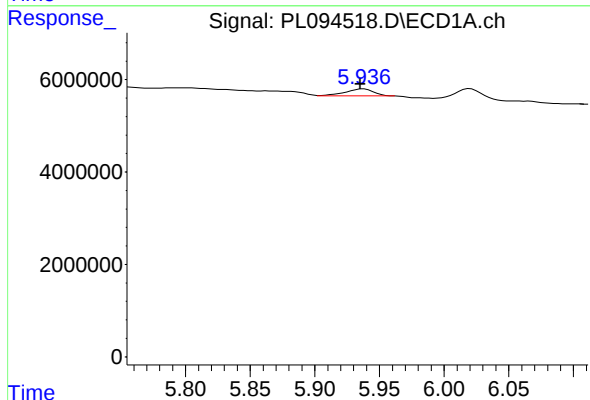


#10 gamma-Chlordane

R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 2216570
Conc: 0.75 ng/ml m

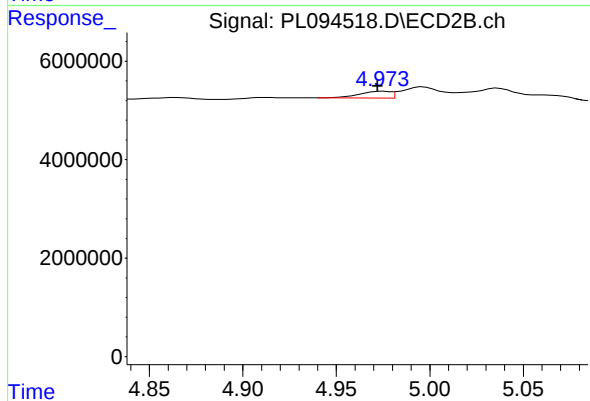

#10 gamma-Chlordane


R.T.: 4.973 min
Delta R.T.: 0.001 min
Response: 1454563
Conc: 0.34 ng/ml m

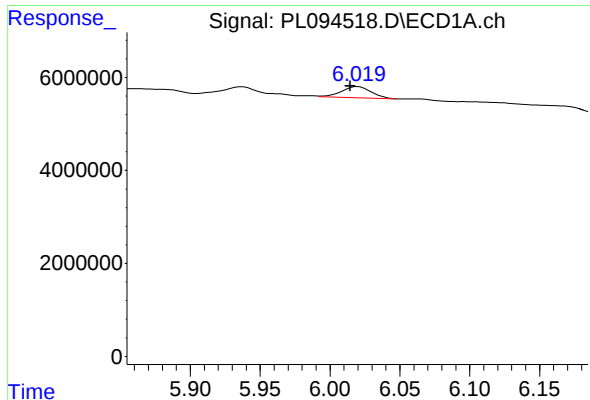

#11 alpha-Chlordane


R.T.: 6.019 min
Delta R.T.: 0.004 min
Response: 3554598
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
DN-B-40

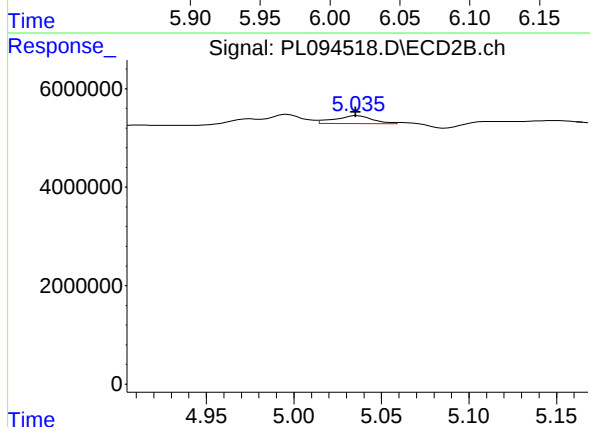


#11 alpha-Chlordane

R.T.: 5.035 min
Delta R.T.: 0.000 min
Response: 2406724
Conc: 0.56 ng/ml m

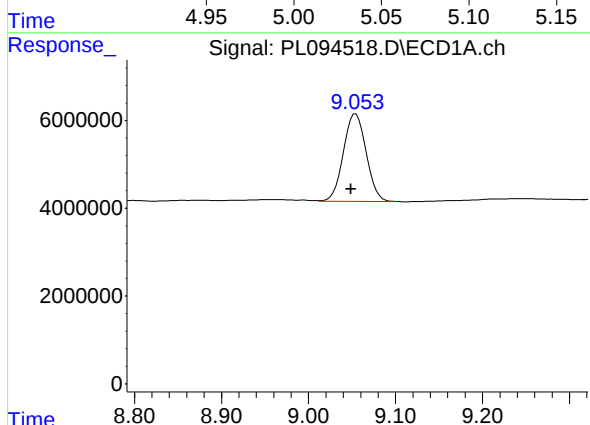

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.004 min
Response: 36434002
Conc: 17.13 ng/ml m

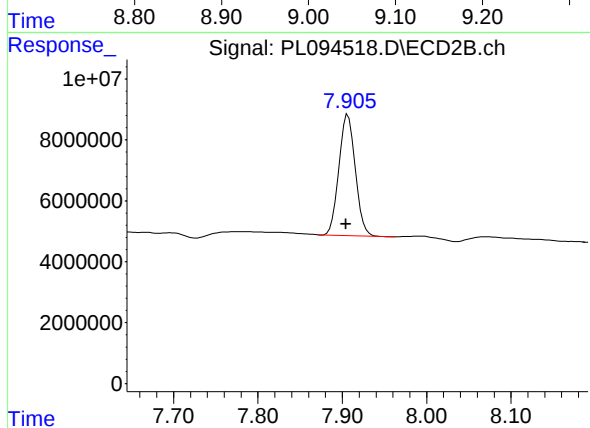

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.002 min
Response: 53711359
Conc: 13.97 ng/ml