
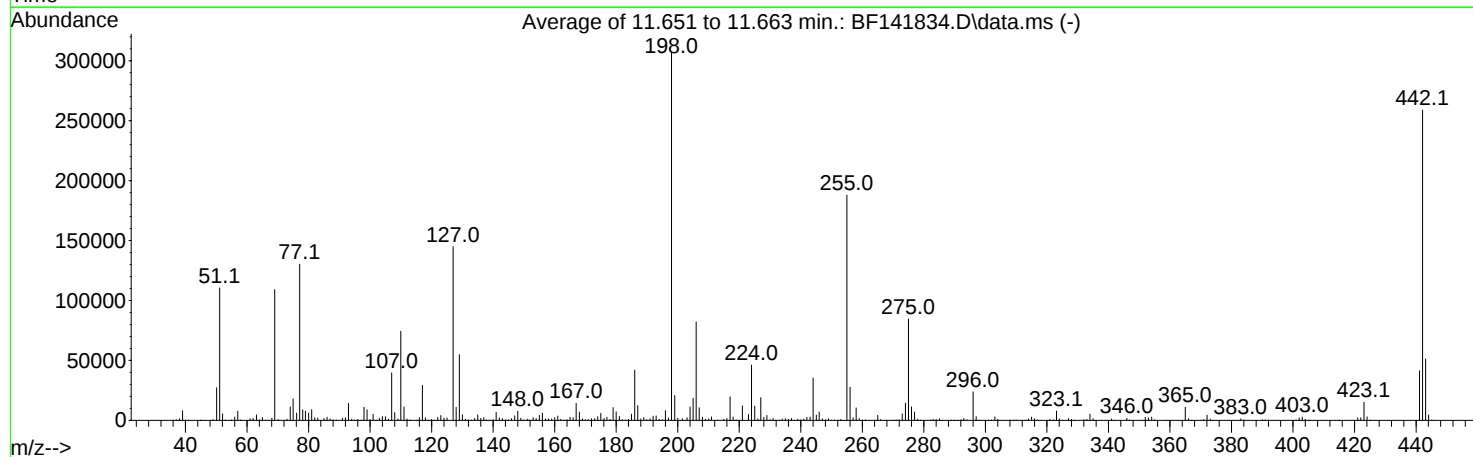


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030525\
Data File : BF141834.D
Acq On : 05 Mar 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 28 01:48:16 2025

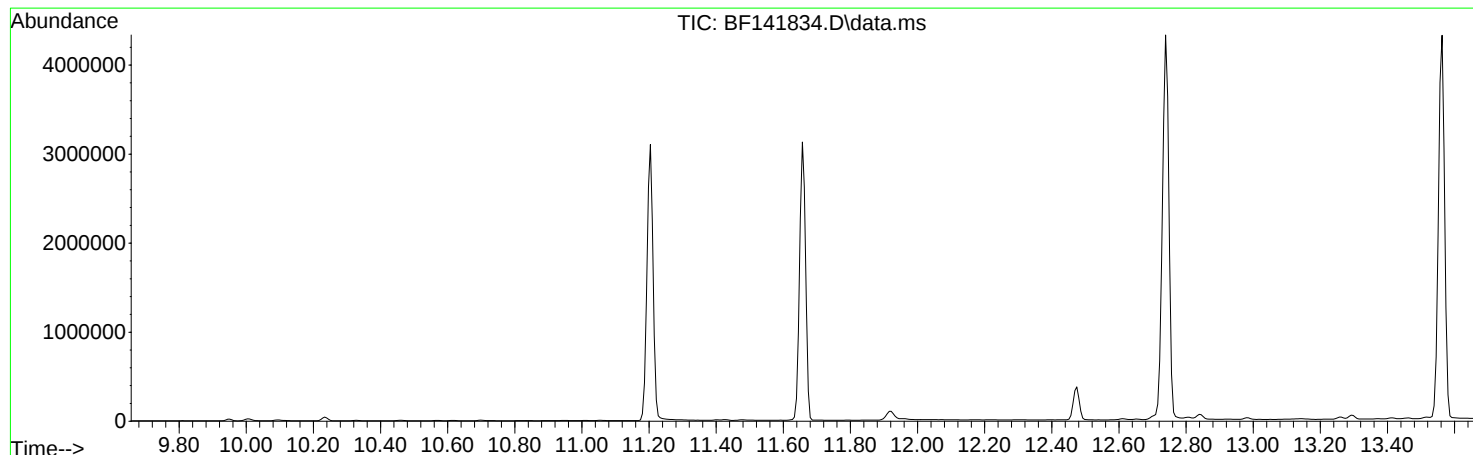

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	110581	PASS
68	69	0.00	2	1.8	1934	PASS
69	198	0.00	100	35.5	109001	PASS
70	69	0.00	2	0.6	688	PASS
127	198	10	80	47.3	145005	PASS
197	198	0.00	2	0.6	1815	PASS
198	198	100	100	100.0	306880	PASS
199	198	5	9	6.8	20715	PASS
275	198	10	60	27.6	84643	PASS
365	198	1	100	3.6	10929	PASS
441	198	0.01	100	13.5	41328	PASS
442	442	50	100	100.0	258816	PASS
443	442	15	24	19.8	51307	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/5/2025	BNA_F	<u>BF141834.D</u>
Compound Name	Response	Retention Time
DDT	1076236	13.563
DDD	16503	13.292
DDE	899	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17402	1093638	1.59

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030525\
Data File : BF141834.D
Acq On : 05 Mar 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 05 11:25:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

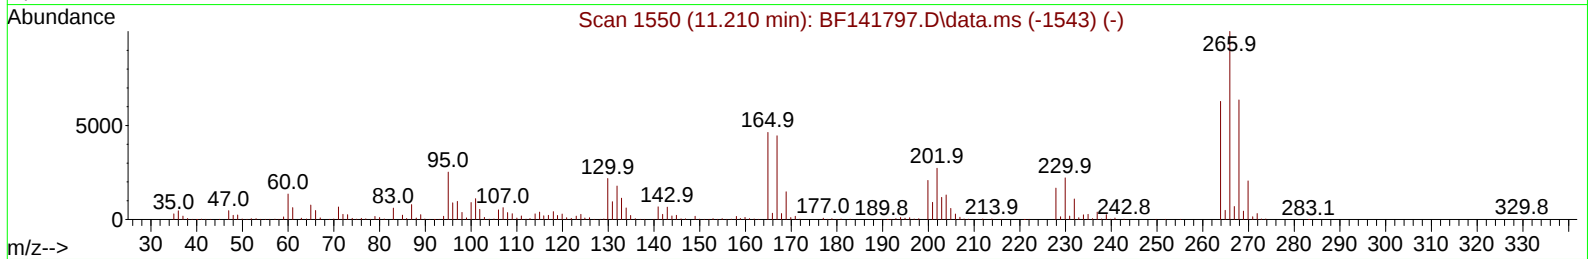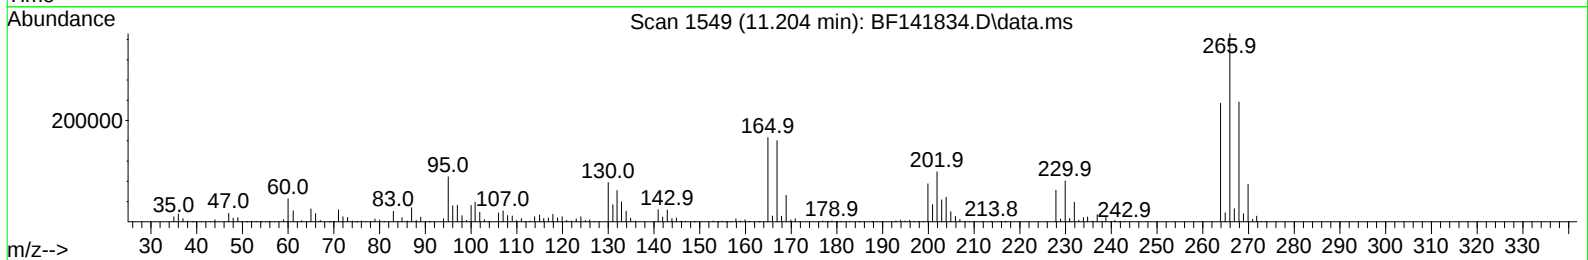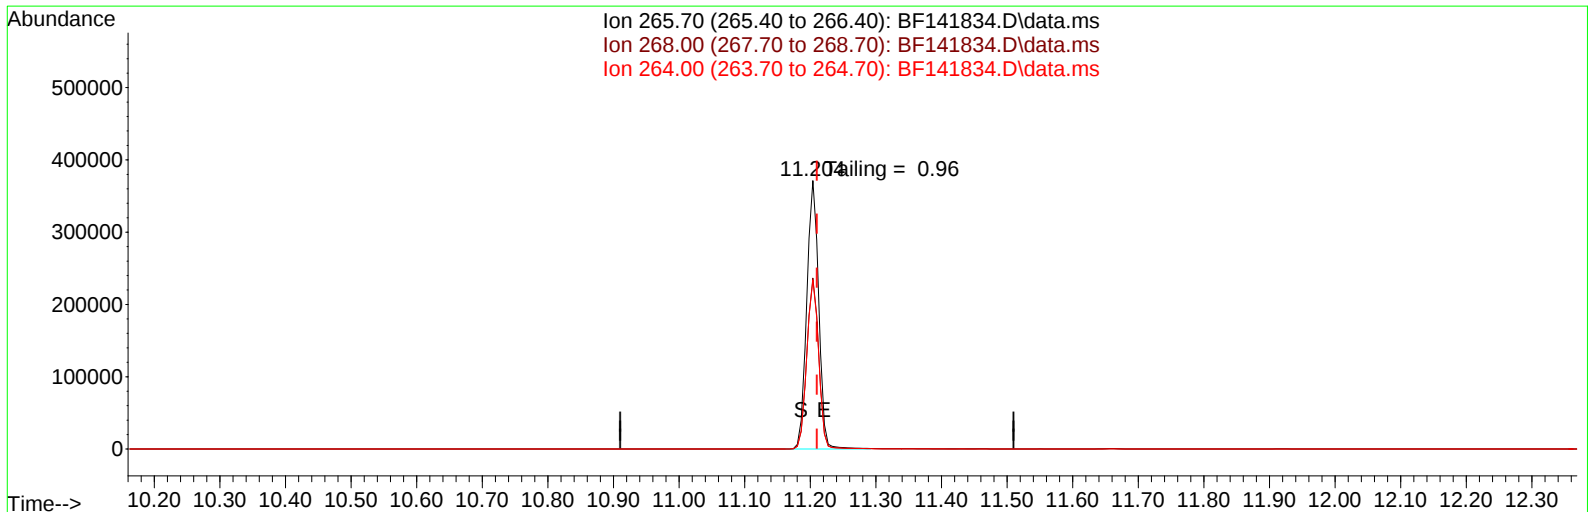

TIC: BF141834.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 20262.40 ng




response 472195

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.68
264.00	62.80	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030525\
Data File : BF141834.D
Acq On : 05 Mar 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 05 11:25:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

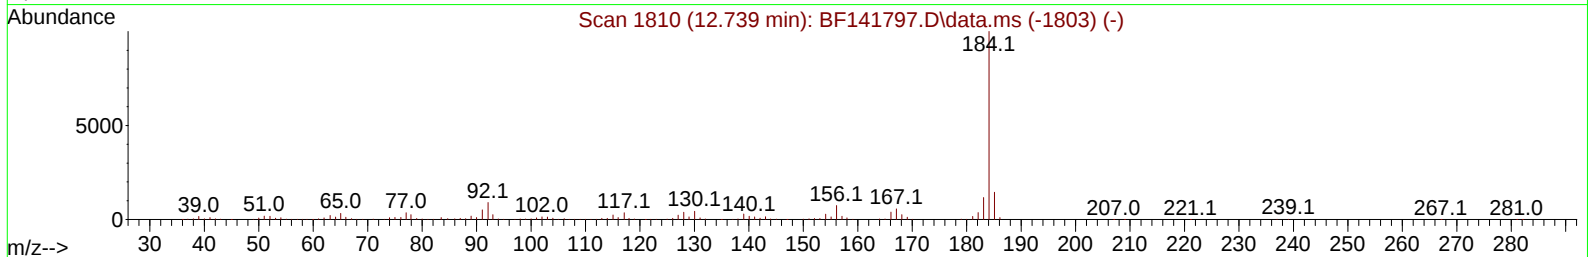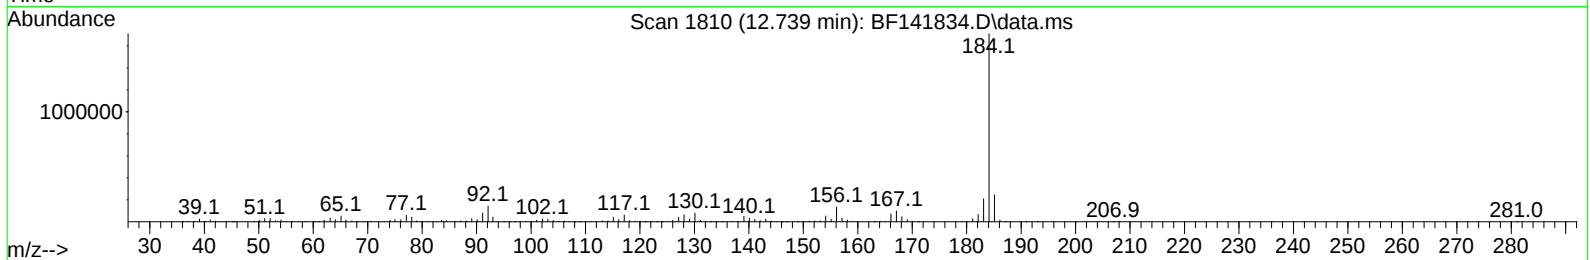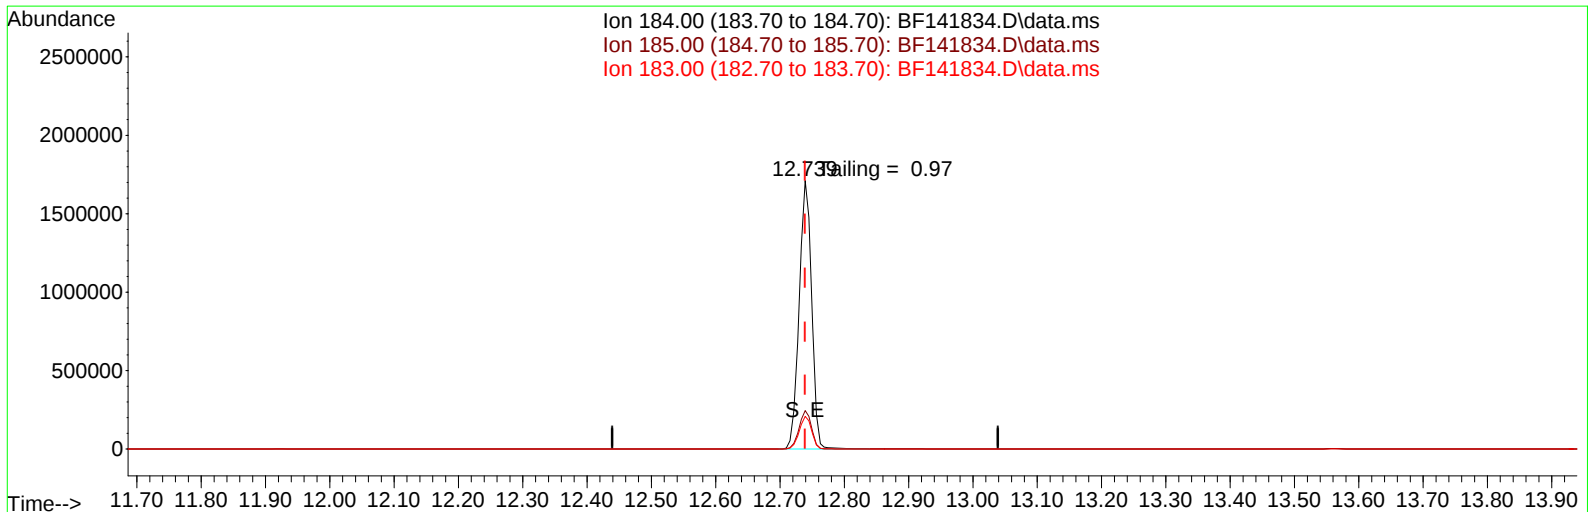

TIC: BF141834.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 56821.39 ng

response 2322895

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.34
183.00	11.70	12.16
0.00	0.00	0.00